

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
 Data File : FF003802.D
 Signal(s) : FID2B.ch
 Acq On : 12 Mar 2019 17:39
 Operator : AJ\SJ
 Sample : K1846-10
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 01:00:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.593	1688303	12.126 ug/ml
Target Compounds			
4) N-TETRADECANE	8.192f	496154	3.094 ug/ml
12) N-OCTACOSANE	16.773	200349	1.326 ug/ml
13) N-TRIACONTANE	17.663	236190	1.606 ug/ml
14) N-DOTRIACONTANE	18.504	382676	2.691 ug/ml
15) N-TETRATRIACONTANE	19.288	79468	0.594 ug/ml
16) N-HEXATRIACONTANE	20.031	87841	0.673 ug/ml
18) N-TETRACONTANE	21.680	655405	5.268 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003802.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 17:39
Operator : AJ\SJ
Sample : K1846-10
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Mar 13 01:00:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

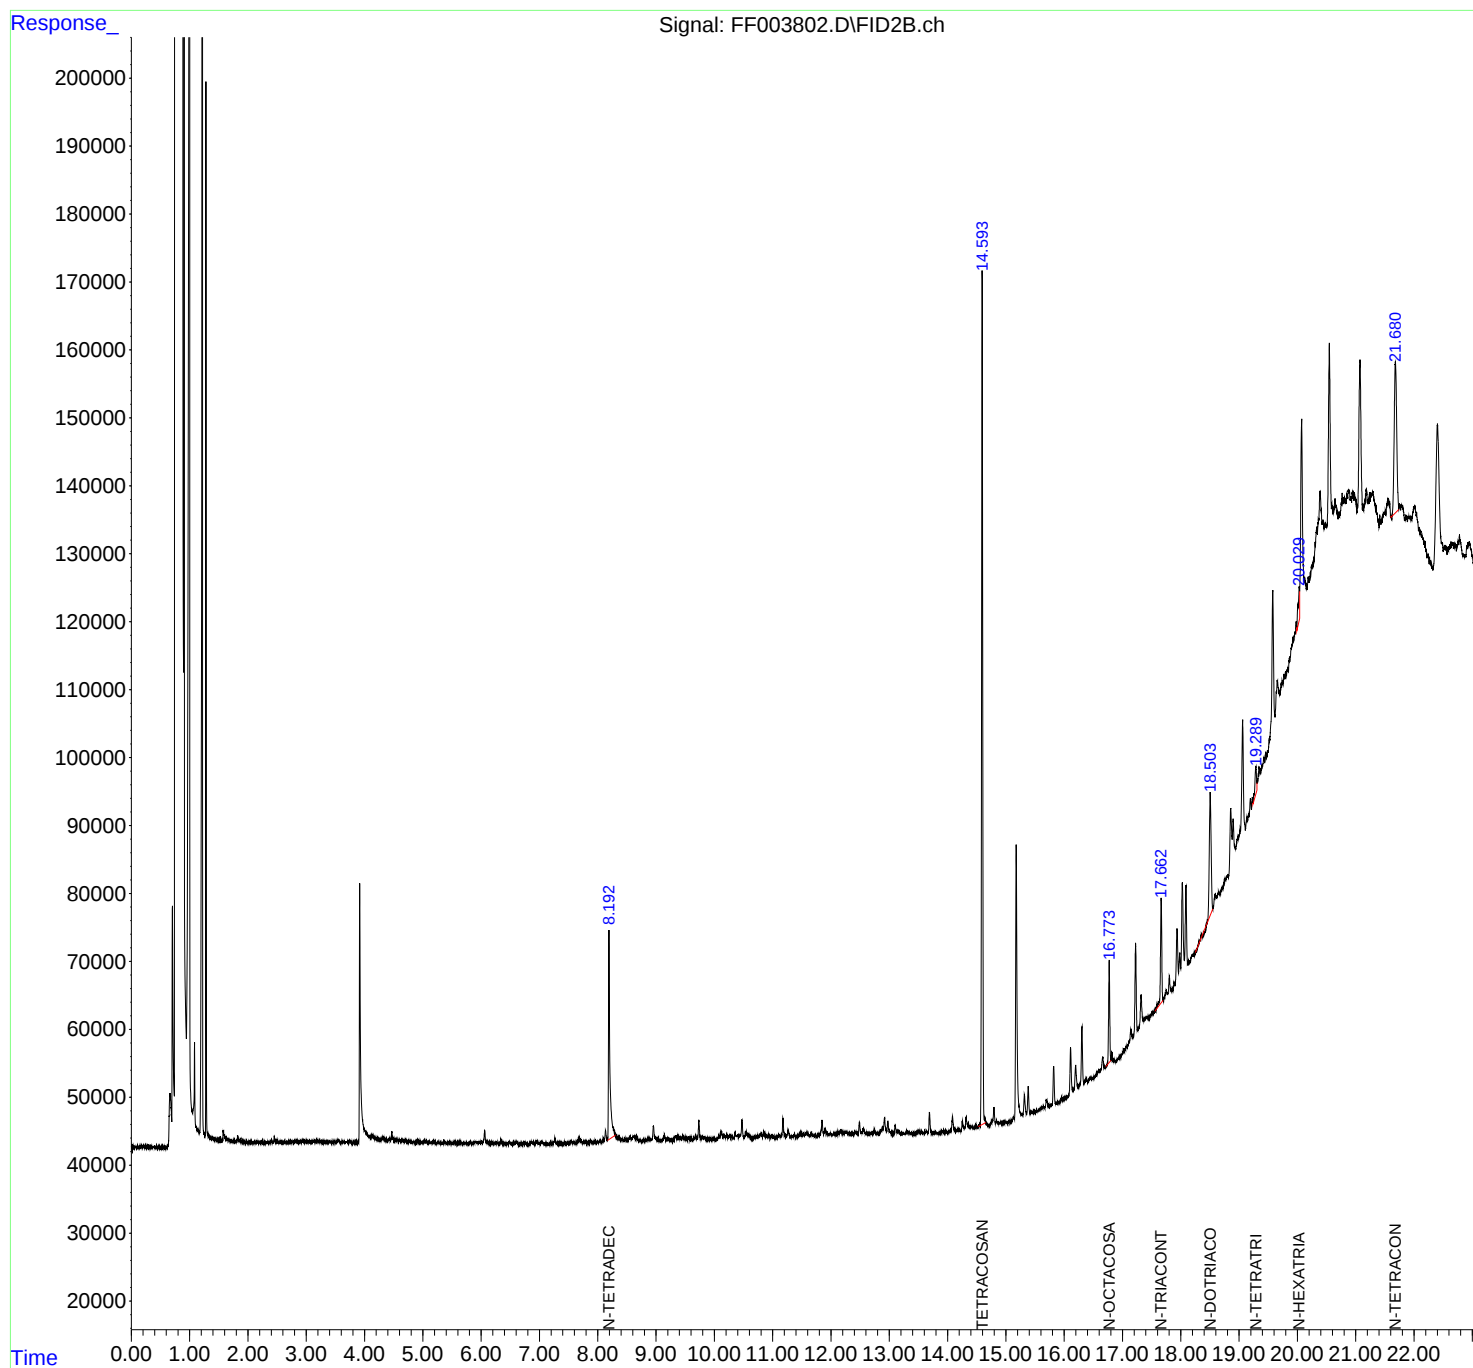


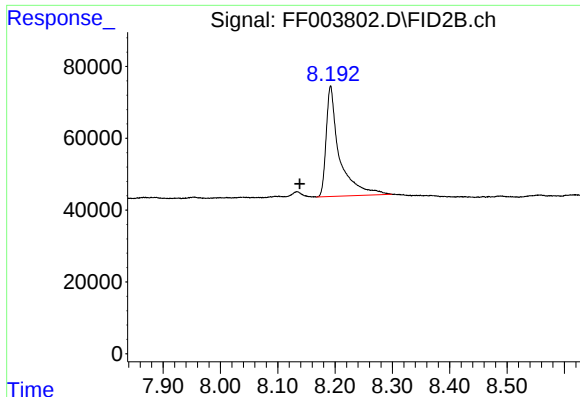

#4 N-TETRADECANE


R.T.: 8.192 min
Delta R.T.: 0.054 min
Response: 496154
Conc: 3.09 ug/ml

Instrument :
FID_F
ClientSampleId :

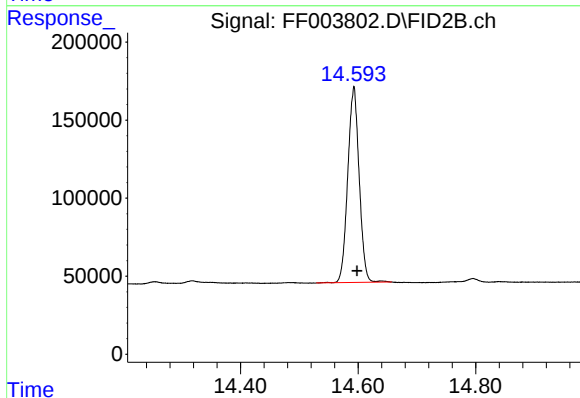


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.593 min
Delta R.T.: -0.005 min
Response: 1688303
Conc: 12.13 ug/ml

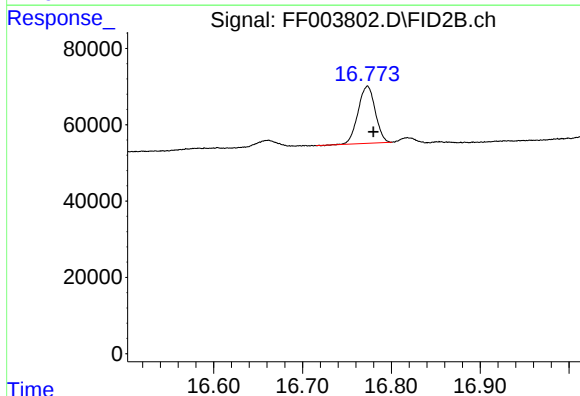


#12 N-OCTACOSANE

R.T.: 16.773 min
Delta R.T.: -0.006 min
Response: 200349
Conc: 1.33 ug/ml

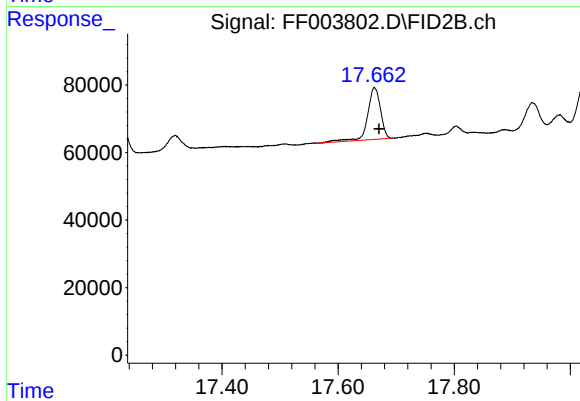

#13 N-TRIACONTANE


R.T.: 17.663 min
Delta R.T.: -0.008 min
Response: 236190
Conc: 1.61 ug/ml

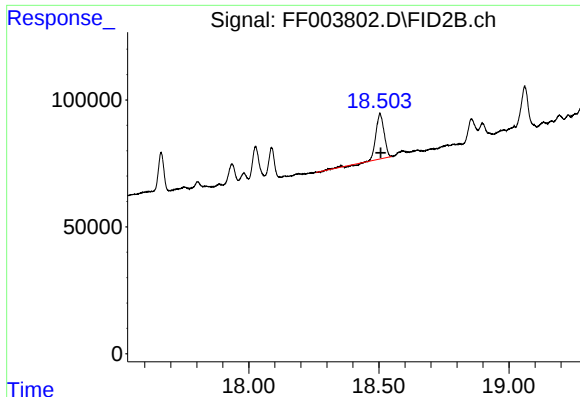

#14 N-DOTRIACONTANE


R.T.: 18.504 min
Delta R.T.: -0.003 min
Response: 382676
Conc: 2.69 ug/ml

Instrument :
FID_F
ClientSampleId :

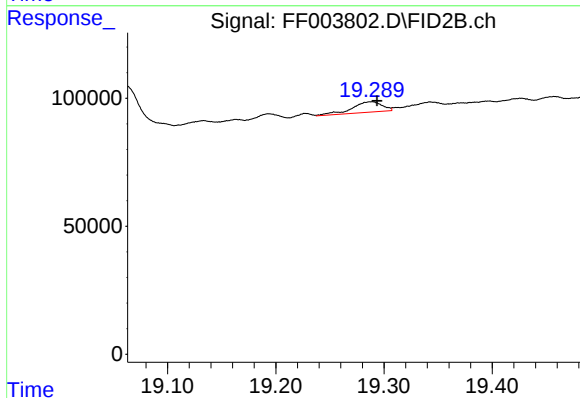


#15 N-TETRATRIACONTANE

R.T.: 19.288 min
Delta R.T.: -0.005 min
Response: 79468
Conc: 0.59 ug/ml

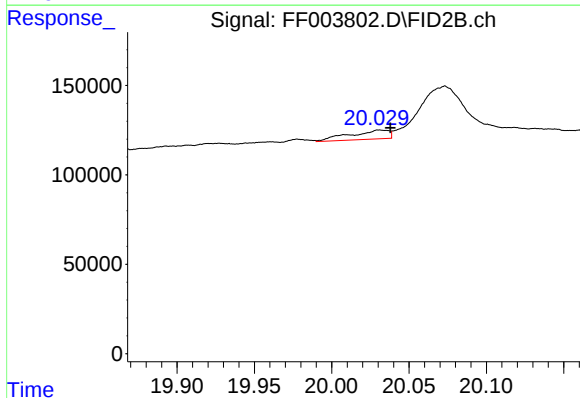

#16 N-HEXATRIACONTANE

R.T.: 20.031 min
Delta R.T.: -0.007 min
Response: 87841
Conc: 0.67 ug/ml

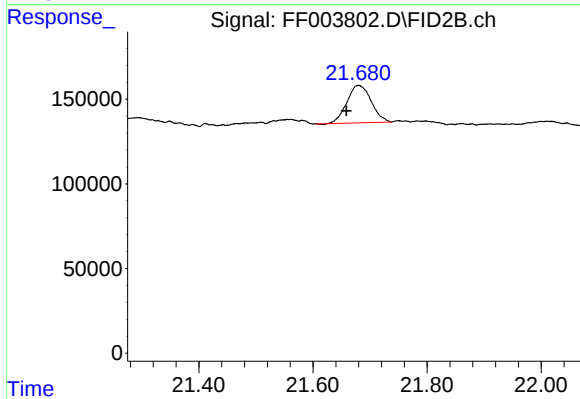

#18 N-TETRACONTANE

R.T.: 21.680 min
Delta R.T.: 0.021 min
Response: 655405
Conc: 5.27 ug/ml