

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
 Data File : FF003805.D
 Signal(s) : FID2B.ch
 Acq On : 12 Mar 2019 19:10
 Operator : AJ\SJ
 Sample : K1846-01 5X
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 01:01:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.592	417958	3.002 ug/ml
Target Compounds			
7) N-EICOSANE	12.542	715461	4.373 ug/ml
10) N-TETRACOSANE	14.769	435481	2.752 ug/ml
12) N-OCTACOSANE	16.779	210200	1.391 ug/ml
13) N-TRIACONTANE	17.661	313433	2.131 ug/ml
14) N-DOTRIACONTANE	18.499	259700	1.826 ug/ml
15) N-TETRATRIACONTANE	19.305	181368	1.355 ug/ml
16) N-HEXATRIACONTANE	20.039	207788	1.592 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003805.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 19:10
Operator : AJ\SJ
Sample : K1846-01 5X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 01:01:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

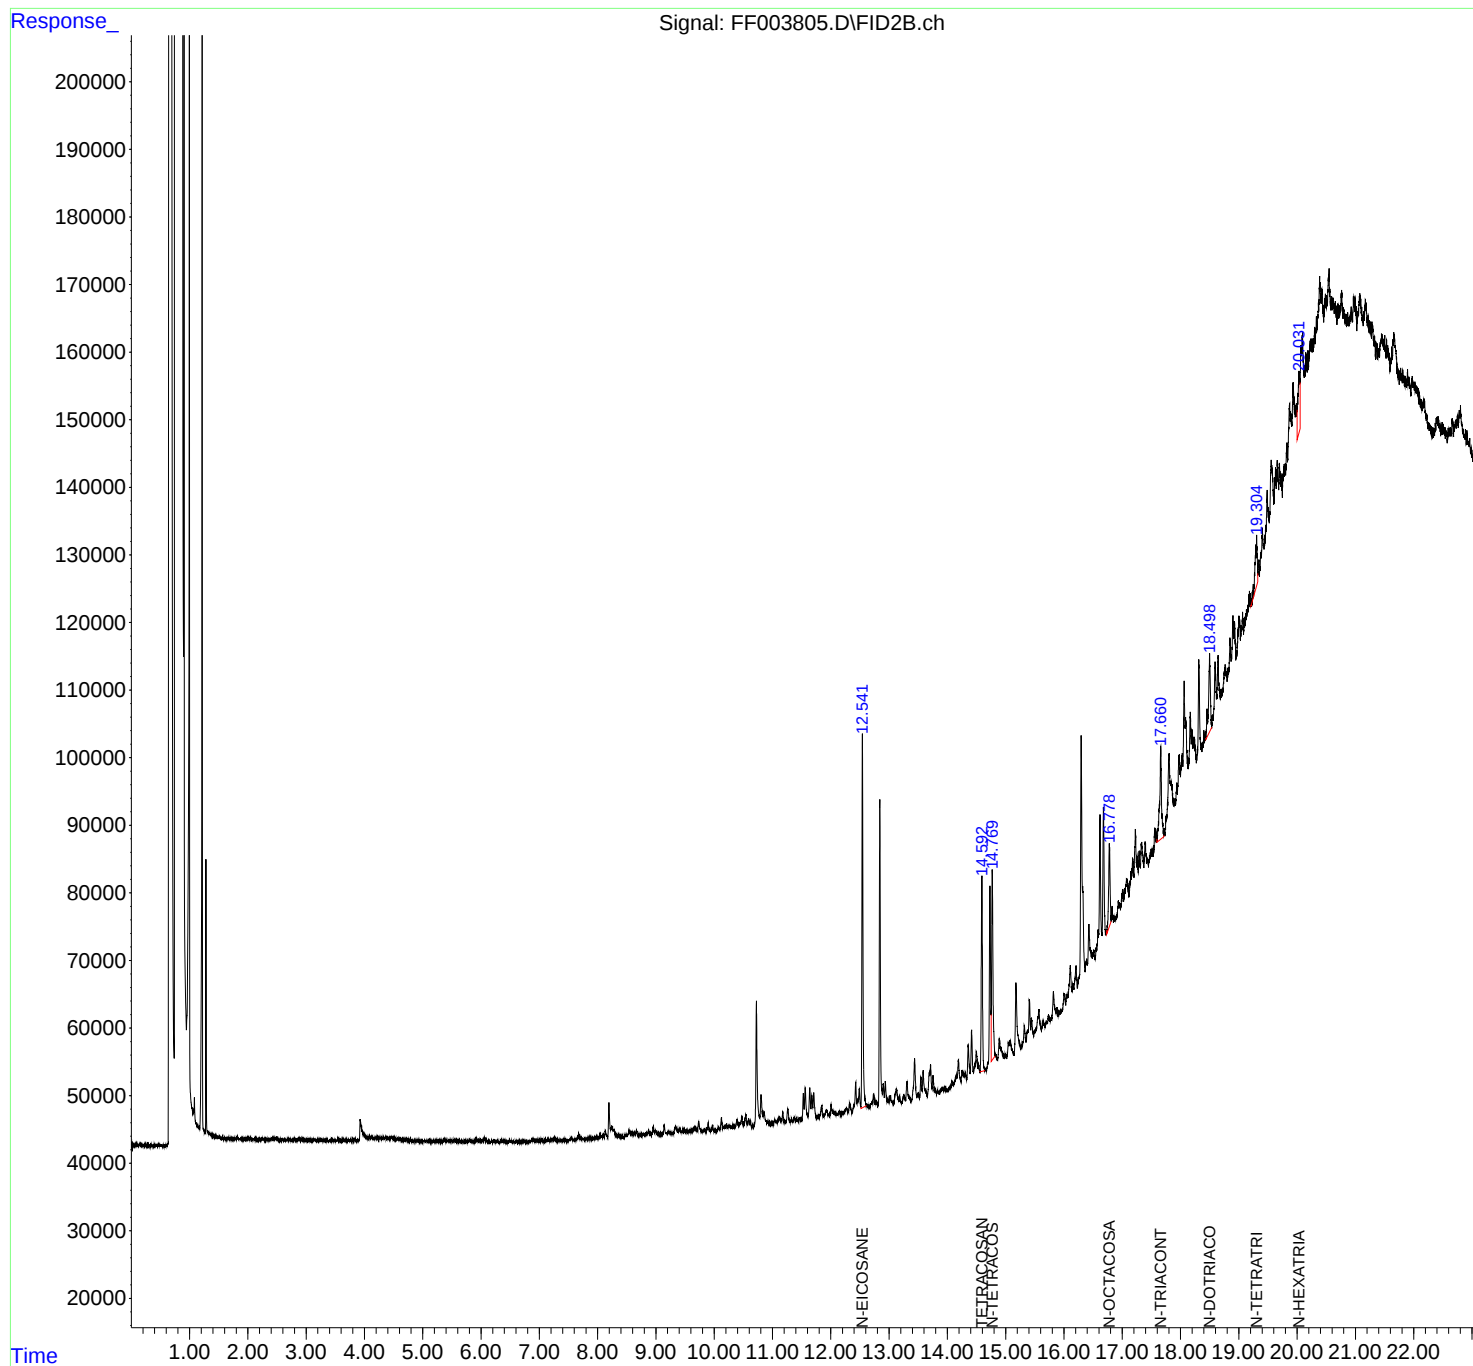


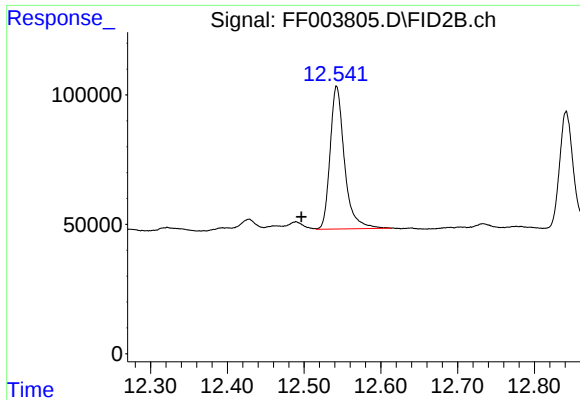

#7 N-EICOSANE


R.T.: 12.542 min
Delta R.T.: 0.046 min
Response: 715461
Conc: 4.37 ug/ml

Instrument :
FID_F
ClientSampleId :

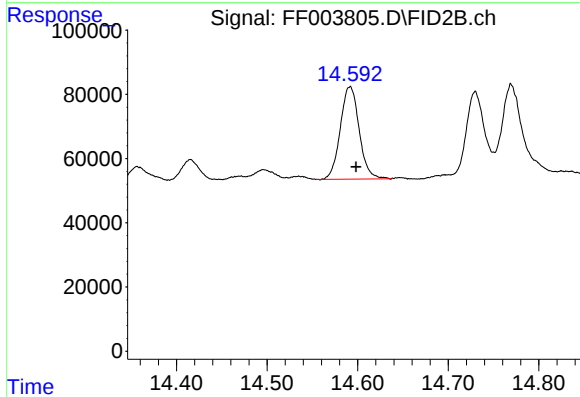


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.592 min
Delta R.T.: -0.007 min
Response: 417958
Conc: 3.00 ug/ml

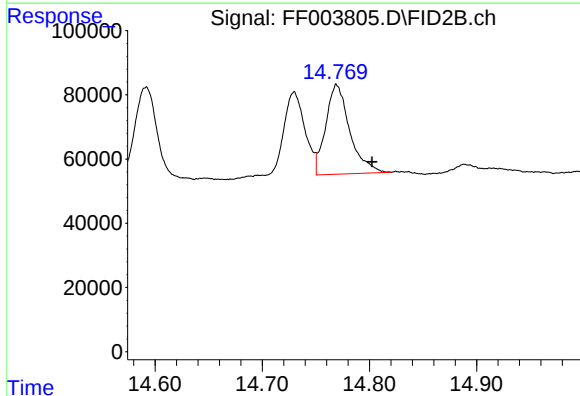


#10 N-TETRACOSANE

R.T.: 14.769 min
Delta R.T.: -0.033 min
Response: 435481
Conc: 2.75 ug/ml

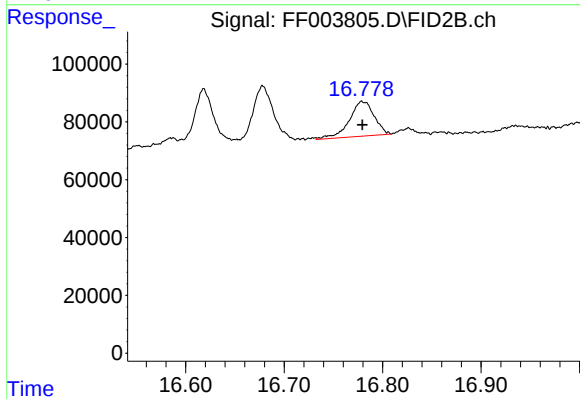

#12 N-OCTACOSANE


R.T.: 16.779 min
Delta R.T.: 0.000 min
Response: 210200
Conc: 1.39 ug/ml

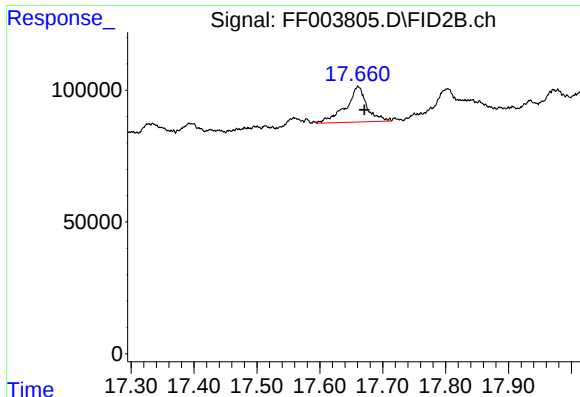

#13 N-TRIACONTANE


R.T.: 17.661 min
Delta R.T.: -0.010 min
Response: 313433
Conc: 2.13 ug/ml

Instrument :
FID_F
ClientSampleId :

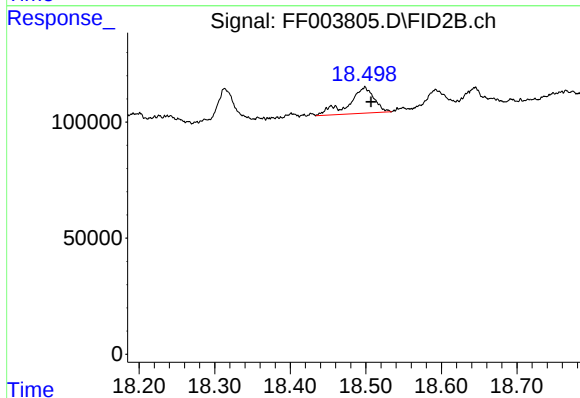


#14 N-DOTRIACONTANE

R.T.: 18.499 min
Delta R.T.: -0.008 min
Response: 259700
Conc: 1.83 ug/ml

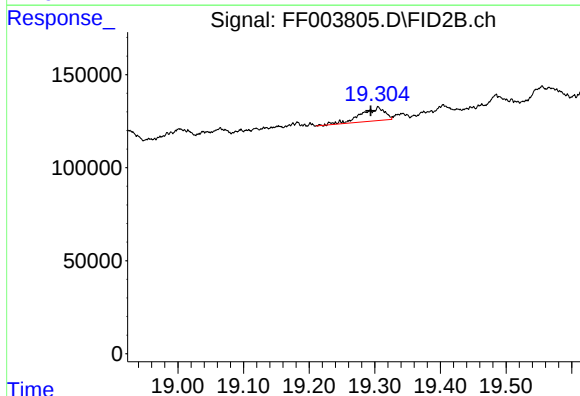

#15 N-TETRATRIACONTANE

R.T.: 19.305 min
Delta R.T.: 0.012 min
Response: 181368
Conc: 1.35 ug/ml

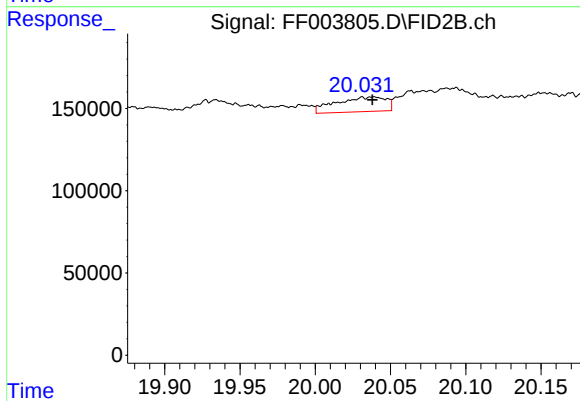

#16 N-HEXATRIACONTANE

R.T.: 20.039 min
Delta R.T.: 0.000 min
Response: 207788
Conc: 1.59 ug/ml