

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
 Data File : FF003806.D
 Signal(s) : FID2B.ch
 Acq On : 12 Mar 2019 19:40
 Operator : AJ\SJ
 Sample : K1846-02 5X
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 01:02:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.591	413243	2.968 ug/ml
Target Compounds			
7) N-EICOSANE	12.544	343002	2.097 ug/ml
10) N-TETRACOSANE	14.772	183375	1.159 ug/ml
12) N-OCTACOSANE	16.776	139493	0.923 ug/ml
13) N-TRIACONTANE	17.660	240158	1.633 ug/ml
14) N-DOTRIACONTANE	18.497	219231	1.542 ug/ml
15) N-TETRATRIACONTANE	19.288	102663	0.767 ug/ml
16) N-HEXATRIACONTANE	20.034	68751	0.527 ug/ml
18) N-TETRACONTANE	21.671	196582	1.580 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003806.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 19:40
Operator : AJ\SJ
Sample : K1846-02 5X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 01:02:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

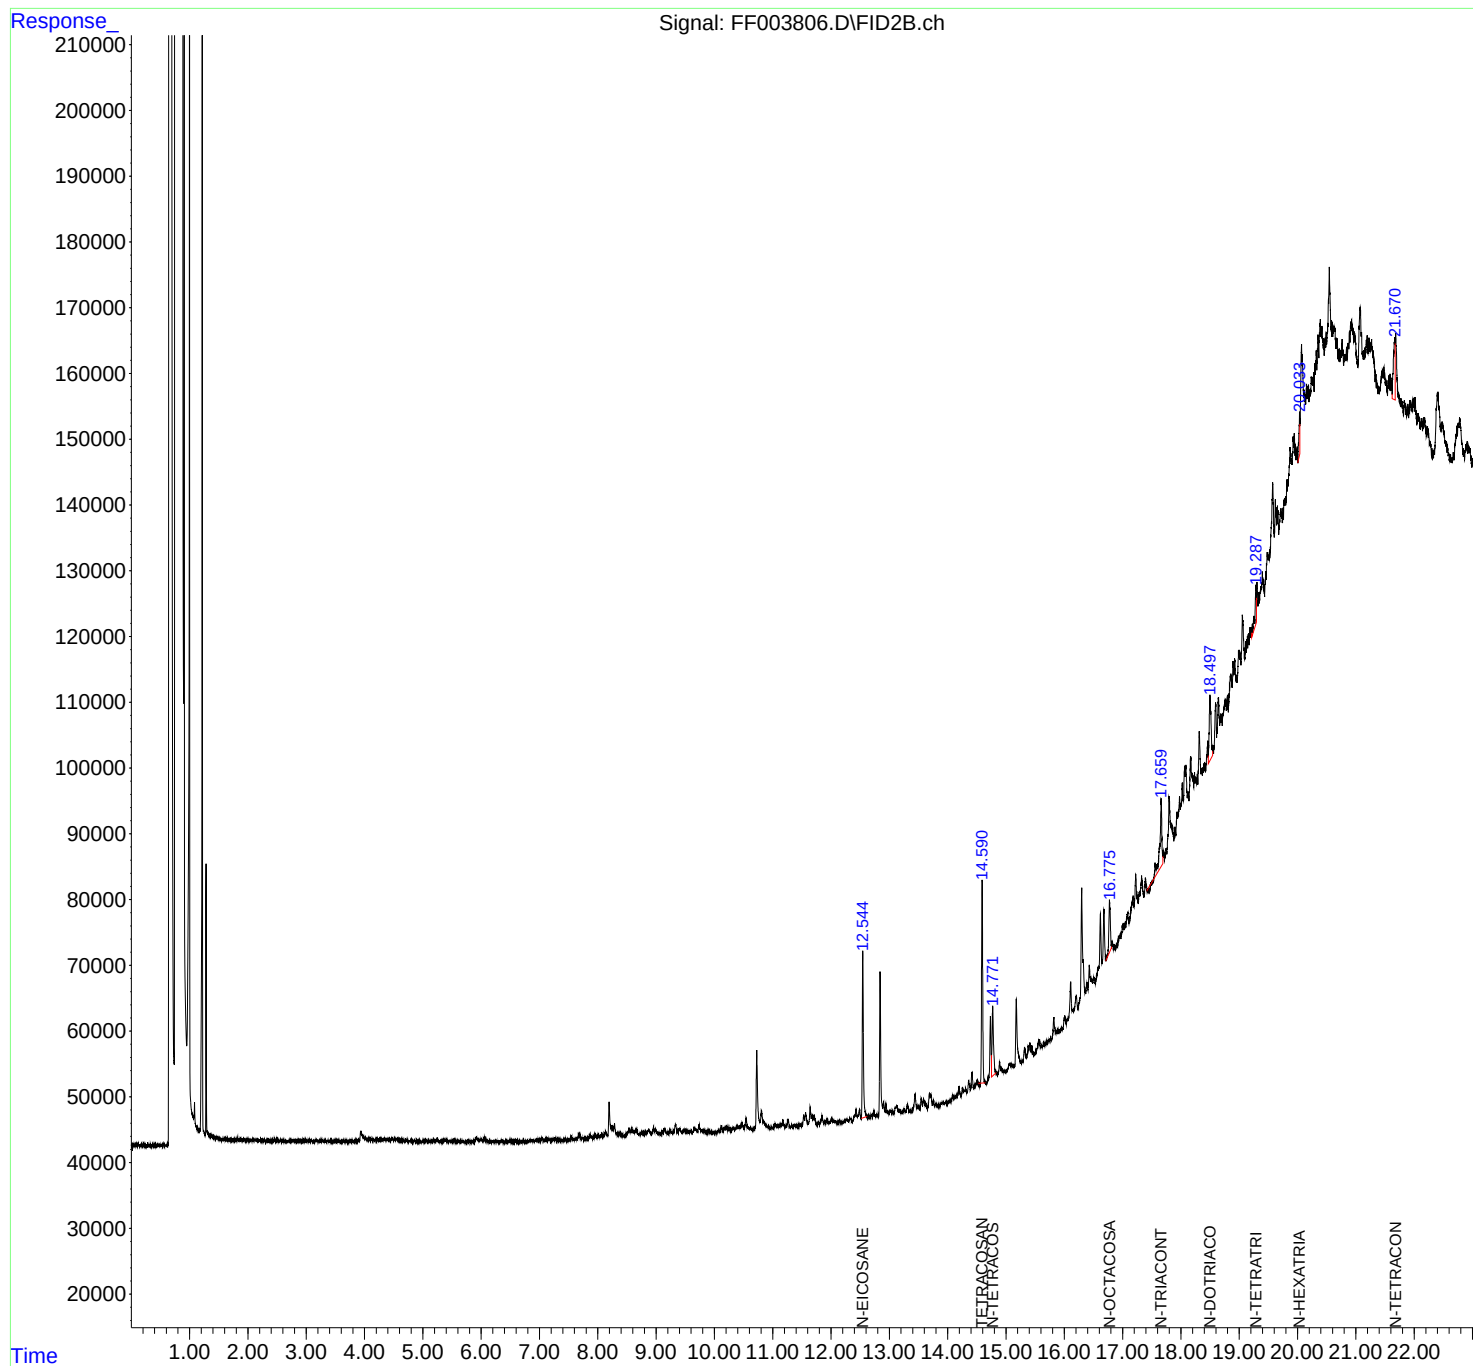


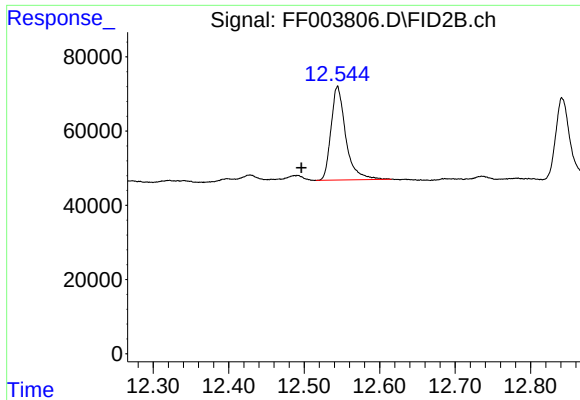

#7 N-EICOSANE


R.T.: 12.544 min
Delta R.T.: 0.048 min
Response: 343002
Conc: 2.10 ug/ml

Instrument :
FID_F
ClientSampleId :

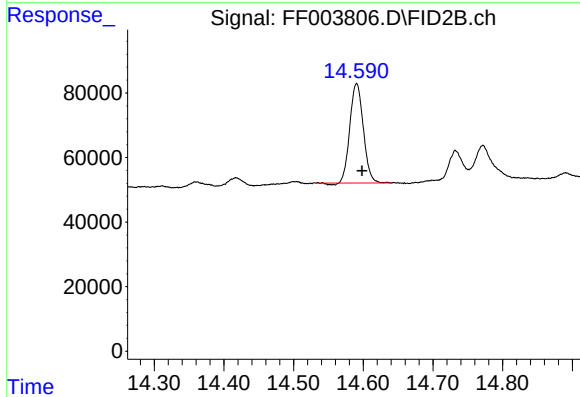


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.591 min
Delta R.T.: -0.008 min
Response: 413243
Conc: 2.97 ug/ml

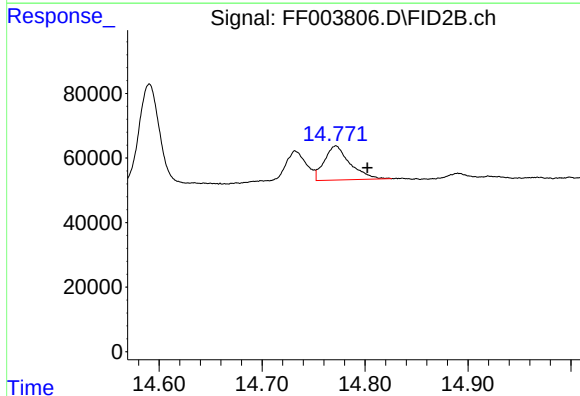


#10 N-TETRACOSANE

R.T.: 14.772 min
Delta R.T.: -0.031 min
Response: 183375
Conc: 1.16 ug/ml

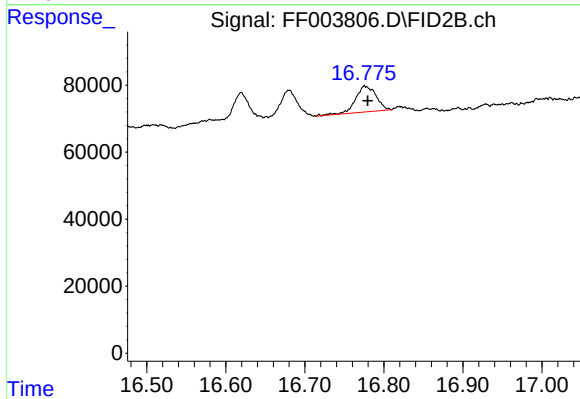

#12 N-OCTACOSANE


R.T.: 16.776 min
Delta R.T.: -0.004 min
Response: 139493
Conc: 0.92 ug/ml

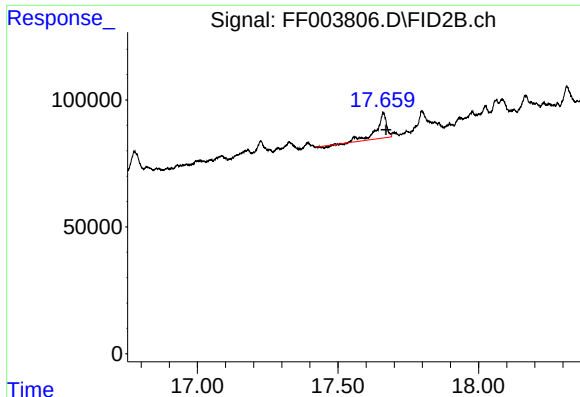

#13 N-TRIACONTANE


R.T.: 17.660 min
Delta R.T.: -0.011 min
Response: 240158
Conc: 1.63 ug/ml

Instrument :
FID_F
ClientSampleId :

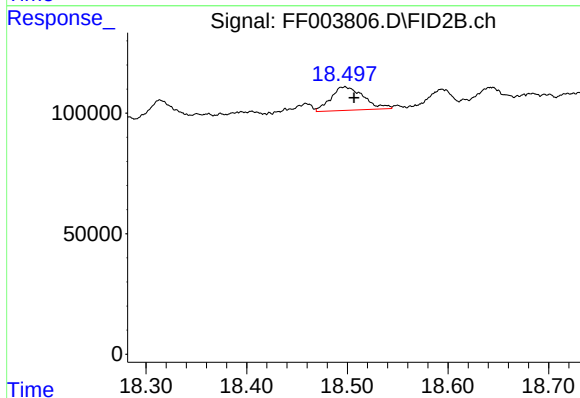


#14 N-DOTRIACONTANE

R.T.: 18.497 min
Delta R.T.: -0.009 min
Response: 219231
Conc: 1.54 ug/ml

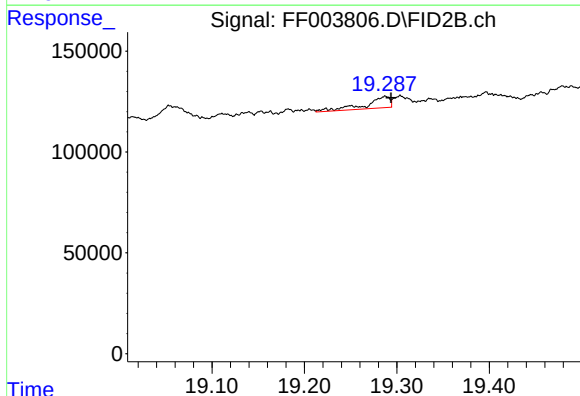


#15 N-TETRATRIACONTANE

R.T.: 19.288 min
Delta R.T.: -0.006 min
Response: 102663
Conc: 0.77 ug/ml

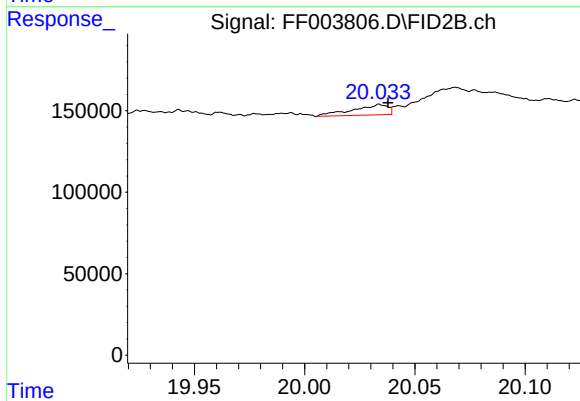

#16 N-HEXATRIACONTANE

R.T.: 20.034 min
Delta R.T.: -0.004 min
Response: 68751
Conc: 0.53 ug/ml

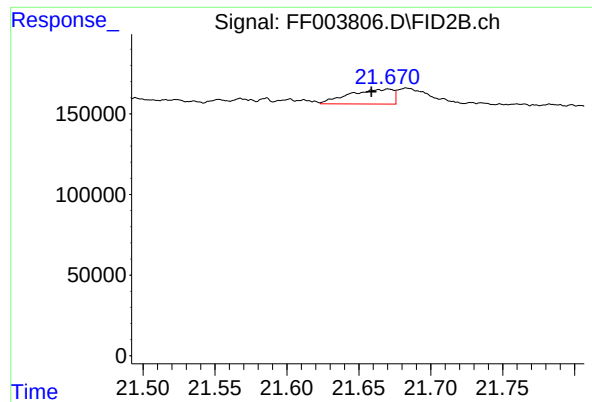

#18 N-TETRACONTANE

R.T.: 21.671 min
Delta R.T.: 0.012 min
Response: 196582
Conc: 1.58 ug/ml

Instrument :
FID_F
ClientSampleId :