

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
 Data File : FF003807.D
 Signal(s) : FID2B.ch
 Acq On : 12 Mar 2019 20:11
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 01:02:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.592	2137509	15.353 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.662	147306	1.001 ug/ml
14) N-DOTRIACONTANE	18.500	294573	2.071 ug/ml
15) N-TETRATRIACONTANE	19.284	176776	1.320 ug/ml
16) N-HEXATRIACONTANE	20.031	67054	0.514 ug/ml
18) N-TETRACONTANE	21.674	404104	3.248 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003807.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 20:11
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Mar 13 01:02:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

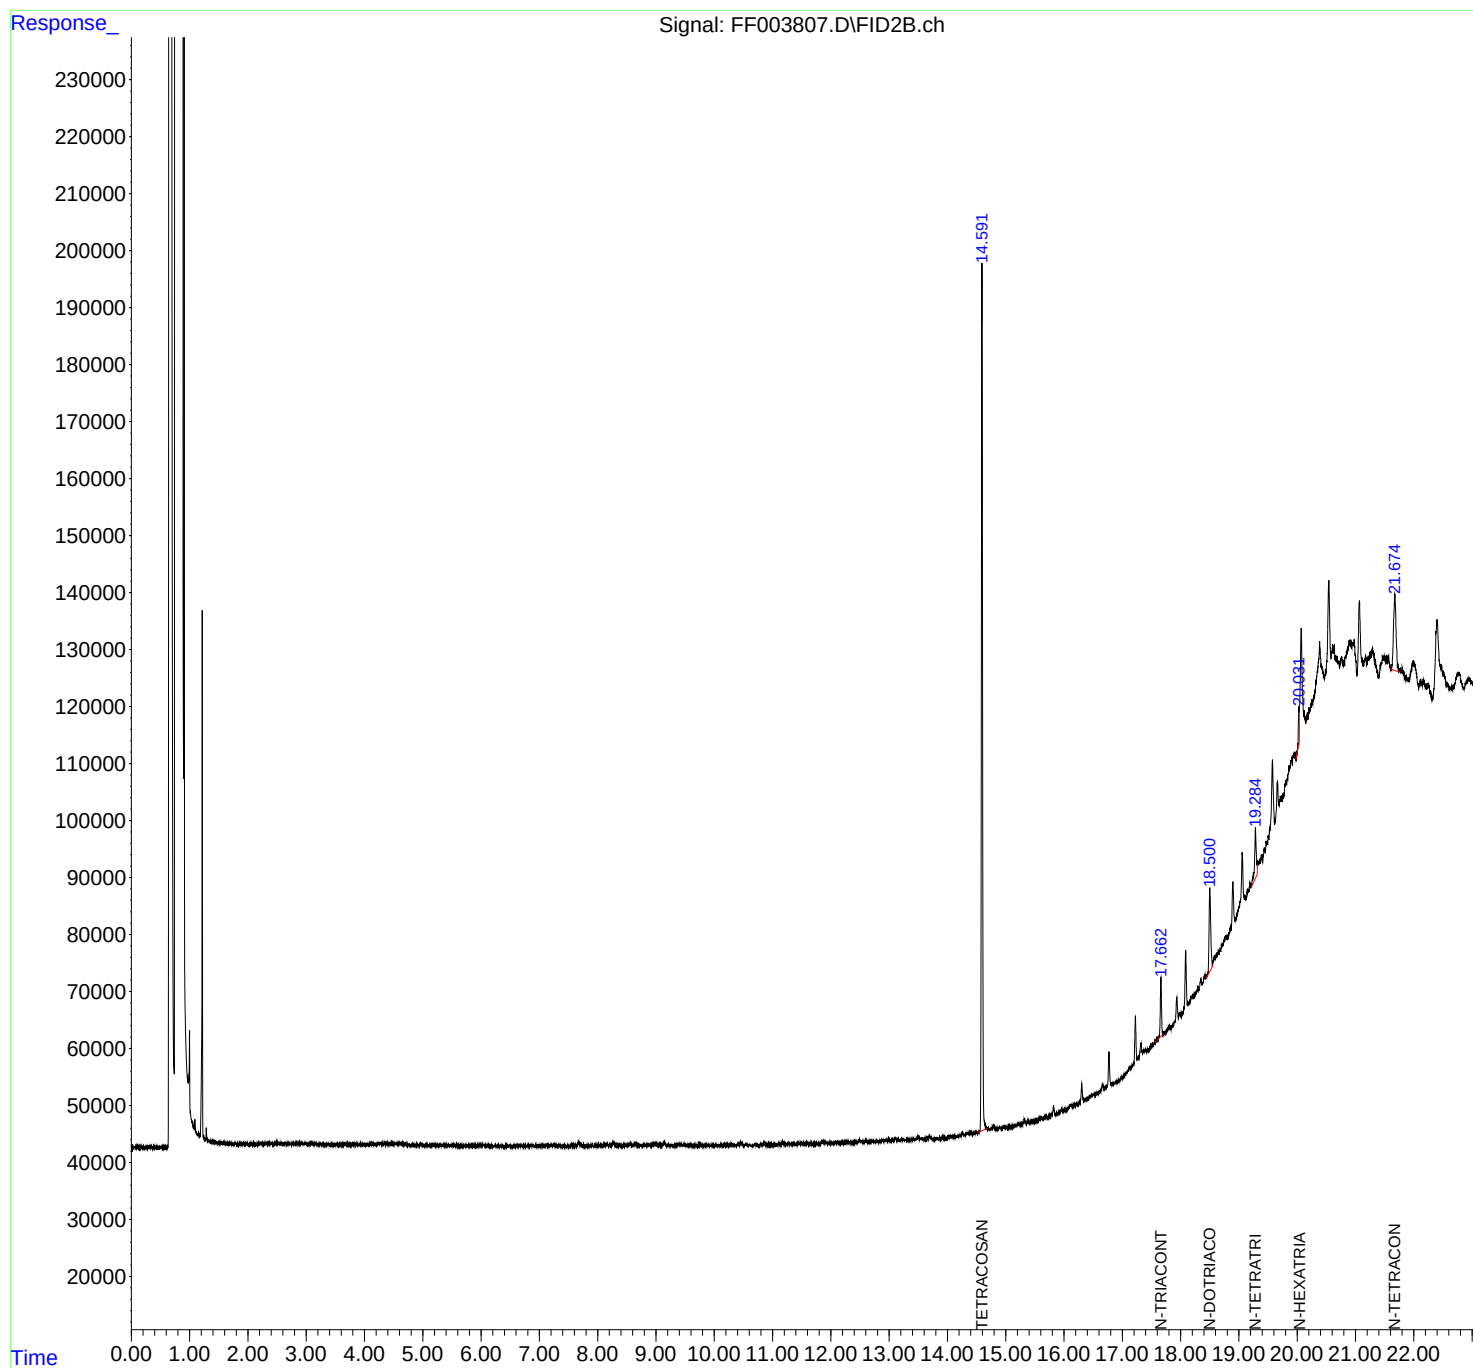


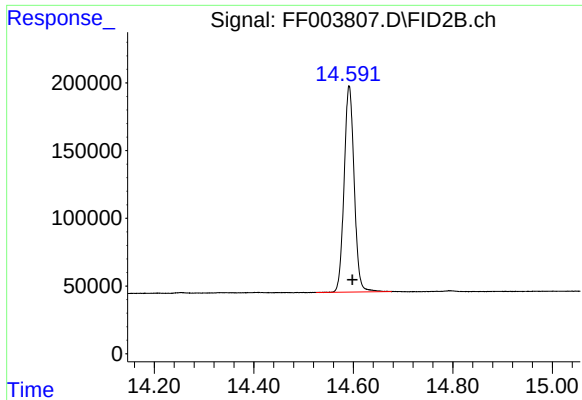

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.592 min
Delta R.T.: -0.006 min
Response: 2137509
Conc: 15.35 ug/ml

Instrument :
FID_F
ClientSampleId :

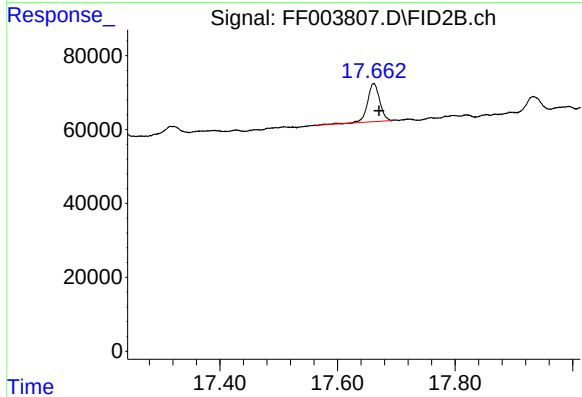


#13 N-TRIACONTANE

R.T.: 17.662 min
Delta R.T.: -0.009 min
Response: 147306
Conc: 1.00 ug/ml

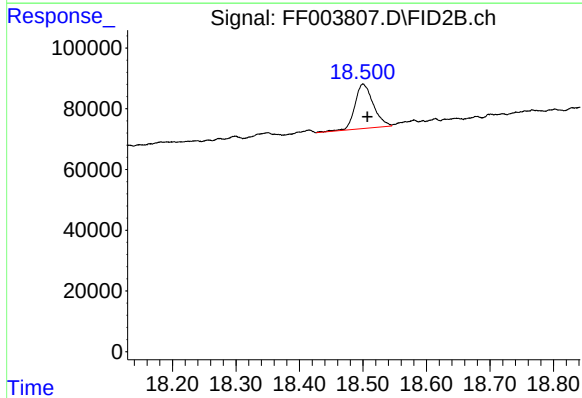


#14 N-DOTRIACONTANE

R.T.: 18.500 min
Delta R.T.: -0.007 min
Response: 294573
Conc: 2.07 ug/ml

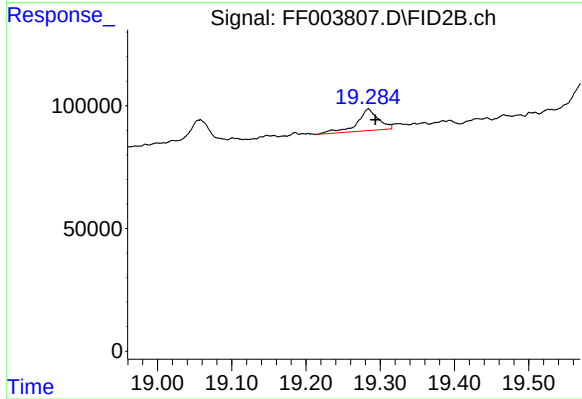

#15 N-TETRATRIACONTANE


R.T.: 19.284 min
Delta R.T.: -0.010 min
Response: 176776
Conc: 1.32 ug/ml

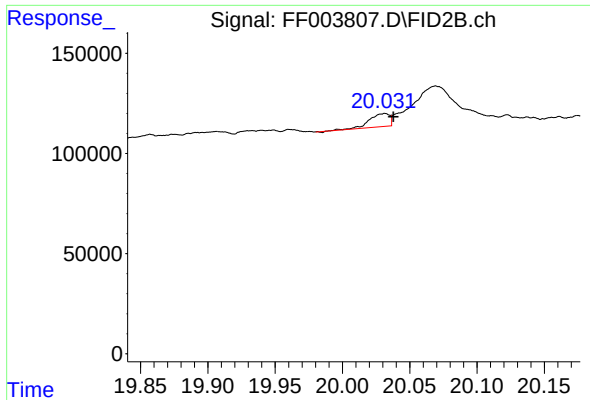

#16 N-HEXATRIACONTANE

R.T.: 20.031 min
Delta R.T.: -0.006 min
Response: 67054
Conc: 0.51 ug/ml

Instrument :
FID_F
ClientSampleId :

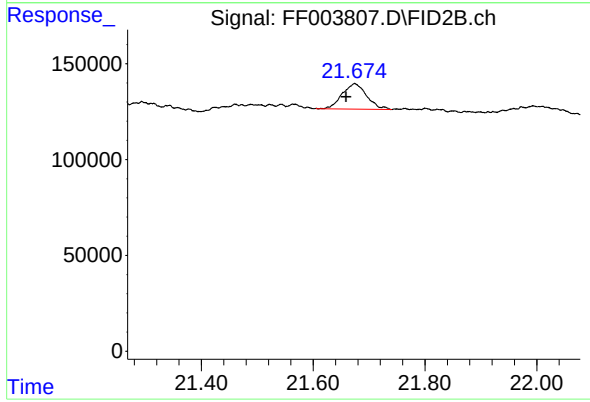

#18 N-TETRACONTANE

R.T.: 21.674 min
Delta R.T.: 0.016 min
Response: 404104
Conc: 3.25 ug/ml