

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
 Data File : FF003804.D
 Signal(s) : FID2B.ch
 Acq On : 12 Mar 2019 18:40
 Operator : AJ\SJ
 Sample : K1846-10MSD
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 TP-1-D2MSD

Integration File: autoint1.e
 Quant Time: Mar 13 01:01:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.591	1894095	13.604 ug/ml
Target Compounds			
2) N-DECANE	4.319	2352481	15.294 ug/ml
3) N-DODECANE	6.340	2425621	15.543 ug/ml
4) N-TETRADECANE	8.134	2478765	15.460 ug/ml
5) N-HEXADECANE	9.734	2488255	15.278 ug/ml
6) N-OCTADECANE	11.177	2462089	14.944 ug/ml
7) N-EICOSANE	12.489	2378942	14.542 ug/ml
8) N-DOCOSANE	13.690	2352586	14.577 ug/ml
10) N-TETRACOSANE	14.796	2359191	14.911 ug/ml
11) N-HEXACOSANE	15.820	2328698	15.088 ug/ml
12) N-OCTACOSANE	16.774	2438144	16.134 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF03804.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 18:40
Operator : AJ\SJ
Sample : K1846-10MSD
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TP-1-D2MSD

Integration File: autoint1.e
Quant Time: Mar 13 01:01:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

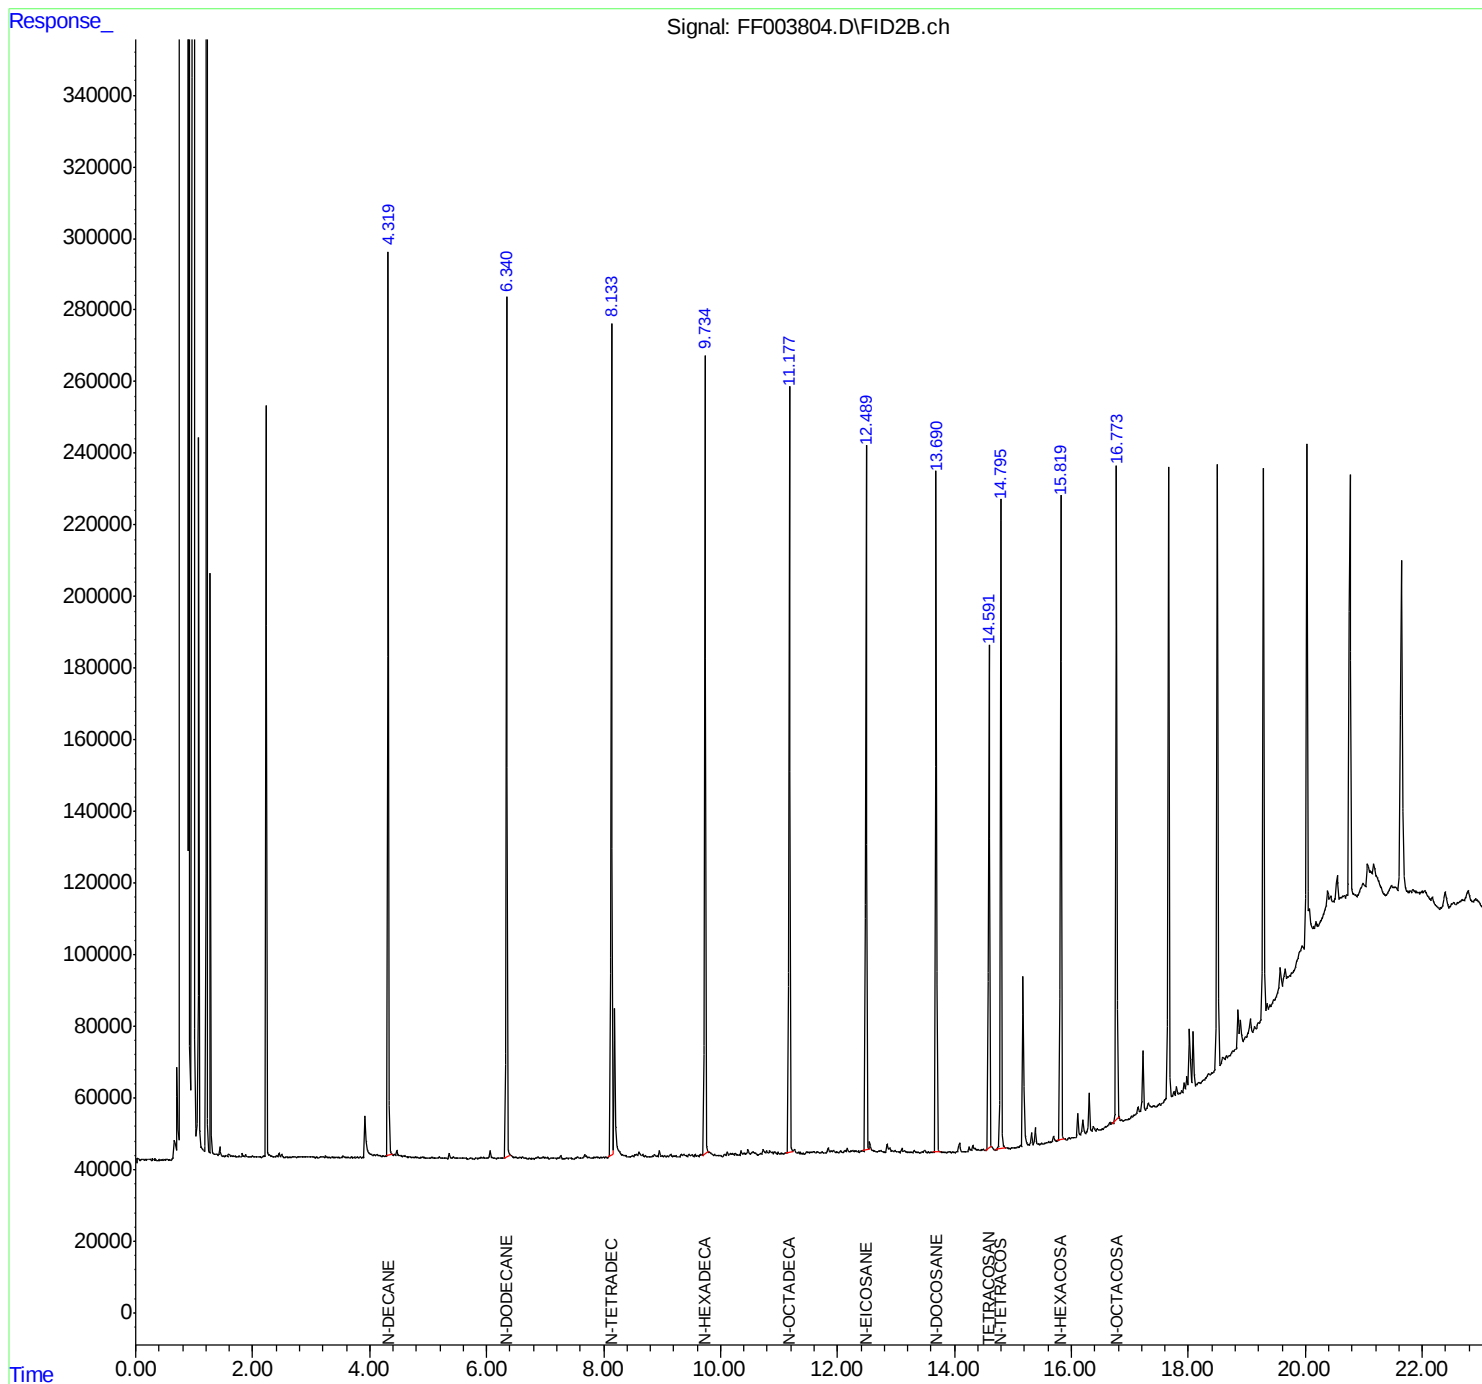


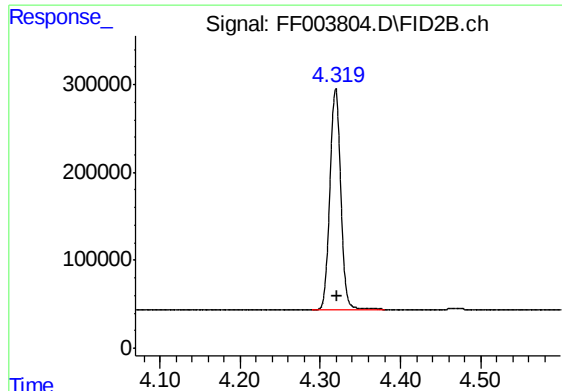

#2 N-DECANE


R.T.: 4.319 min
Delta R.T.: -0.002 min
Response: 2352481
Conc: 15.29 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-1-D2MSD

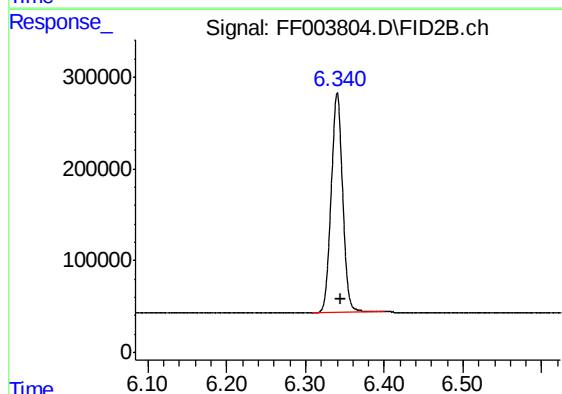


#3 N-DODECANE

R.T.: 6.340 min
Delta R.T.: -0.004 min
Response: 2425621
Conc: 15.54 ug/ml

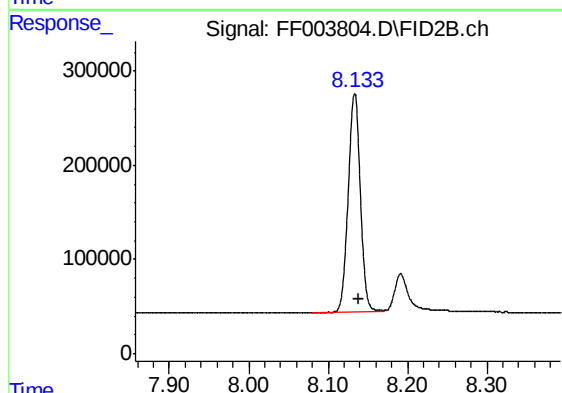


#4 N-TETRADECANE

R.T.: 8.134 min
Delta R.T.: -0.005 min
Response: 2478765
Conc: 15.46 ug/ml

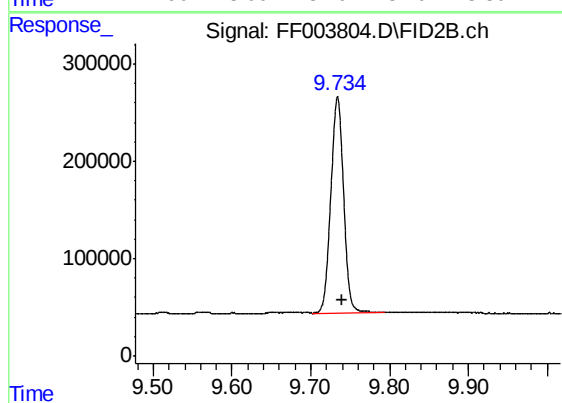

#5 N-HEXADECANE


R.T.: 9.734 min
Delta R.T.: -0.006 min
Response: 2488255
Conc: 15.28 ug/ml

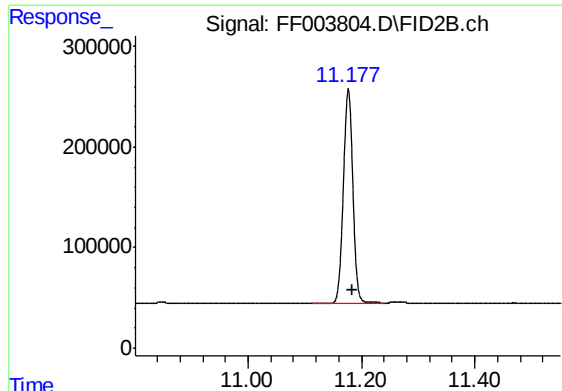

#6 N-OCTADECANE


R.T.: 11.177 min
Delta R.T.: -0.007 min
Response: 2462089
Conc: 14.94 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-1-D2MSD

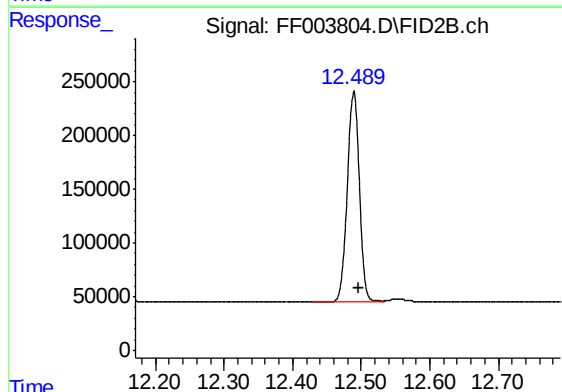


#7 N-EICOSANE

R.T.: 12.489 min
Delta R.T.: -0.007 min
Response: 2378942
Conc: 14.54 ug/ml

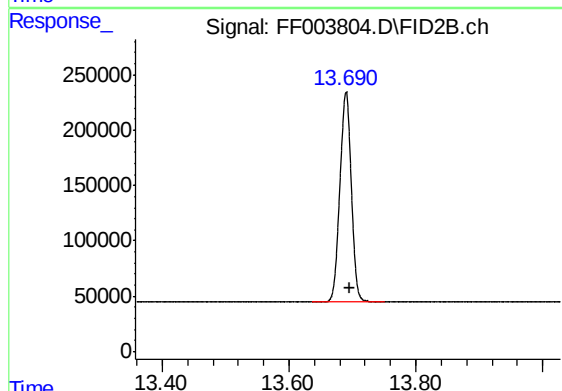


#8 N-DOCOSANE

R.T.: 13.690 min
Delta R.T.: -0.007 min
Response: 2352586
Conc: 14.58 ug/ml

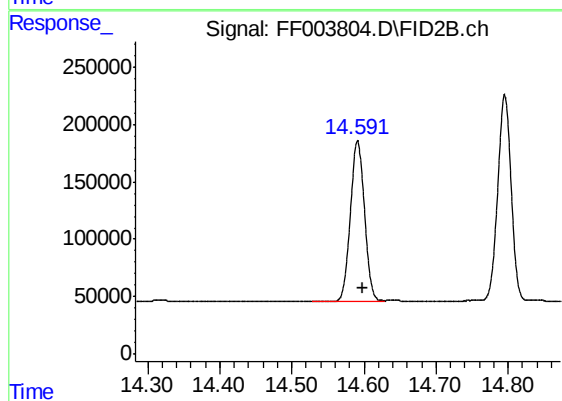

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.591 min
Delta R.T.: -0.007 min
Response: 1894095
Conc: 13.60 ug/ml

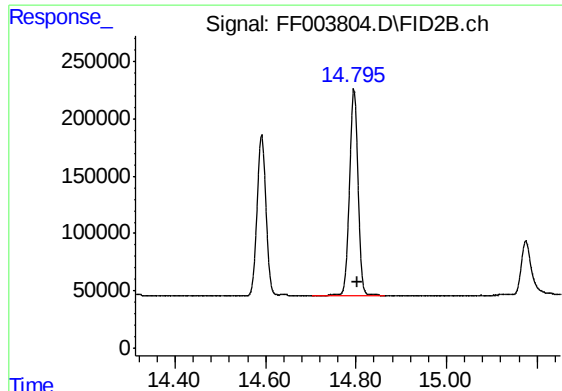

#10 N-TETRACOSANE


R.T.: 14.796 min
Delta R.T.: -0.007 min
Response: 2359191
Conc: 14.91 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-1-D2MSD

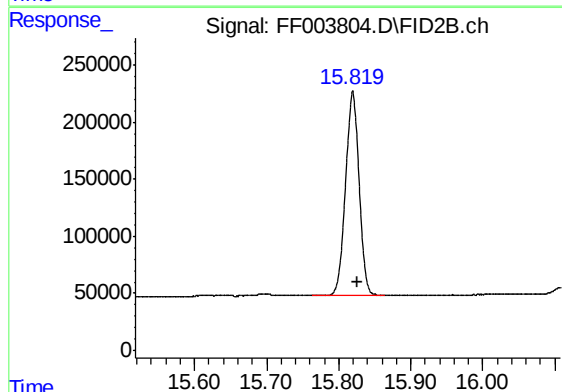

#11 N-HEXACOSANE

R.T.: 15.820 min
Delta R.T.: -0.007 min
Response: 2328698
Conc: 15.09 ug/ml

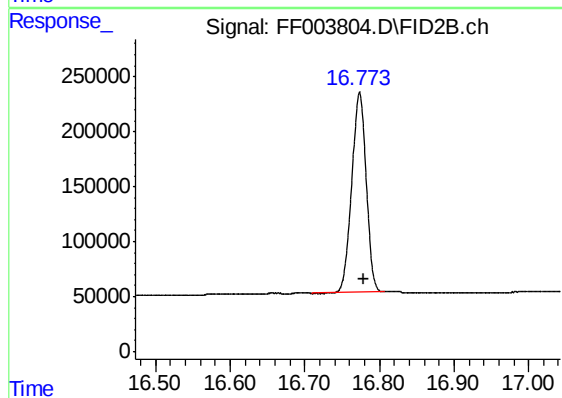

#12 N-OCTACOSANE

R.T.: 16.774 min
Delta R.T.: -0.006 min
Response: 2438144
Conc: 16.13 ug/ml