

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031220\
Data File : FF006536.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2020 09:35
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 13 01:34:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.585	2505136	19.465 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.636	101882	0.720 ug/ml
14) N-DOTRIACONTANE	18.466	214171	1.589 ug/ml
16) N-HEXATRIACONTANE	20.012	275775	3.003 ug/ml
18) N-TETRACONTANE	21.582	346113	5.002 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031220\
Data File : FF006536.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2020 09:35
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 13 01:34:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

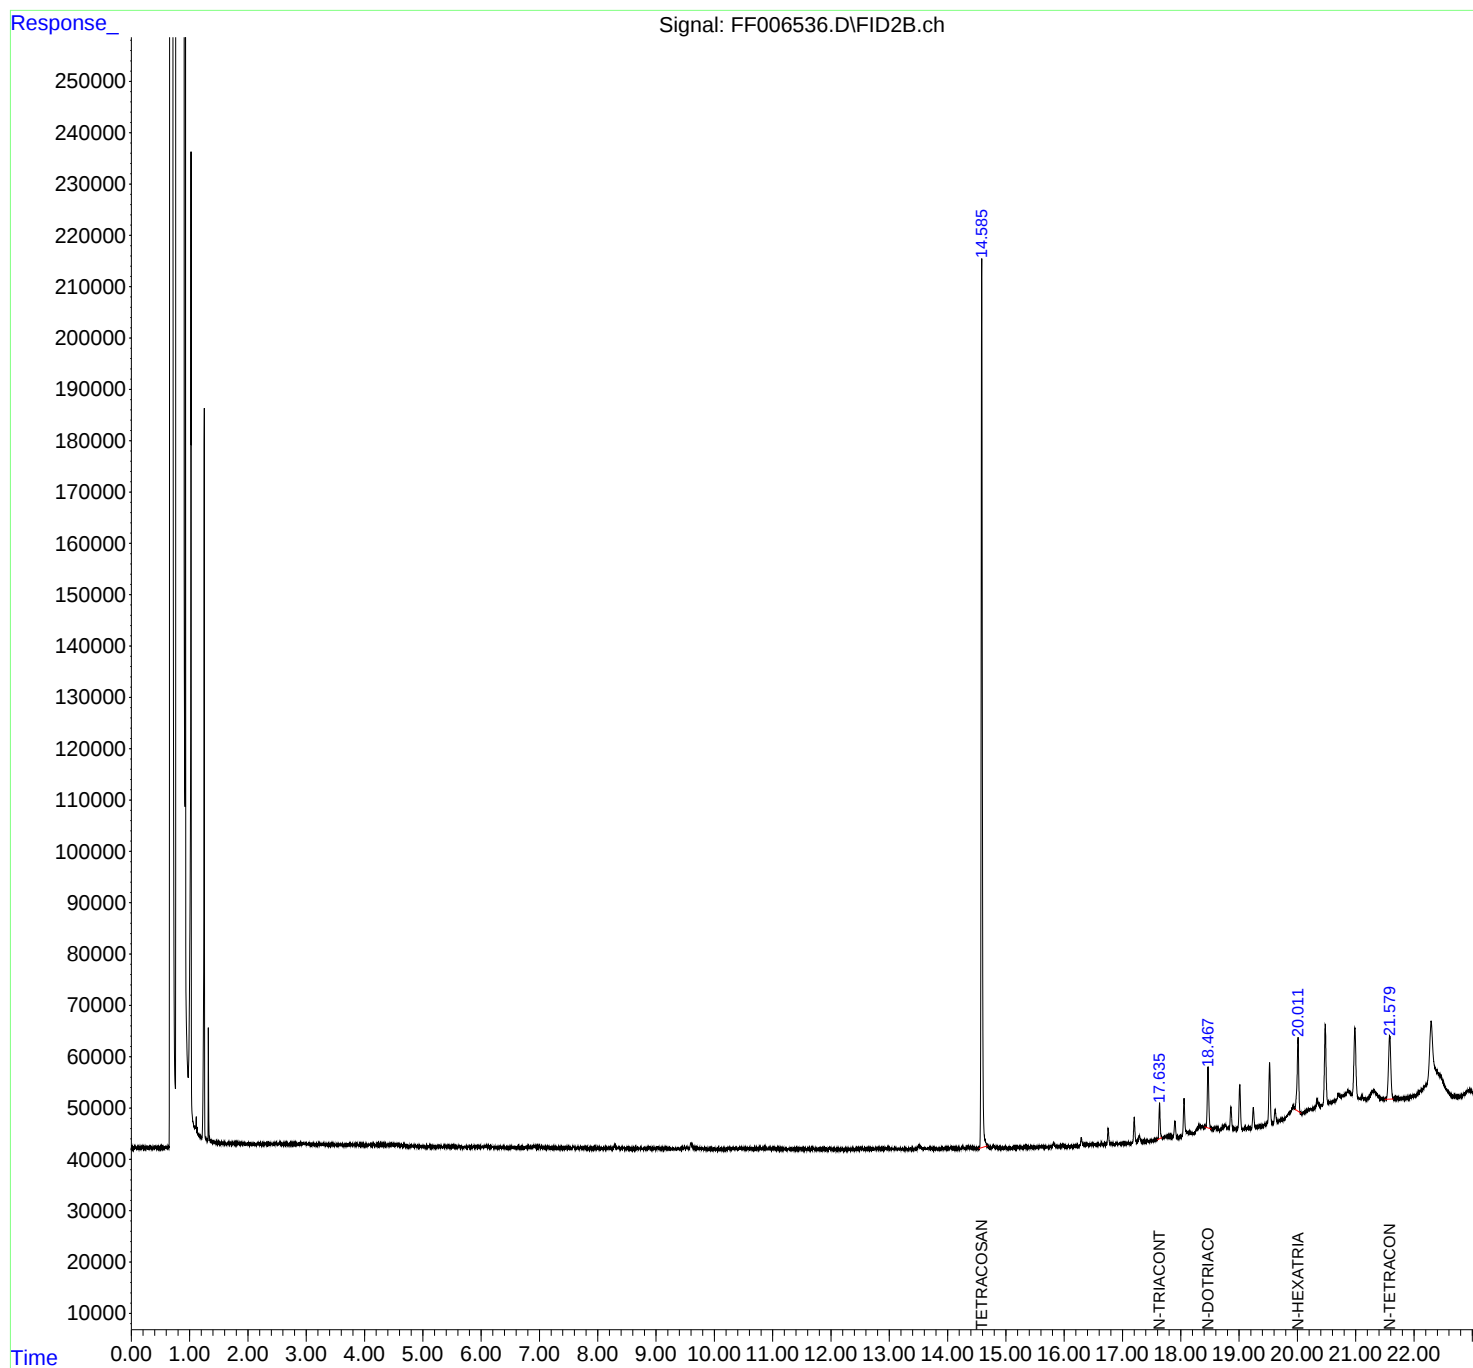

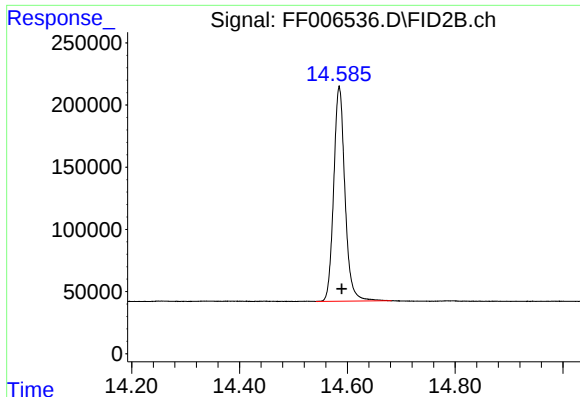


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.585 min
Delta R.T.: -0.005 min
Response: 2505136
Conc: 19.46 ug/ml

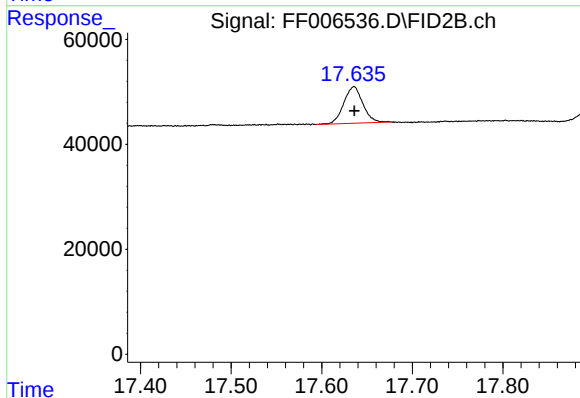


#13 N-TRIACONTANE

R.T.: 17.636 min
Delta R.T.: 0.000 min
Response: 101882
Conc: 0.72 ug/ml

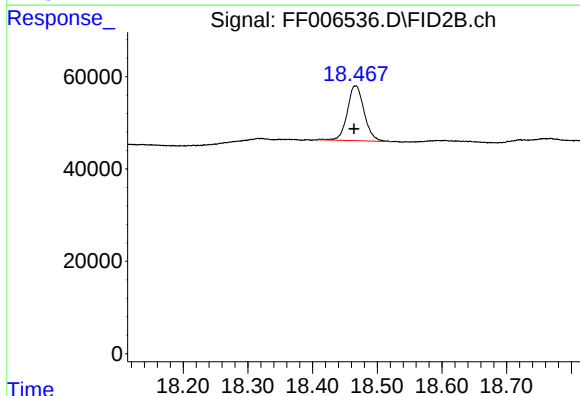


#14 N-DOTRIACONTANE

R.T.: 18.466 min
Delta R.T.: 0.002 min
Response: 214171
Conc: 1.59 ug/ml

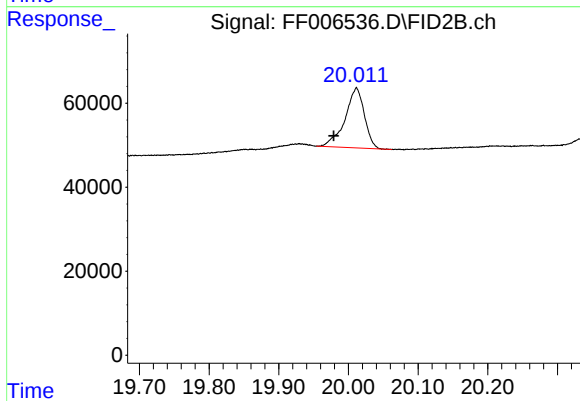

#16 N-HEXATRIACONTANE

R.T.: 20.012 min
Delta R.T.: 0.033 min
Response: 275775
Conc: 3.00 ug/ml

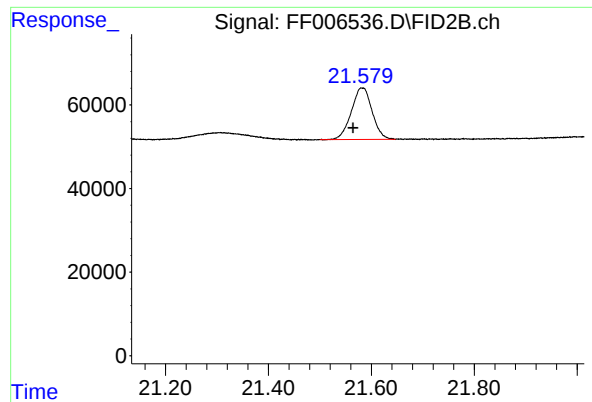

#18 N-TETRACONTANE

R.T.: 21.582 min
Delta R.T.: 0.018 min
Response: 346113
Conc: 5.00 ug/ml