

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
Data File : FF003812.D
Signal(s) : FID2B.ch
Acq On : 13 Mar 2019 10:52
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 14 00:59:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.334	2799363	17.937 ug/ml
12)	N-OCTACOSANE	16.772	2646503	17.513 ug/ml
13)	N-TRIACONTANE	17.660	181420	1.233 ug/ml
14)	N-DOTRIACONTANE	18.497	235836	1.658 ug/ml
15)	N-TETRATRIACONTANE	19.284	134483	1.004 ug/ml
16)	N-HEXATRIACONTANE	20.028	100000	0.766 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
Data File : FF003812.D
Signal(s) : FID2B.ch
Acq On : 13 Mar 2019 10:52
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 14 00:59:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

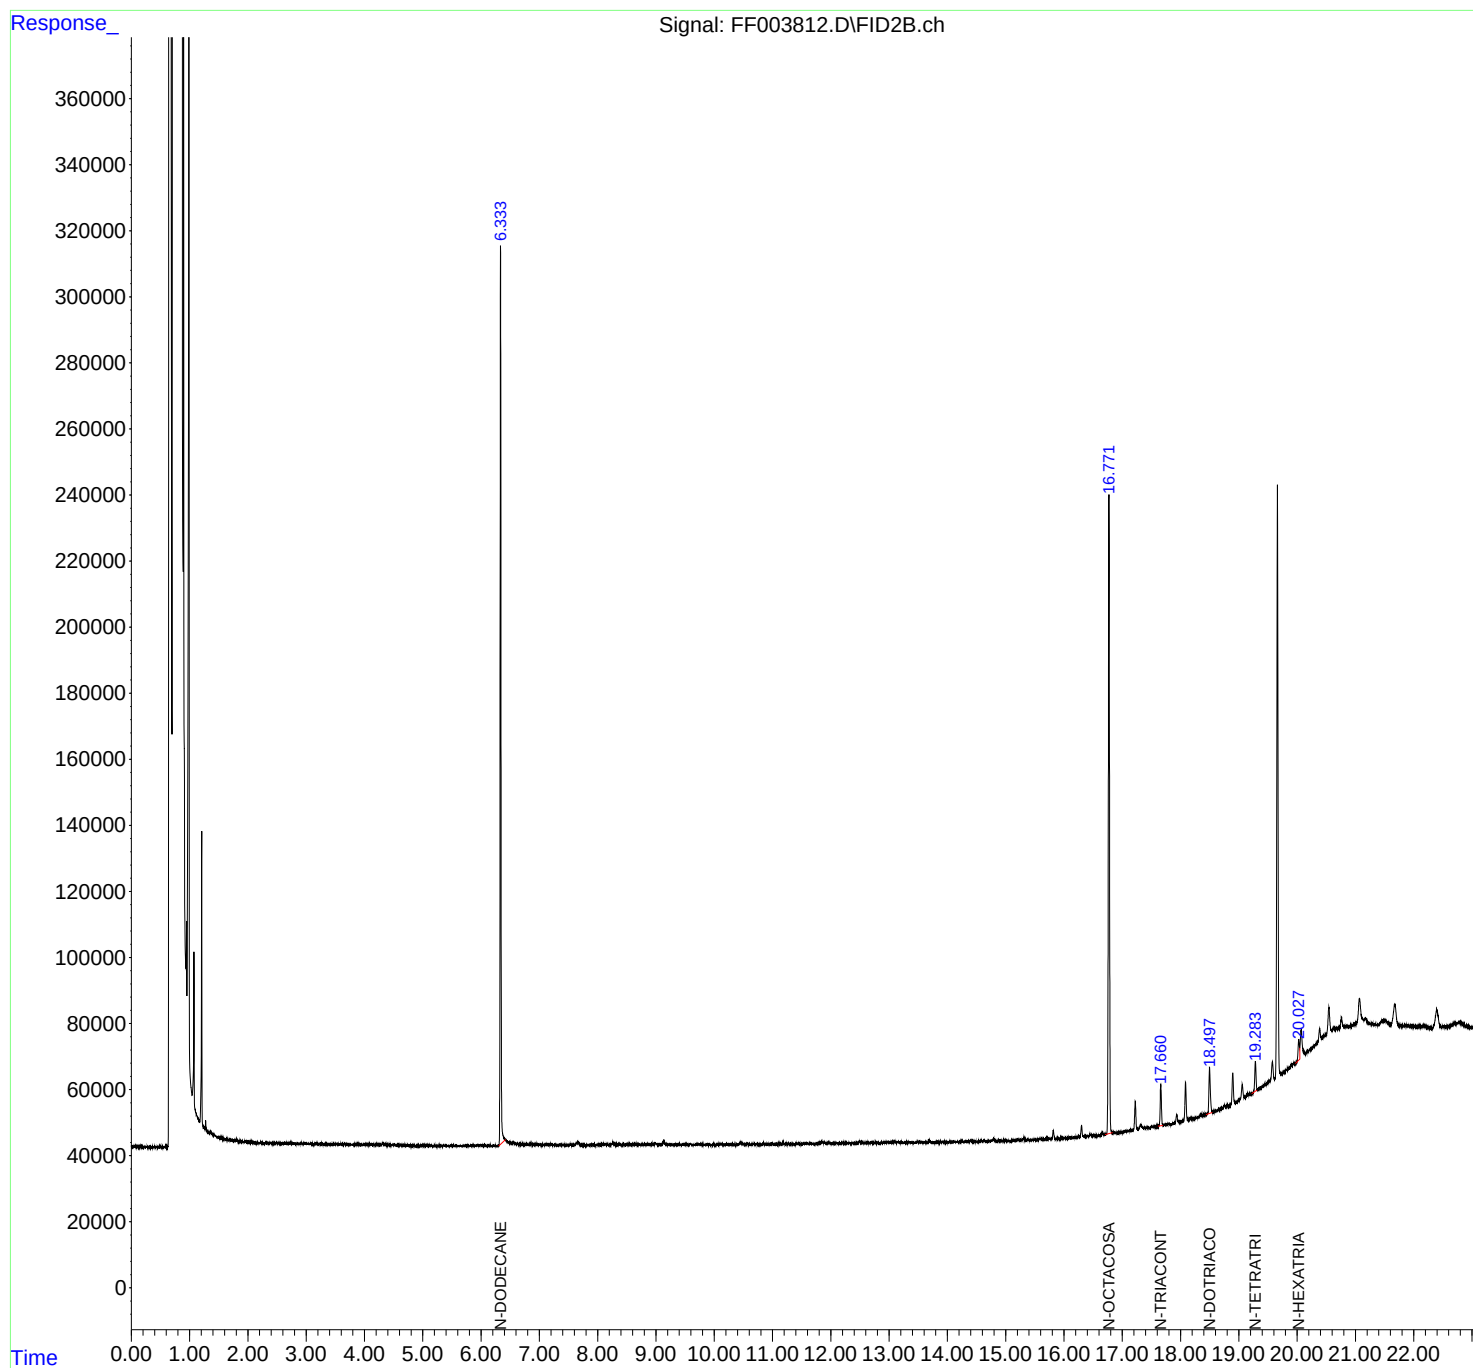


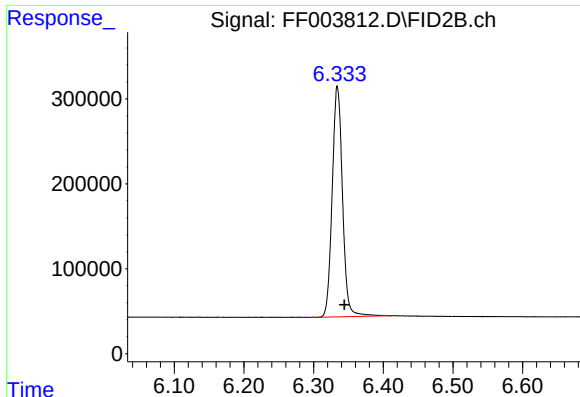

#3 N-DODECANE


R.T.: 6.334 min
Delta R.T.: -0.010 min
Response: 2799363
Conc: 17.94 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

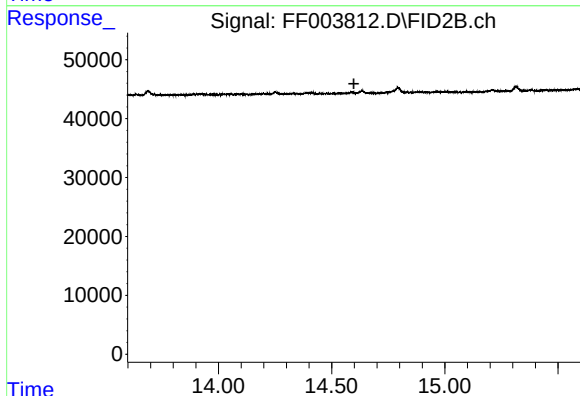


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.598 min
Response: 0
Conc: N.D.

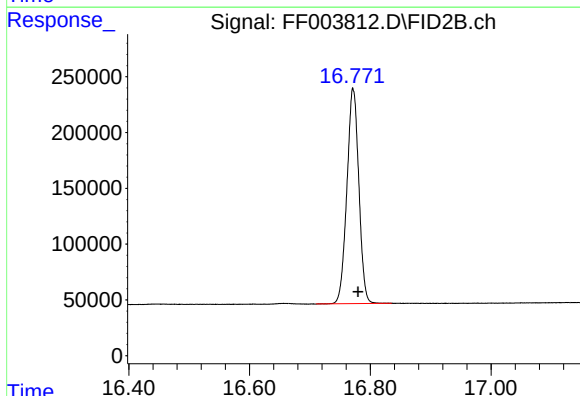


#12 N-OCTACOSANE

R.T.: 16.772 min
Delta R.T.: -0.008 min
Response: 2646503
Conc: 17.51 ug/ml

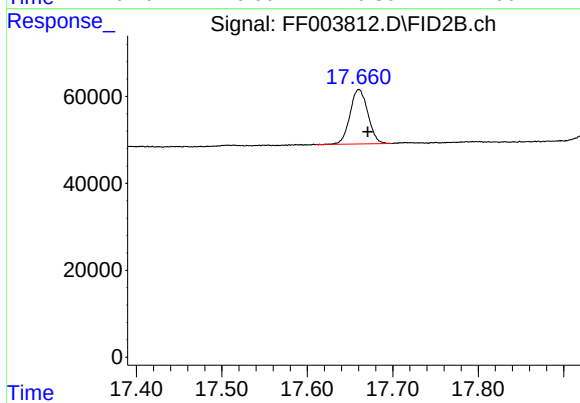

#13 N-TRIACONTANE


R.T.: 17.660 min
Delta R.T.: -0.010 min
Response: 181420
Conc: 1.23 ug/ml

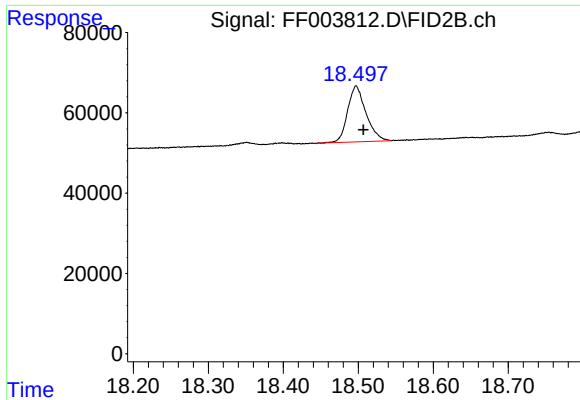

#14 N-DOTRIACONTANE


R.T.: 18.497 min
Delta R.T.: -0.010 min
Response: 235836
Conc: 1.66 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

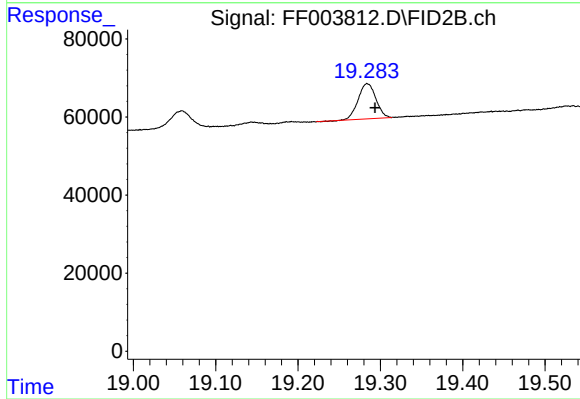

#15 N-TETRATRIACONTANE

R.T.: 19.284 min
Delta R.T.: -0.010 min
Response: 134483
Conc: 1.00 ug/ml

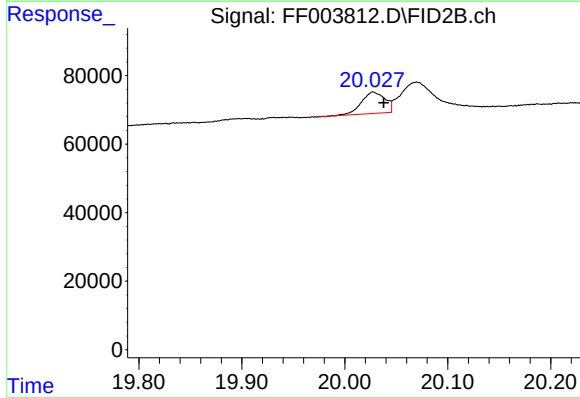

#16 N-HEXATRIACONTANE

R.T.: 20.028 min
Delta R.T.: -0.010 min
Response: 100000
Conc: 0.77 ug/ml