

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
 Data File : FF003813.D
 Signal(s) : FID2B.ch
 Acq On : 13 Mar 2019 11:31
 Operator : AJ\SJ
 Sample : K1846-01 2X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 TP-2-1

Integration File: autoint1.e
 Quant Time: Mar 14 00:59:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.590	1079030	7.750 ug/ml
Target Compounds			
4) N-TETRADECANE	8.187	179146	1.117 ug/ml
7) N-EICOSANE	12.486	84620	0.517 ug/ml
8) N-DOCOSANE	13.708	227041	1.407 ug/ml
10) N-TETRACOSANE	14.766	1207976	7.635 ug/ml
11) N-HEXACOSANE	15.816	146190	0.947 ug/ml
12) N-OCTACOSANE	16.779	654772	4.333 ug/ml
13) N-TRIACONTANE	17.662	973482	6.618 ug/ml
14) N-DOTRIACONTANE	18.499	569163	4.002 ug/ml
15) N-TETRATRIACONTANE	19.297	1502440	11.221 ug/ml
16) N-HEXATRIACONTANE	20.035	740278	5.673 ug/ml
17) N-OCTATRIACONTANE	20.777	668072	5.786 ug/ml
18) N-TETRACONTANE	21.661	295660	2.377 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
Data File : FF003813.D
Signal(s) : FID2B.ch
Acq On : 13 Mar 2019 11:31
Operator : AJ\SJ
Sample : K1846-01 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TP-2-1

Integration File: autoint1.e
Quant Time: Mar 14 00:59:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

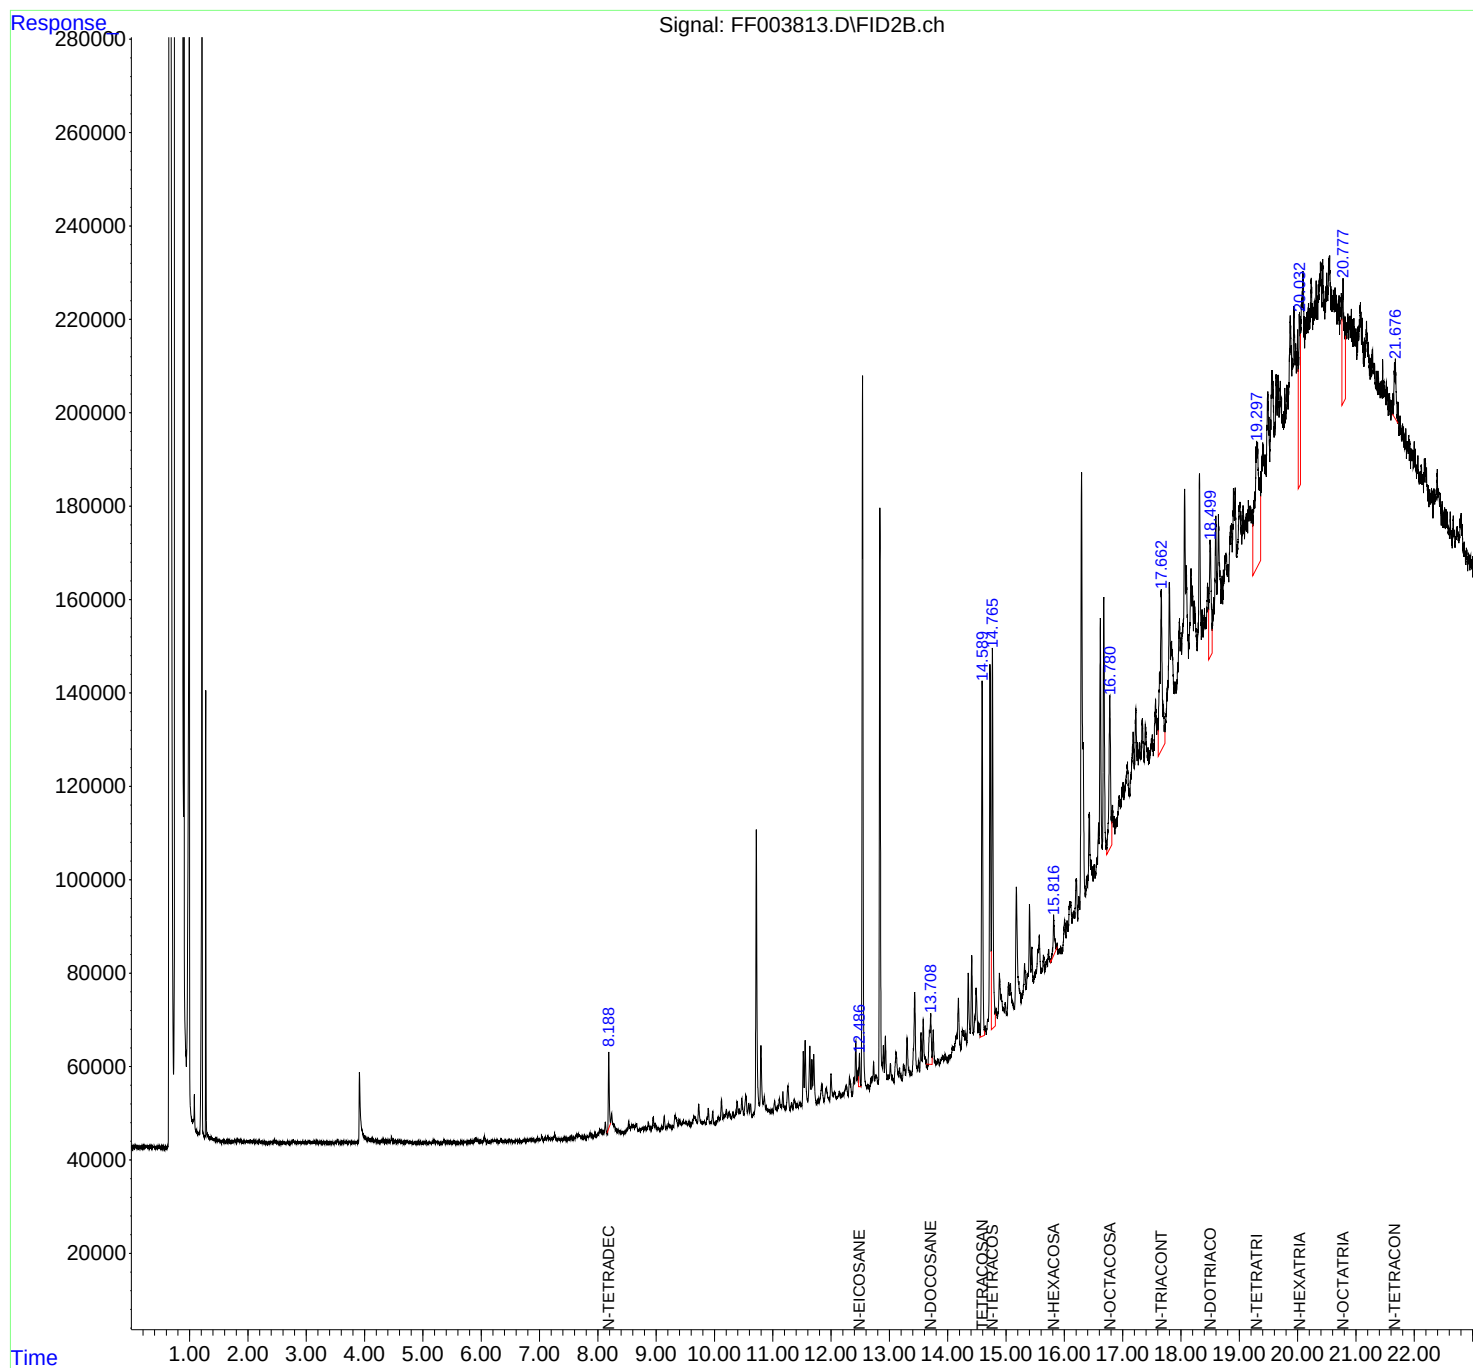


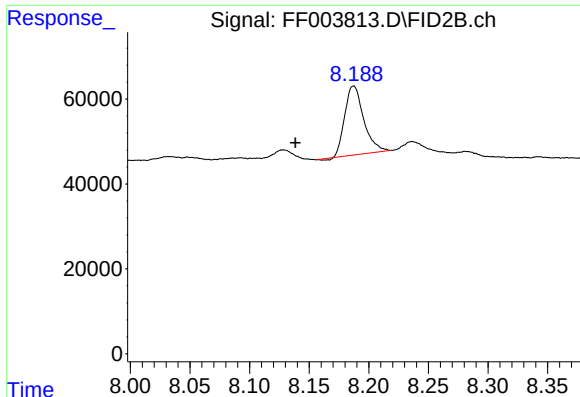

#4 N-TETRADECANE


R.T.: 8.187 min
Delta R.T.: 0.049 min
Response: 179146
Conc: 1.12 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-2-1

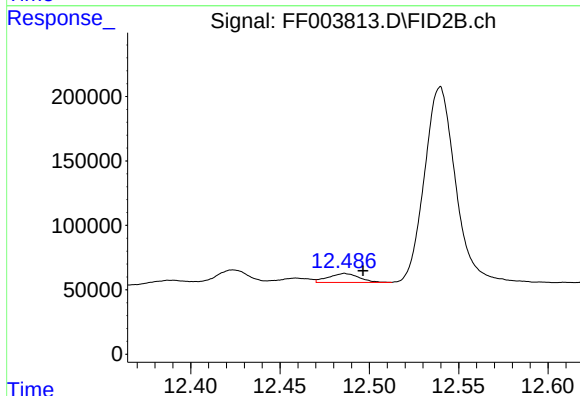


#7 N-EICOSANE

R.T.: 12.486 min
Delta R.T.: -0.010 min
Response: 84620
Conc: 0.52 ug/ml

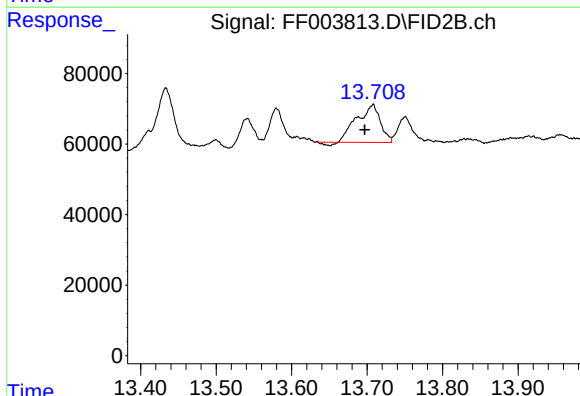


#8 N-DOCOSANE

R.T.: 13.708 min
Delta R.T.: 0.011 min
Response: 227041
Conc: 1.41 ug/ml

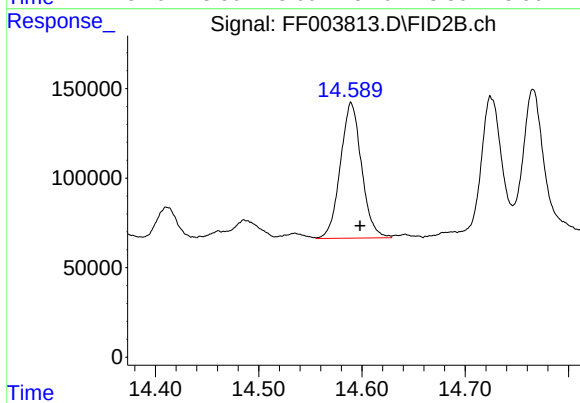

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.590 min
Delta R.T.: -0.009 min
Response: 1079030
Conc: 7.75 ug/ml

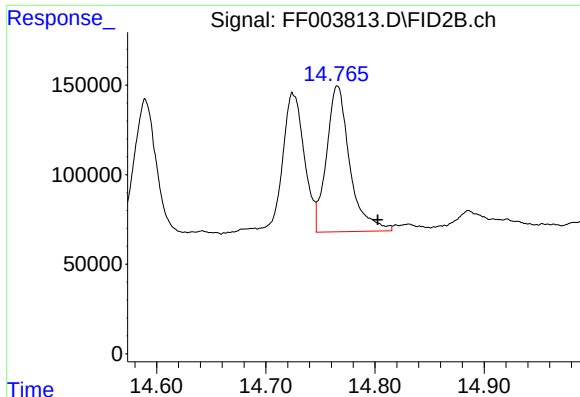

#10 N-TETRACOSANE


R.T.: 14.766 min
Delta R.T.: -0.037 min
Response: 1207976
Conc: 7.63 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-2-1

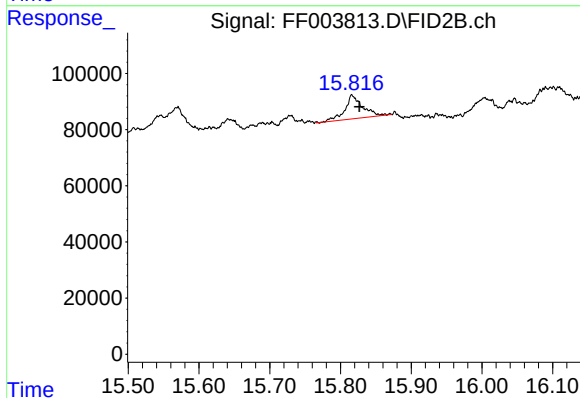


#11 N-HEXACOSANE

R.T.: 15.816 min
Delta R.T.: -0.011 min
Response: 146190
Conc: 0.95 ug/ml

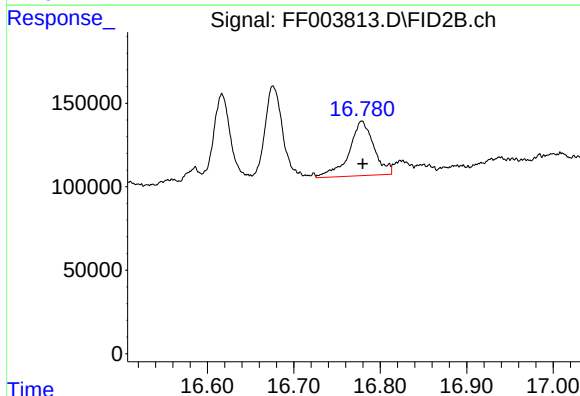


#12 N-OCTACOSANE

R.T.: 16.779 min
Delta R.T.: 0.000 min
Response: 654772
Conc: 4.33 ug/ml

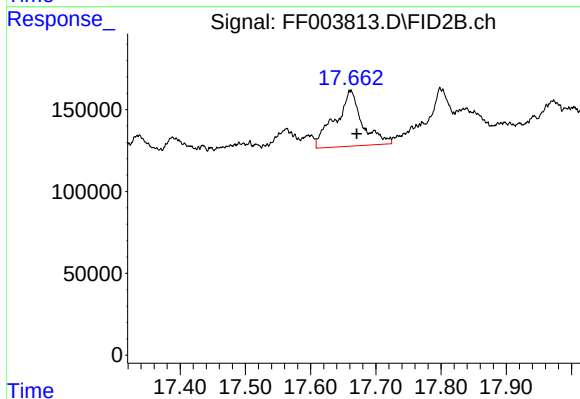

#13 N-TRIACONTANE


R.T.: 17.662 min
Delta R.T.: -0.009 min
Response: 973482
Conc: 6.62 ug/ml

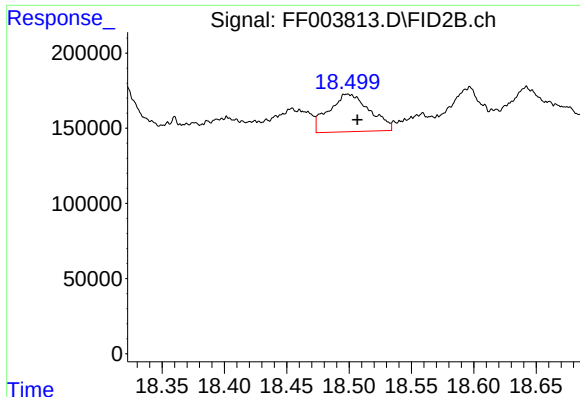

#14 N-DOTRIACONTANE


R.T.: 18.499 min
Delta R.T.: -0.007 min
Response: 569163
Conc: 4.00 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-2-1

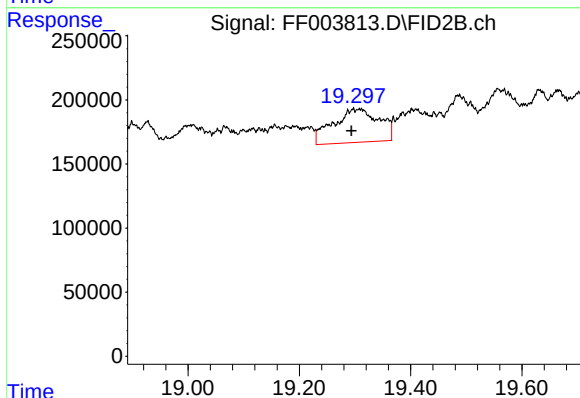


#15 N-TETRATRIACONTANE

R.T.: 19.297 min
Delta R.T.: 0.004 min
Response: 1502440
Conc: 11.22 ug/ml

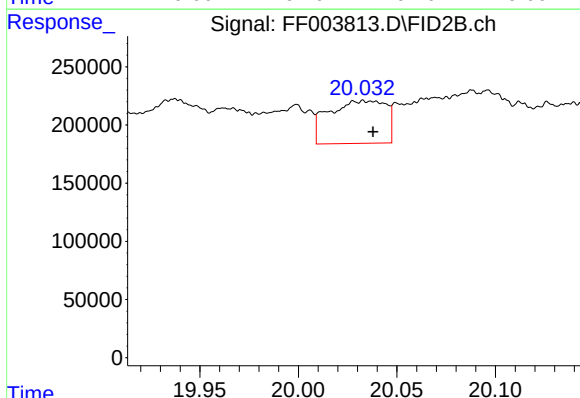


#16 N-HEXATRIACONTANE

R.T.: 20.035 min
Delta R.T.: -0.003 min
Response: 740278
Conc: 5.67 ug/ml

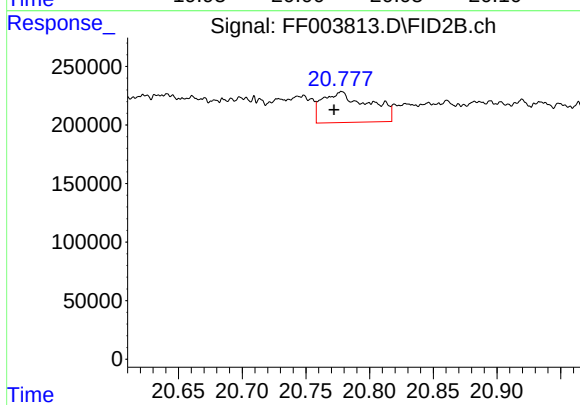

#17 N-OCTATRIACONTANE

R.T.: 20.777 min
Delta R.T.: 0.005 min
Response: 668072
Conc: 5.79 ug/ml

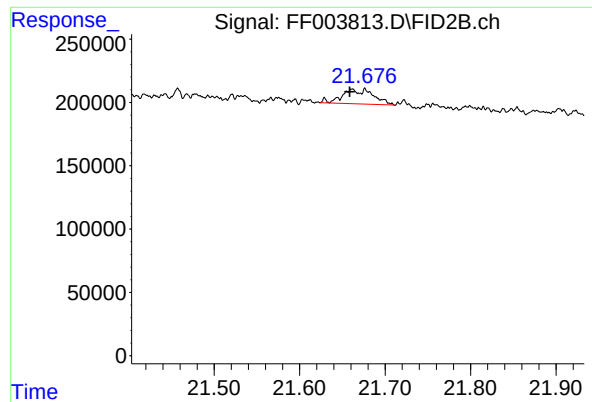

#18 N-TETRACONTANE

R.T.: 21.661 min
Delta R.T.: 0.003 min
Response: 295660
Conc: 2.38 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-2-1