

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
 Data File : FF003814.D
 Signal(s) : FID2B.ch
 Acq On : 13 Mar 2019 12:01
 Operator : AJ\SJ
 Sample : K1846-02 2X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 TP-2-2

Integration File: autoint1.e
 Quant Time: Mar 14 00:59:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.591	1118026	8.030 ug/ml
Target Compounds			
4) N-TETRADECANE	8.190f	195797	1.221 ug/ml
7) N-EICOSANE	12.541	941007	5.752 ug/ml
10) N-TETRACOSANE	14.768	479685	3.032 ug/ml
11) N-HEXACOSANE	15.823	110564	0.716 ug/ml
12) N-OCTACOSANE	16.778	569649	3.770 ug/ml
13) N-TRIACONTANE	17.661	600387	4.081 ug/ml
14) N-DOTRIACONTANE	18.502	671027	4.719 ug/ml
15) N-TETRATRIACONTANE	19.310	1216862	9.088 ug/ml
16) N-HEXATRIACONTANE	20.046	1413312	10.832 ug/ml
17) N-OCTATRIACONTANE	20.763	1247574	10.805 ug/ml
18) N-TETRACONTANE	21.661	161980	1.302 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
Data File : FF003814.D
Signal(s) : FID2B.ch
Acq On : 13 Mar 2019 12:01
Operator : AJ\SJ
Sample : K1846-02 2X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TP-2-2

Integration File: autoint1.e
Quant Time: Mar 14 00:59:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

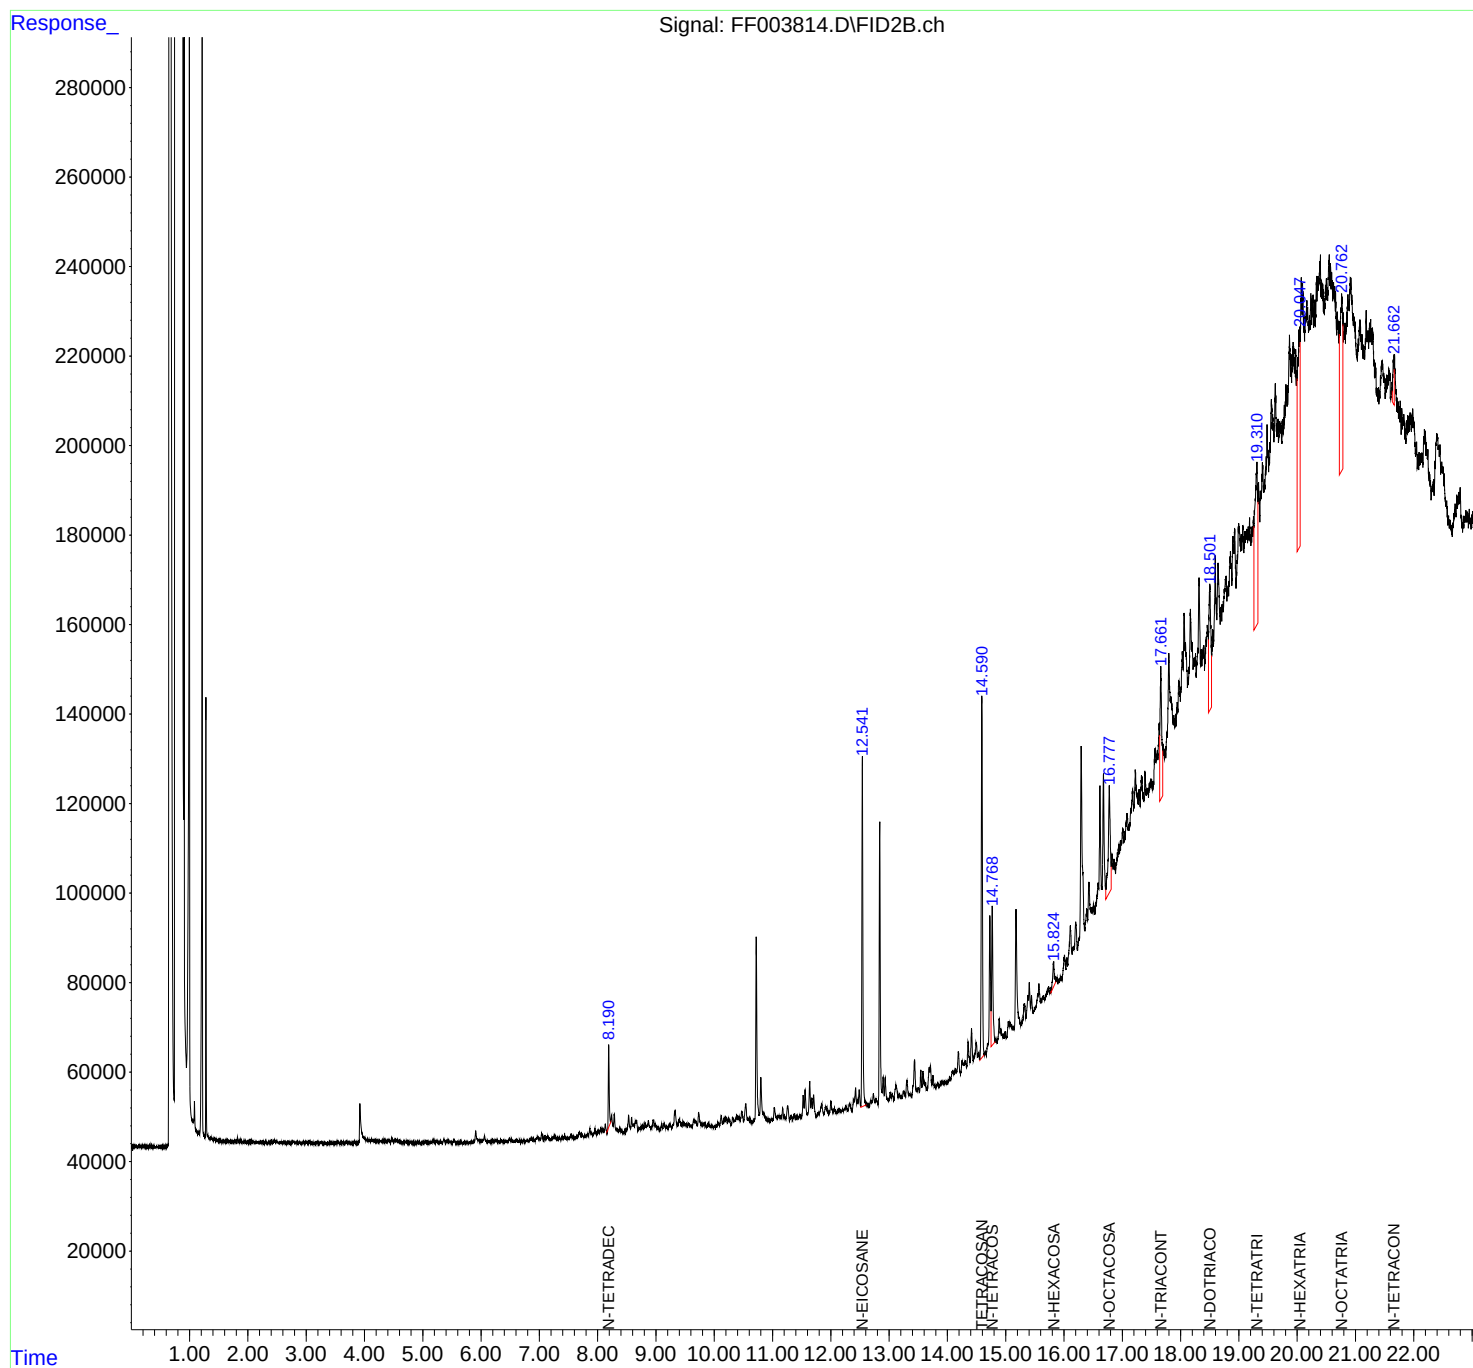


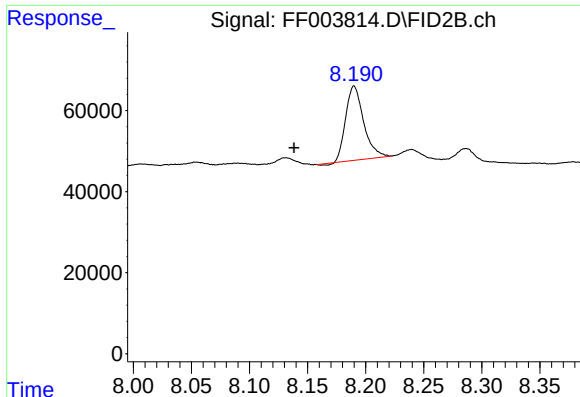

#4 N-TETRADECANE


R.T.: 8.190 min
Delta R.T.: 0.052 min
Response: 195797
Conc: 1.22 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-2-2

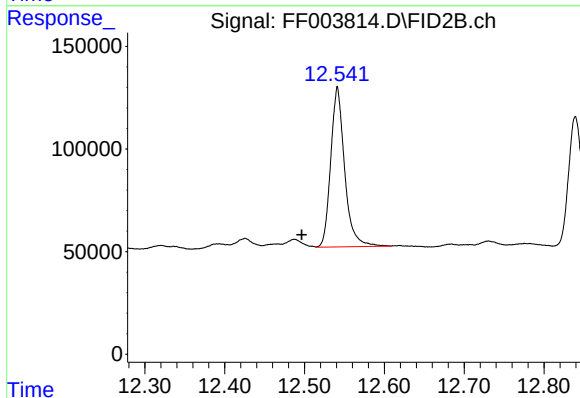


#7 N-EICOSANE

R.T.: 12.541 min
Delta R.T.: 0.045 min
Response: 941007
Conc: 5.75 ug/ml

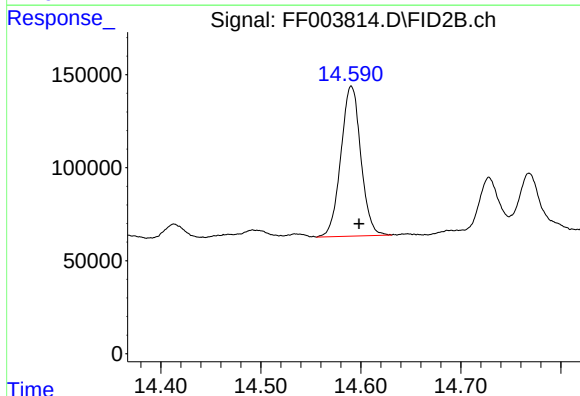


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.591 min
Delta R.T.: -0.008 min
Response: 1118026
Conc: 8.03 ug/ml

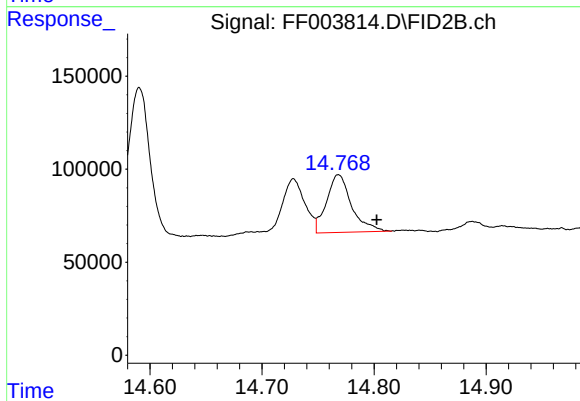

#10 N-TETRACOSANE


R.T.: 14.768 min
Delta R.T.: -0.034 min
Response: 479685
Conc: 3.03 ug/ml

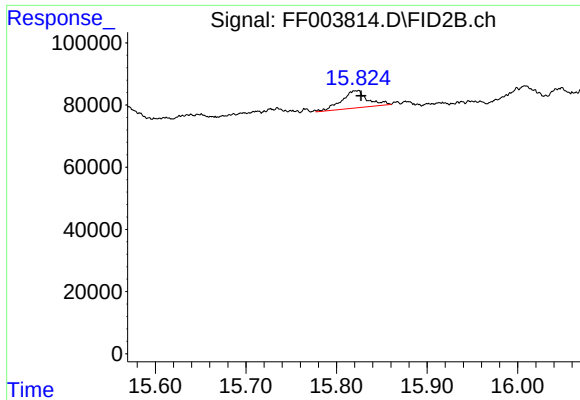

#11 N-HEXACOSANE


R.T.: 15.823 min
Delta R.T.: -0.003 min
Response: 110564
Conc: 0.72 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-2-2

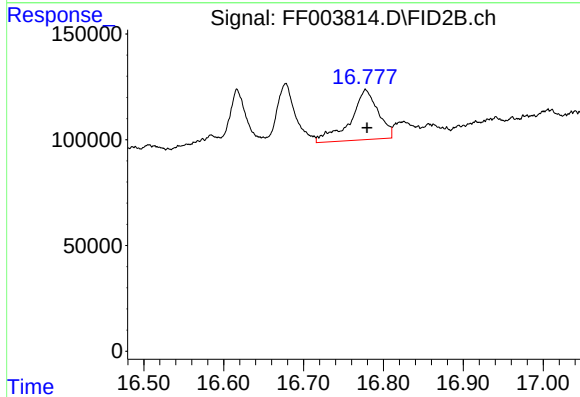


#12 N-OCTACOSANE

R.T.: 16.778 min
Delta R.T.: -0.002 min
Response: 569649
Conc: 3.77 ug/ml

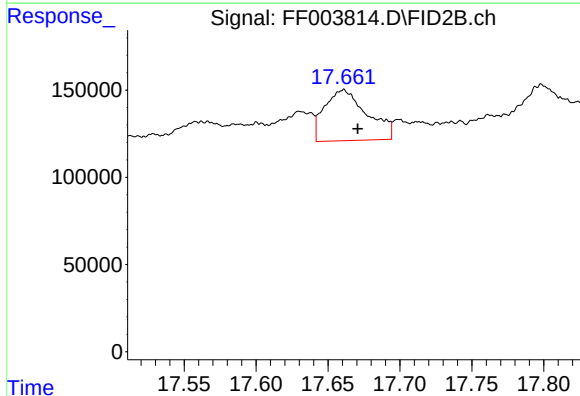


#13 N-TRIACONTANE

R.T.: 17.661 min
Delta R.T.: -0.010 min
Response: 600387
Conc: 4.08 ug/ml

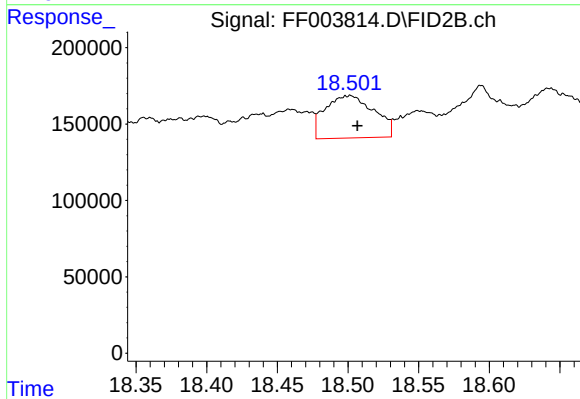

#14 N-DOTRIACONTANE


R.T.: 18.502 min
Delta R.T.: -0.005 min
Response: 671027
Conc: 4.72 ug/ml

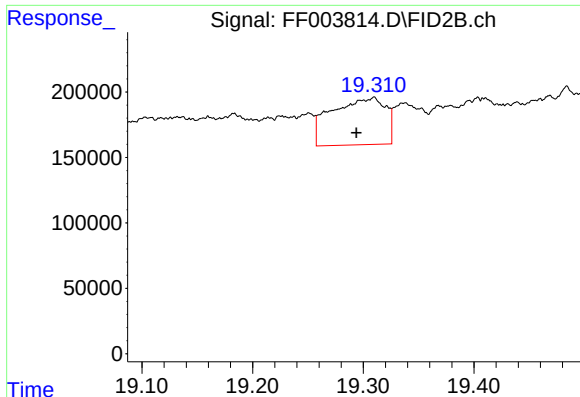

#15 N-TETRATRIACONTANE


R.T.: 19.310 min
Delta R.T.: 0.016 min
Response: 1216862
Conc: 9.09 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-2-2

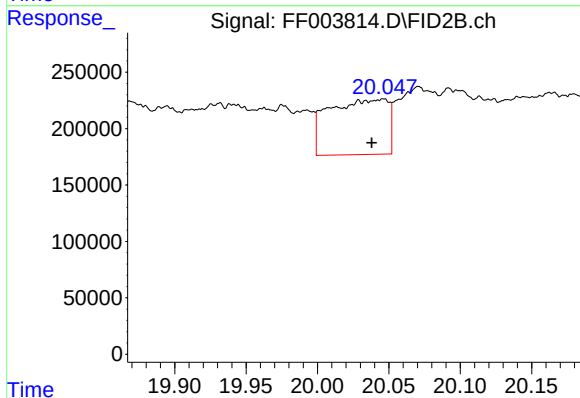


#16 N-HEXATRIACONTANE

R.T.: 20.046 min
Delta R.T.: 0.008 min
Response: 1413312
Conc: 10.83 ug/ml

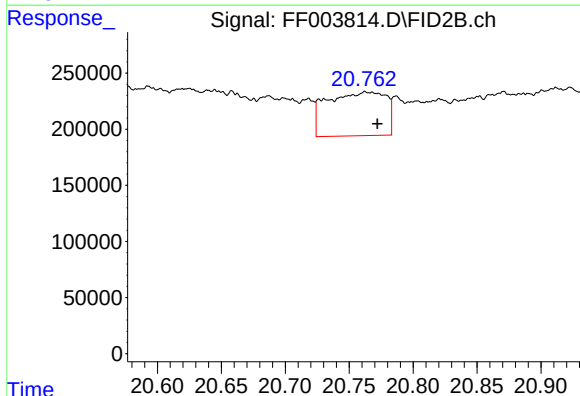

#17 N-OCTATRIACONTANE

R.T.: 20.763 min
Delta R.T.: -0.010 min
Response: 1247574
Conc: 10.80 ug/ml

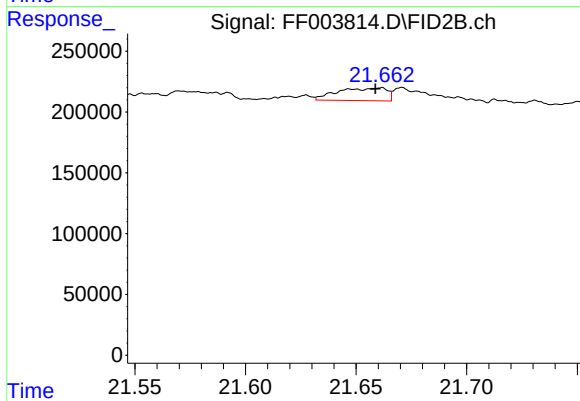

#18 N-TETRACONTANE

R.T.: 21.661 min
Delta R.T.: 0.002 min
Response: 161980
Conc: 1.30 ug/ml