

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
 Data File : FF003815.D
 Signal(s) : FID2B.ch
 Acq On : 13 Mar 2019 12:31
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 14 01:00:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.591	2046470	14.699 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.660	268394	1.825 ug/ml
14) N-DOTRIACONTANE	18.497	229459	1.614 ug/ml
15) N-TETRATRIACONTANE	19.295	146296	1.093 ug/ml
16) N-HEXATRIACONTANE	20.071	690716	5.294 ug/ml
18) N-TETRACONTANE	21.676	336404	2.704 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
Data File : FF003815.D
Signal(s) : FID2B.ch
Acq On : 13 Mar 2019 12:31
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 14 01:00:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

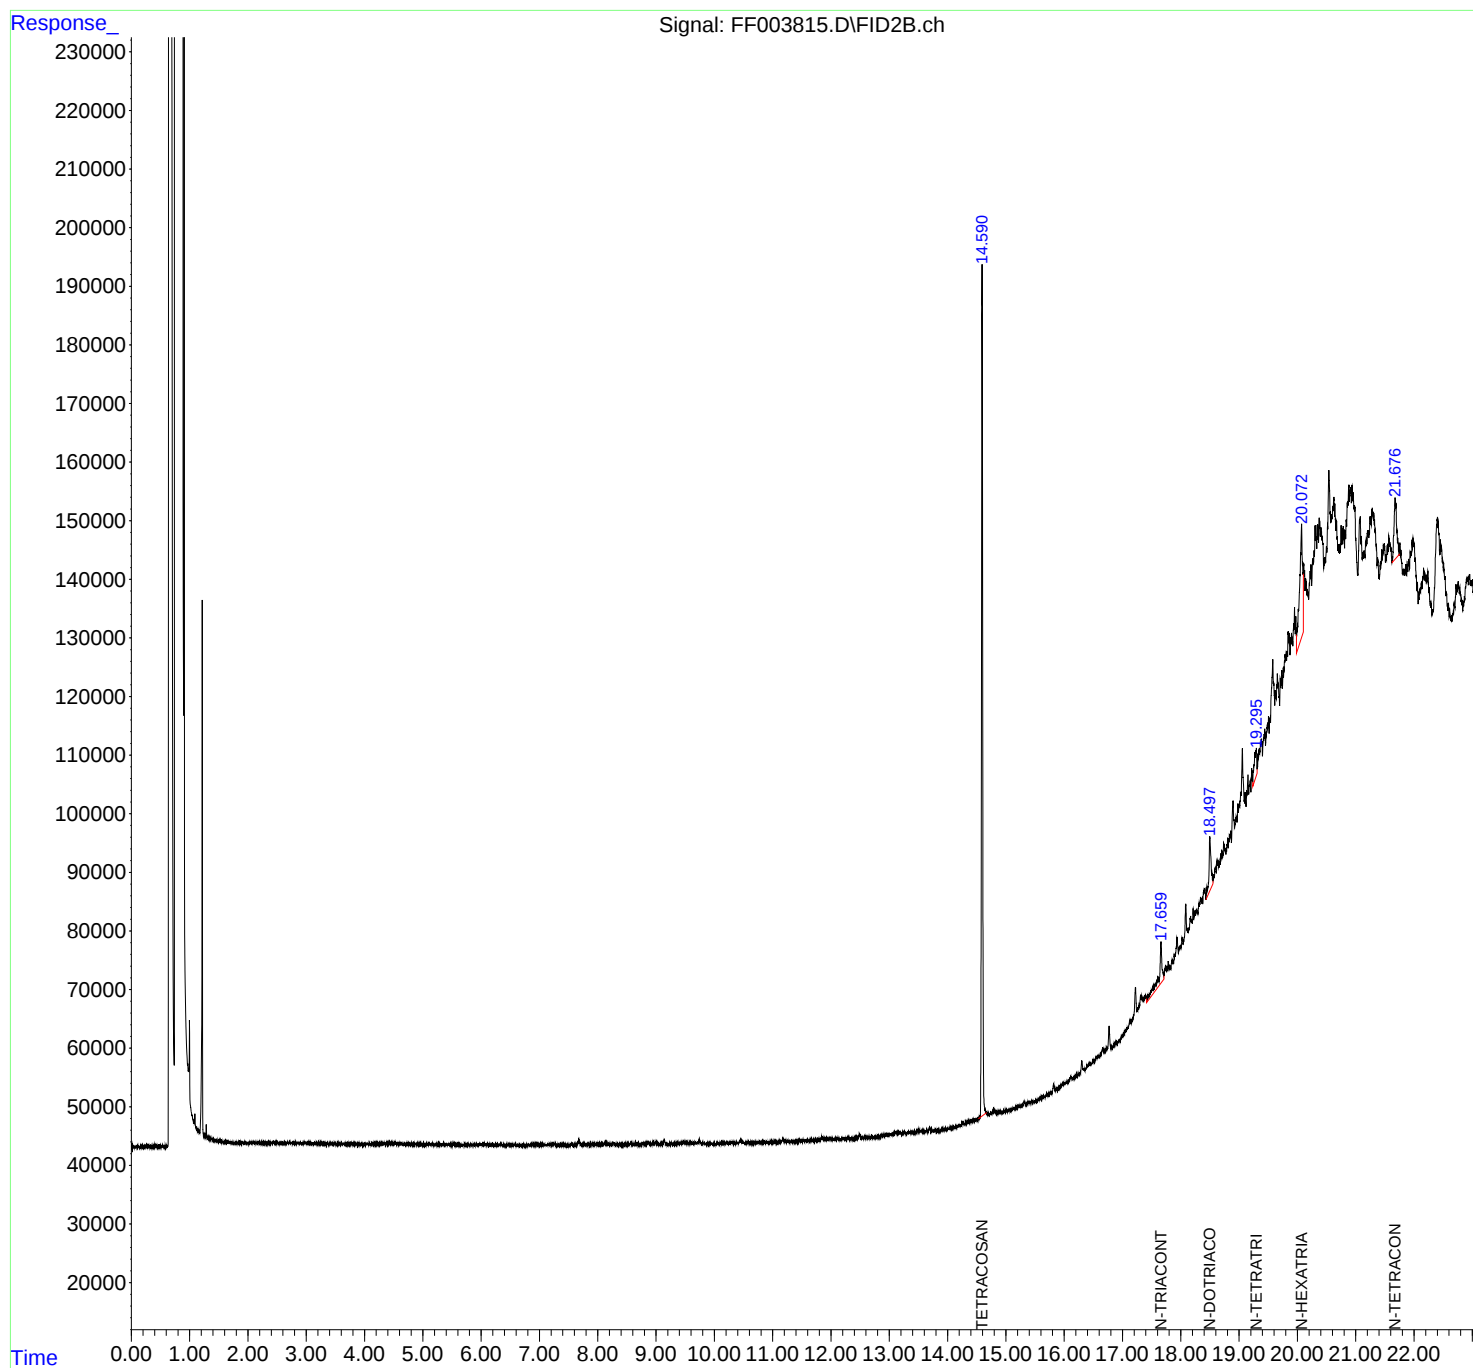


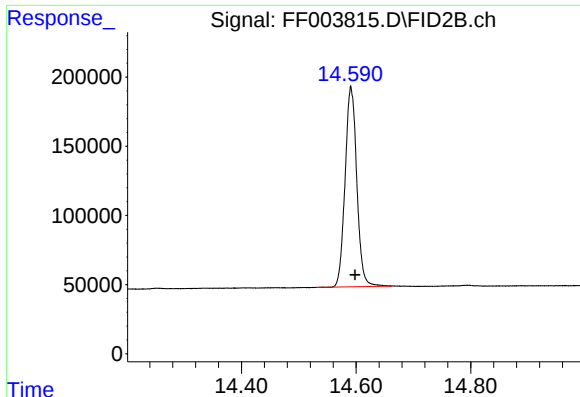

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.591 min
Delta R.T.: -0.007 min
Response: 2046470
Conc: 14.70 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

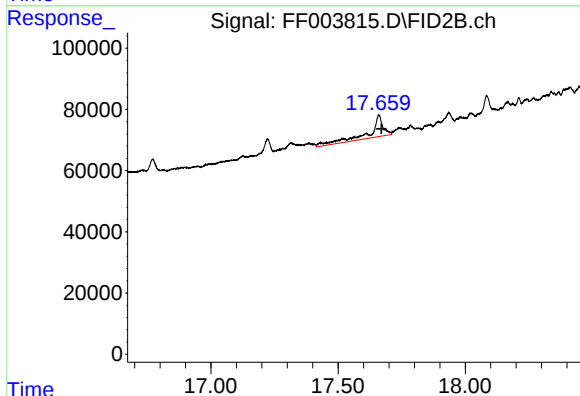


#13 N-TRIACONTANE

R.T.: 17.660 min
Delta R.T.: -0.010 min
Response: 268394
Conc: 1.82 ug/ml

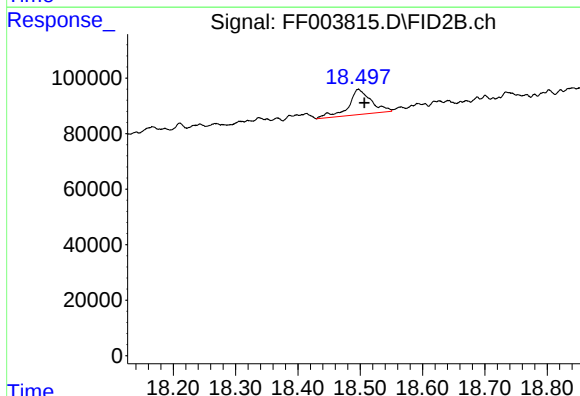


#14 N-DOTRIACONTANE

R.T.: 18.497 min
Delta R.T.: -0.009 min
Response: 229459
Conc: 1.61 ug/ml

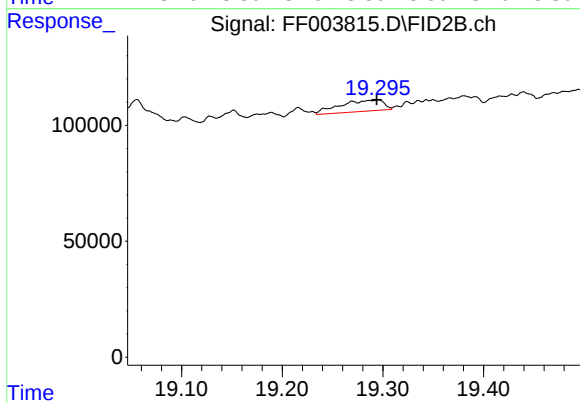

#15 N-TETRATRIACONTANE


R.T.: 19.295 min
Delta R.T.: 0.000 min
Response: 146296
Conc: 1.09 ug/ml

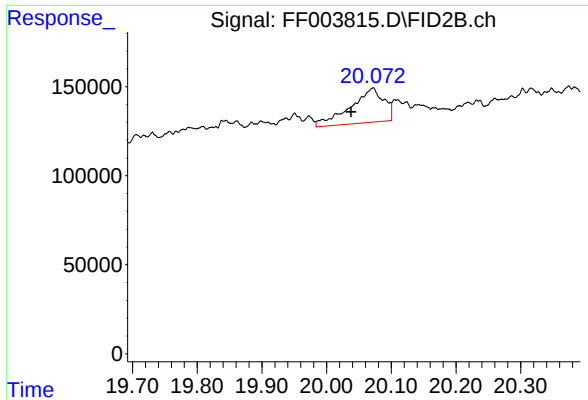

#16 N-HEXATRIACONTANE

R.T.: 20.071 min
Delta R.T.: 0.033 min
Response: 690716
Conc: 5.29 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

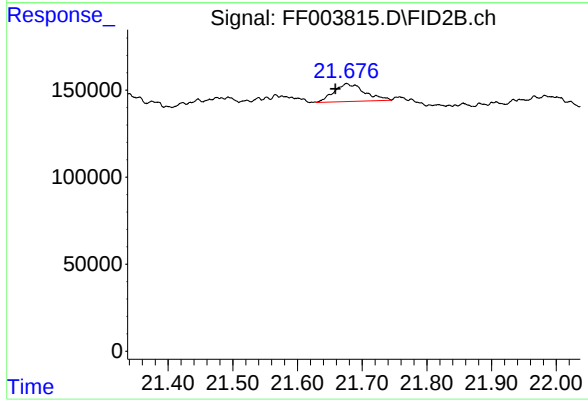

#18 N-TETRACONTANE

R.T.: 21.676 min
Delta R.T.: 0.017 min
Response: 336404
Conc: 2.70 ug/ml