

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
 Data File : FF003822.D
 Signal(s) : FID2B.ch
 Acq On : 13 Mar 2019 18:19
 Operator : AJ\SJ
 Sample : K1866-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 MR-MH-03-COMP

Integration File: autoint1.e
 Quant Time: Mar 14 01:04:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.588	1198721	8.610 ug/ml
Target Compounds			
4) N-TETRADECANE	8.192f	116984	0.730 ug/ml
7) N-EICOSANE	12.542	455095	2.782 ug/ml
10) N-TETRACOSANE	14.769	340908	2.155 ug/ml
11) N-HEXACOSANE	15.815	155916	1.010 ug/ml
12) N-OCTACOSANE	16.769	301605	1.996 ug/ml
13) N-TRIACONTANE	17.658	291591	1.982 ug/ml
14) N-DOTRIACONTANE	18.492	325307	2.288 ug/ml
16) N-HEXATRIACONTANE	20.070	170647	1.308 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
Data File : FF003822.D
Signal(s) : FID2B.ch
Acq On : 13 Mar 2019 18:19
Operator : AJ\SJ
Sample : K1866-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MR-MH-03-COMP

Integration File: autoint1.e
Quant Time: Mar 14 01:04:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

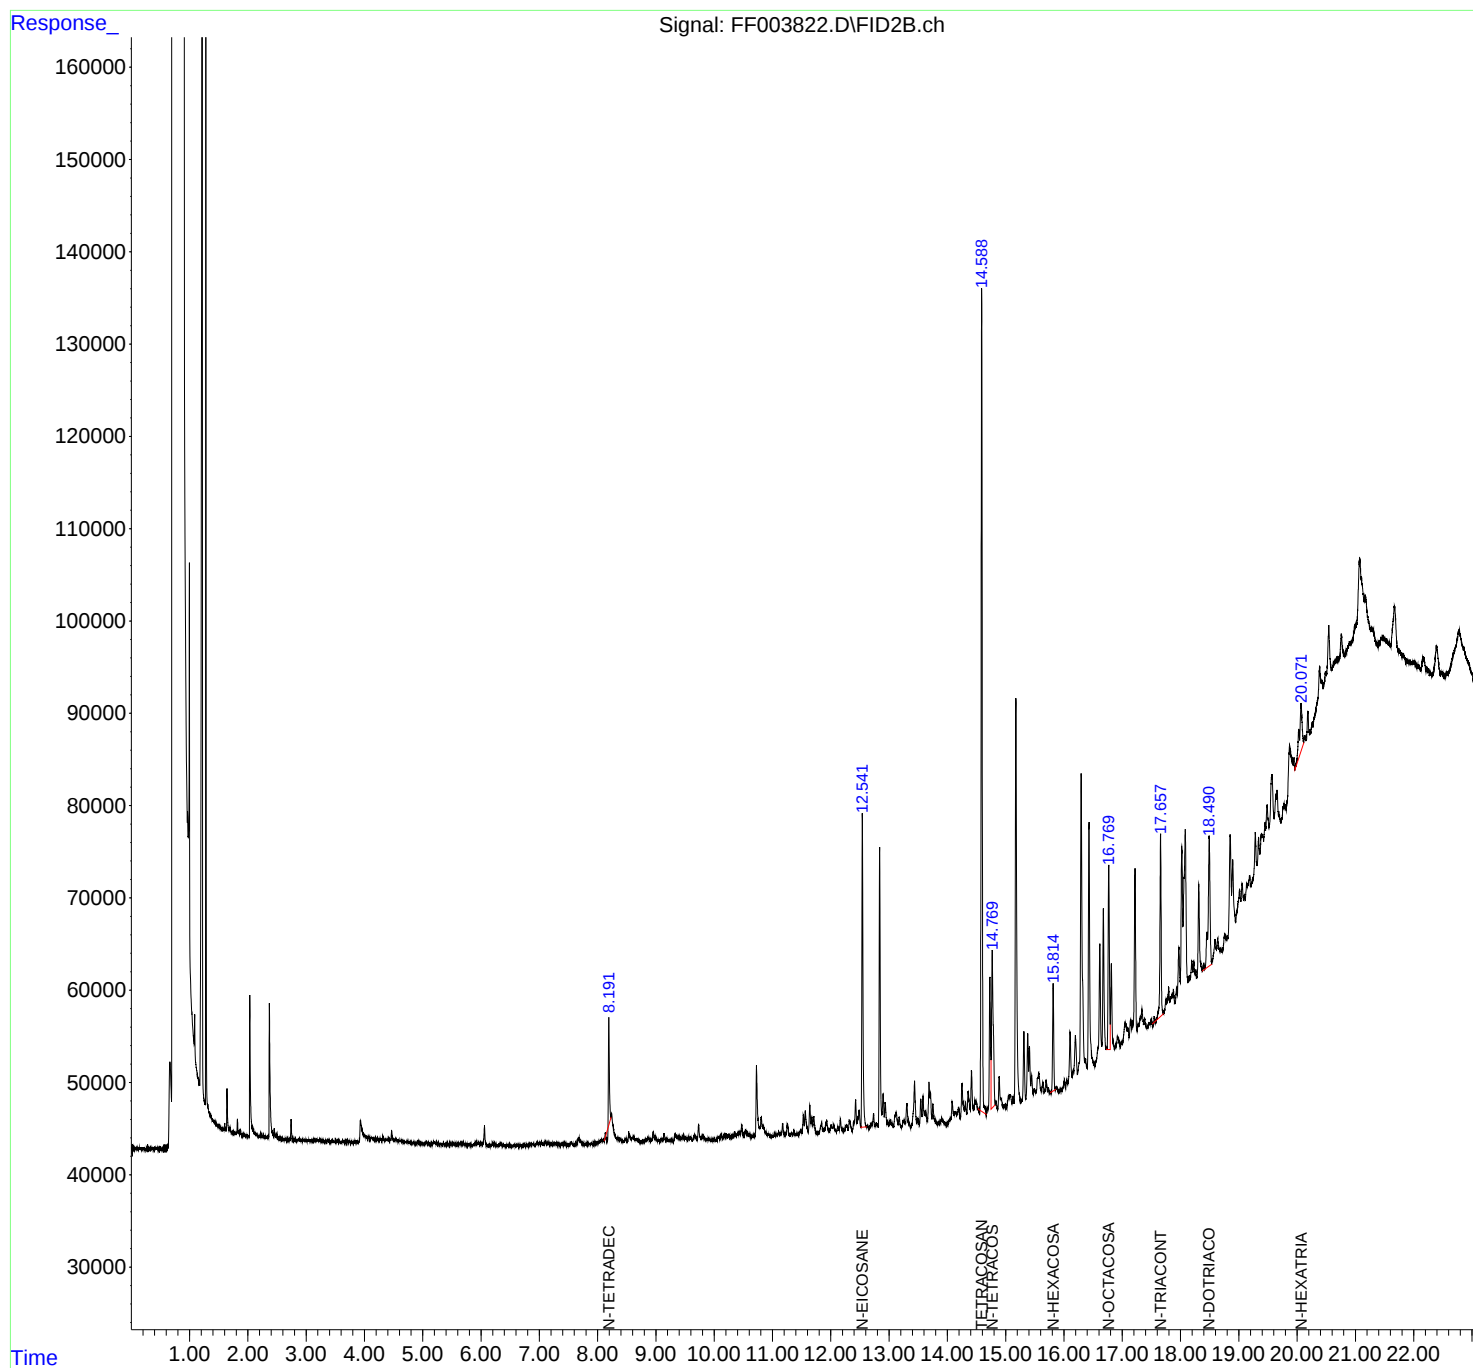


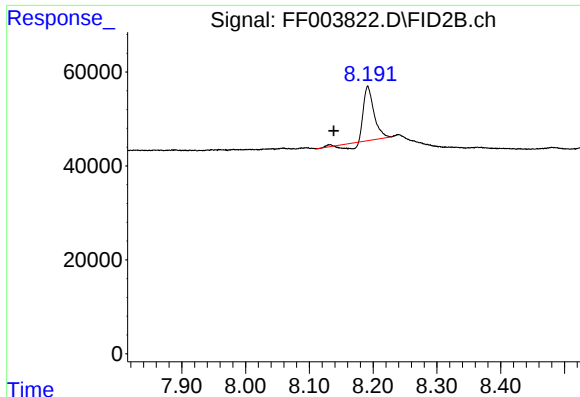

#4 N-TETRADECANE


R.T.: 8.192 min
Delta R.T.: 0.054 min
Response: 116984
Conc: 0.73 ug/ml

Instrument :
FID_F
ClientSampleId :
MR-MH-03-COMP

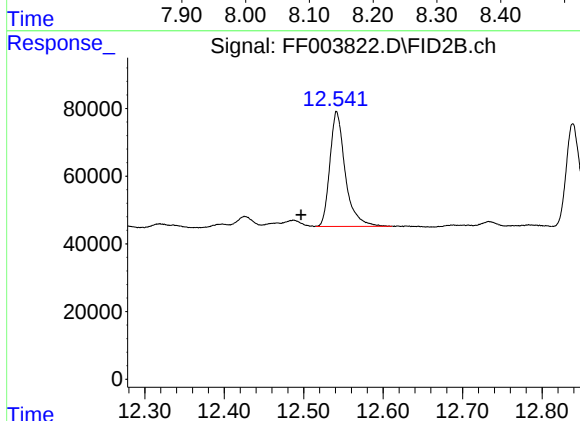


#7 N-EICOSANE

R.T.: 12.542 min
Delta R.T.: 0.045 min
Response: 455095
Conc: 2.78 ug/ml

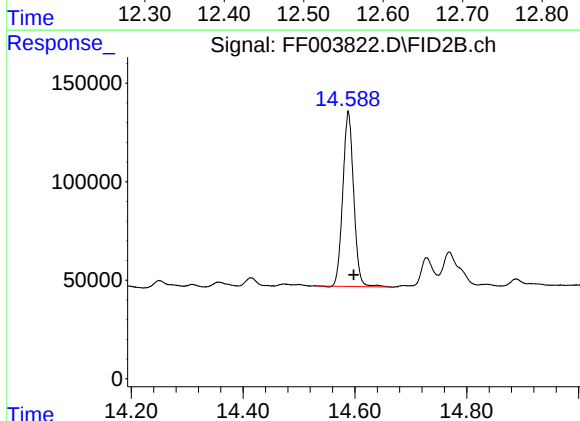


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.588 min
Delta R.T.: -0.010 min
Response: 1198721
Conc: 8.61 ug/ml

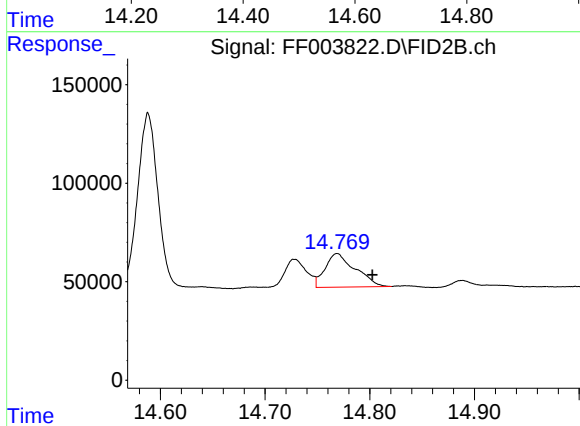

#10 N-TETRACOSANE


R.T.: 14.769 min
Delta R.T.: -0.034 min
Response: 340908
Conc: 2.15 ug/ml

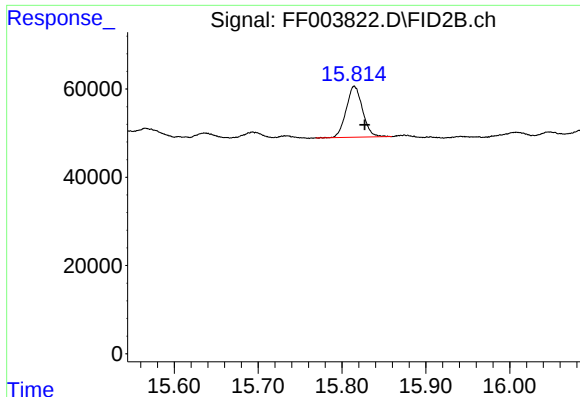

#11 N-HEXACOSANE


R.T.: 15.815 min
Delta R.T.: -0.012 min
Response: 155916
Conc: 1.01 ug/ml

Instrument :
FID_F
ClientSampleId :
MR-MH-03-COMP

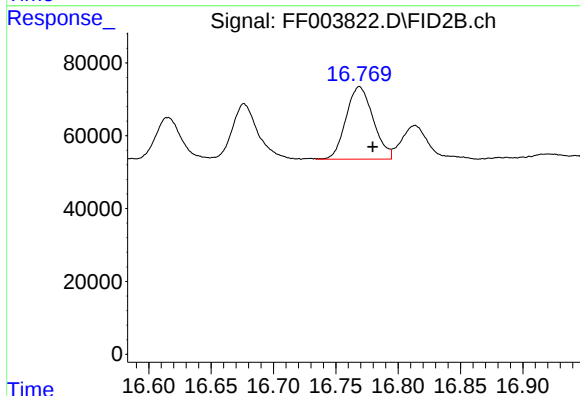


#12 N-OCTACOSANE

R.T.: 16.769 min
Delta R.T.: -0.011 min
Response: 301605
Conc: 2.00 ug/ml

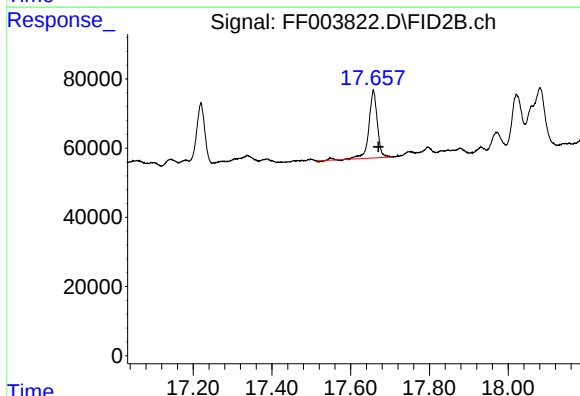


#13 N-TRIACONTANE

R.T.: 17.658 min
Delta R.T.: -0.013 min
Response: 291591
Conc: 1.98 ug/ml

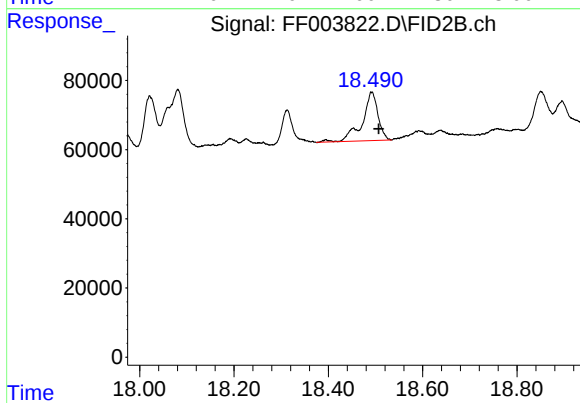

#14 N-DOTRIACONTANE

R.T.: 18.492 min
Delta R.T.: -0.015 min
Response: 325307
Conc: 2.29 ug/ml

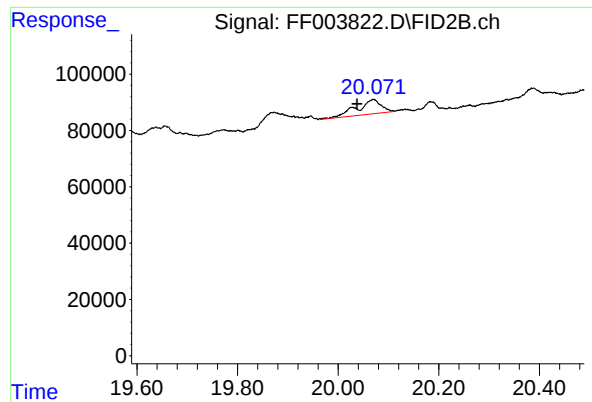

#16 N-HEXATRIACONTANE

R.T.: 20.070 min
Delta R.T.: 0.032 min
Response: 170647
Conc: 1.31 ug/ml

Instrument :
FID_F
ClientSampleId :
MR-MH-03-COMP