

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
 Data File : FF003824.D
 Signal(s) : FID2B.ch
 Acq On : 13 Mar 2019 19:20
 Operator : AJ\SJ
 Sample : K1866-07
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 MR-MH-01-COMP

Integration File: autoint1.e
 Quant Time: Mar 14 01:05:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.588	1508349	10.834 ug/ml
Target Compounds			
4) N-TETRADECANE	8.192f	314799	1.963 ug/ml
11) N-HEXACOSANE	15.816	122783	0.796 ug/ml
12) N-OCTACOSANE	16.769	278558	1.843 ug/ml
13) N-TRIACONTANE	17.659	308007	2.094 ug/ml
14) N-DOTRIACONTANE	18.491	359534	2.528 ug/ml
15) N-TETRATRIACONTANE	19.339	53783	0.402 ug/ml
16) N-HEXATRIACONTANE	20.068	152026	1.165 ug/ml
18) N-TETRACONTANE	21.633	101356	0.815 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
Data File : FF003824.D
Signal(s) : FID2B.ch
Acq On : 13 Mar 2019 19:20
Operator : AJ\SJ
Sample : K1866-07
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MR-MH-01-COMP

Integration File: autoint1.e
Quant Time: Mar 14 01:05:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

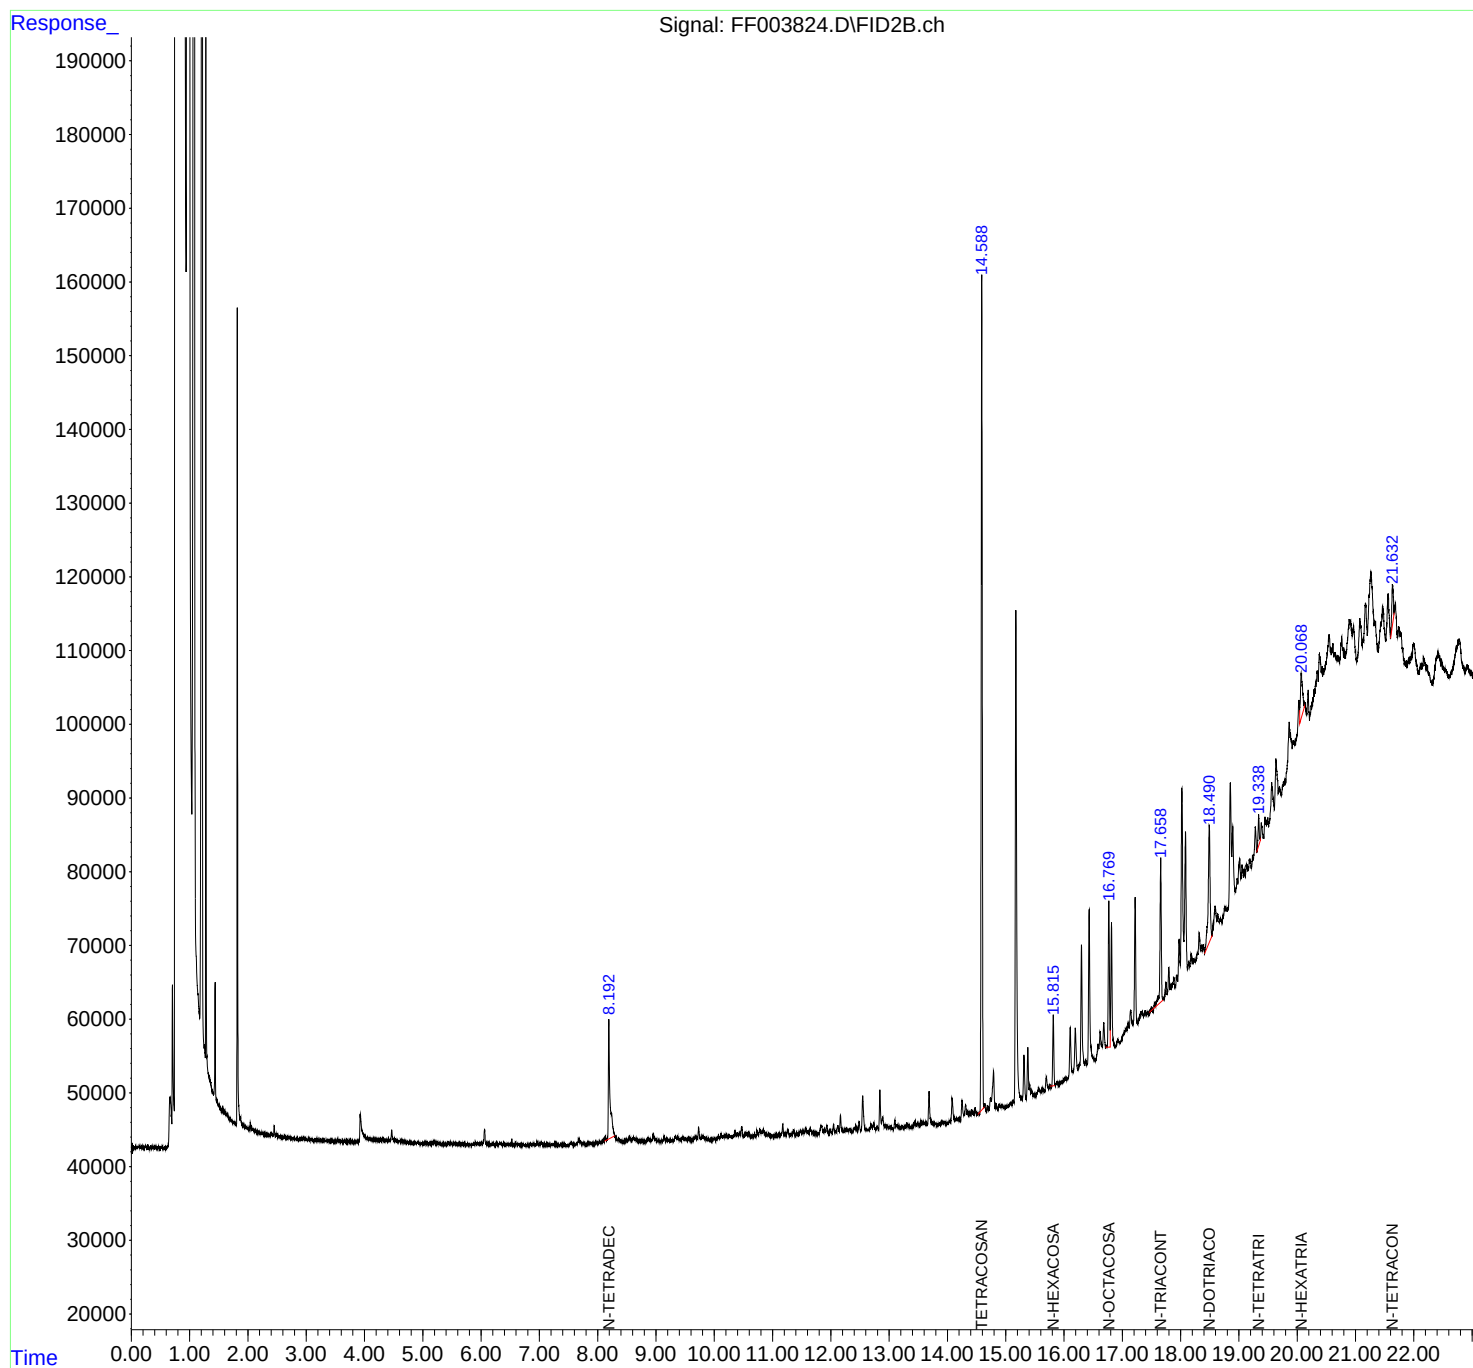


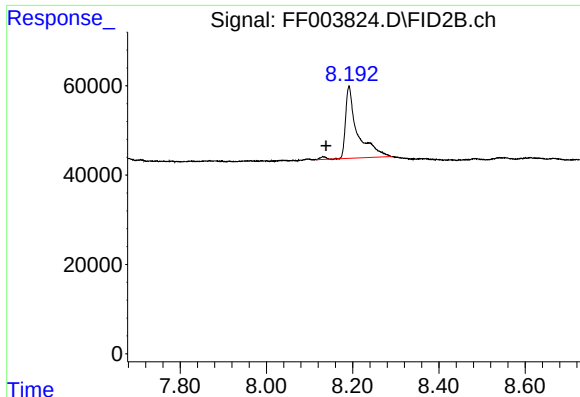

#4 N-TETRADECANE


R.T.: 8.192 min
Delta R.T.: 0.053 min
Response: 314799
Conc: 1.96 ug/ml

Instrument :
FID_F
ClientSampleId :
MR-MH-01-COMP

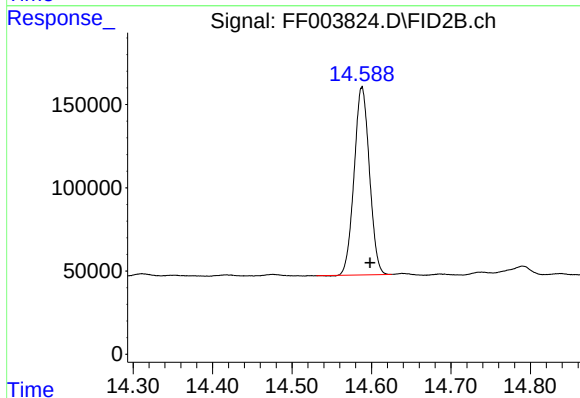


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.588 min
Delta R.T.: -0.010 min
Response: 1508349
Conc: 10.83 ug/ml

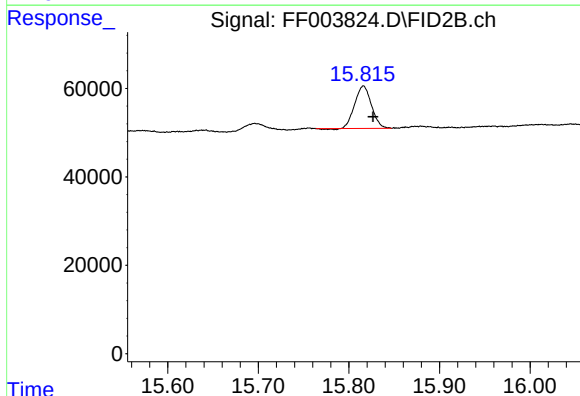


#11 N-HEXACOSANE

R.T.: 15.816 min
Delta R.T.: -0.011 min
Response: 122783
Conc: 0.80 ug/ml

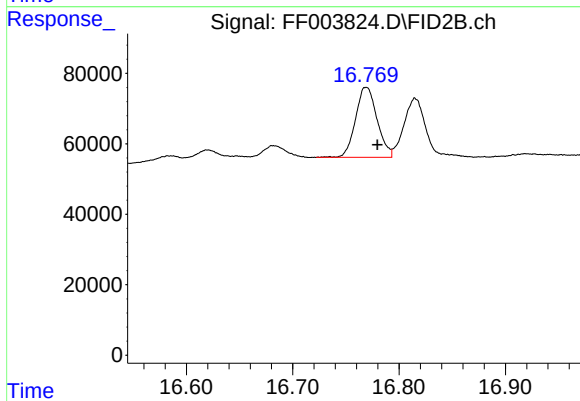

#12 N-OCTACOSANE


R.T.: 16.769 min
Delta R.T.: -0.011 min
Response: 278558
Conc: 1.84 ug/ml

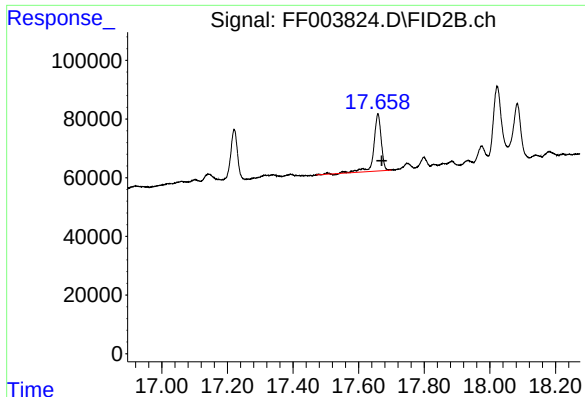

#13 N-TRIACONTANE


R.T.: 17.659 min
Delta R.T.: -0.012 min
Response: 308007
Conc: 2.09 ug/ml

Instrument :
FID_F
ClientSampleId :
MR-MH-01-COMP

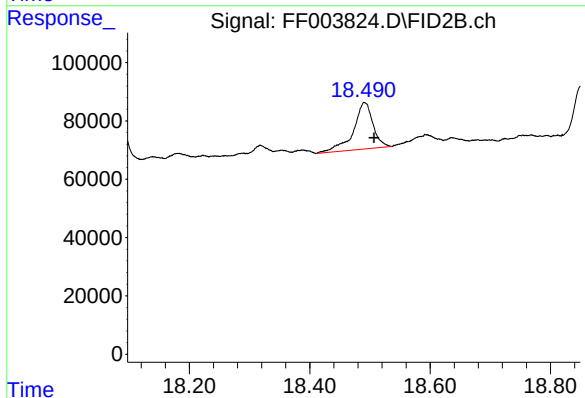


#14 N-DOTRIACONTANE

R.T.: 18.491 min
Delta R.T.: -0.016 min
Response: 359534
Conc: 2.53 ug/ml

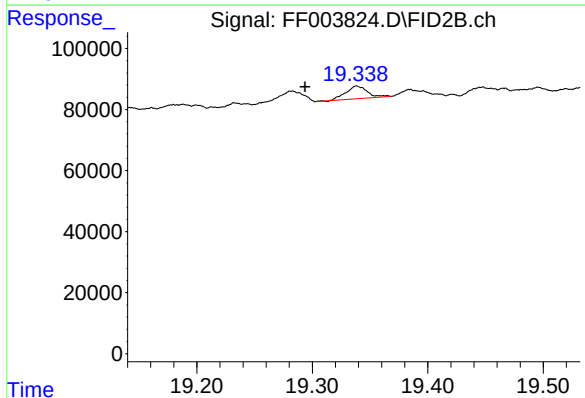


#15 N-TETRATRIACONTANE

R.T.: 19.339 min
Delta R.T.: 0.045 min
Response: 53783
Conc: 0.40 ug/ml

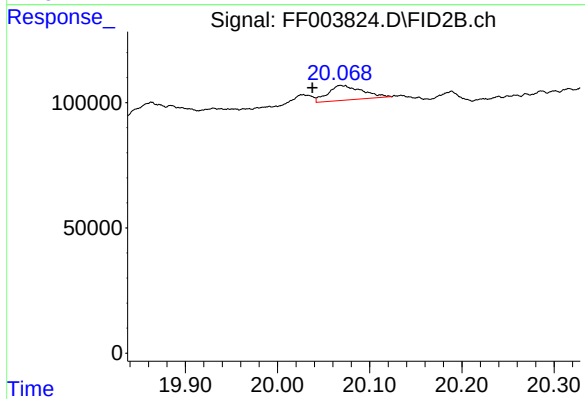

#16 N-HEXATRIACONTANE

R.T.: 20.068 min
Delta R.T.: 0.030 min
Response: 152026
Conc: 1.17 ug/ml

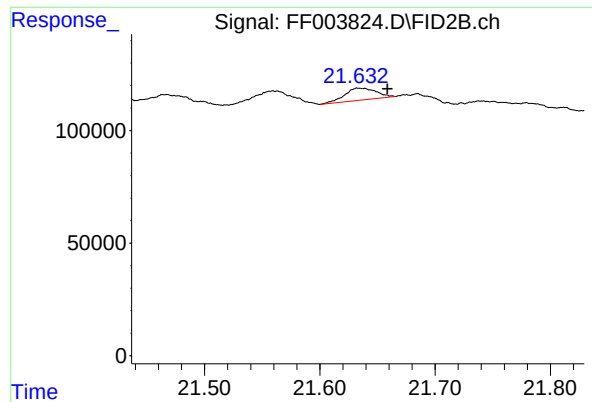

#18 N-TETRACONTANE

R.T.: 21.633 min
Delta R.T.: -0.025 min
Response: 101356
Conc: 0.81 ug/ml

Instrument :
FID_F
ClientSampleId :
MR-MH-01-COMP