

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
 Data File : FF003825.D
 Signal(s) : FID2B.ch
 Acq On : 13 Mar 2019 19:51
 Operator : AJ\SJ
 Sample : K1866-09
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 MR-MH-15-COMP

Integration File: autoint1.e
 Quant Time: Mar 14 01:05:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.589	1565407	11.243 ug/ml
Target Compounds			
4) N-TETRADECANE	8.190f	220833	1.377 ug/ml
7) N-EICOSANE	12.541	415697	2.541 ug/ml
10) N-TETRACOSANE	14.769	283297	1.791 ug/ml
11) N-HEXACOSANE	15.816	139383	0.903 ug/ml
12) N-OCTACOSANE	16.769	267708	1.772 ug/ml
13) N-TRIACONTANE	17.660	317852	2.161 ug/ml
14) N-DOTRIACONTANE	18.492	646379	4.545 ug/ml
15) N-TETRATRIACONTANE	19.339	165565	1.237 ug/ml
16) N-HEXATRIACONTANE	20.066	144675	1.109 ug/ml
18) N-TETRACONTANE	21.666	213593	1.717 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
Data File : FF003825.D
Signal(s) : FID2B.ch
Acq On : 13 Mar 2019 19:51
Operator : AJ\SJ
Sample : K1866-09
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MR-MH-15-COMP

Integration File: autoint1.e
Quant Time: Mar 14 01:05:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

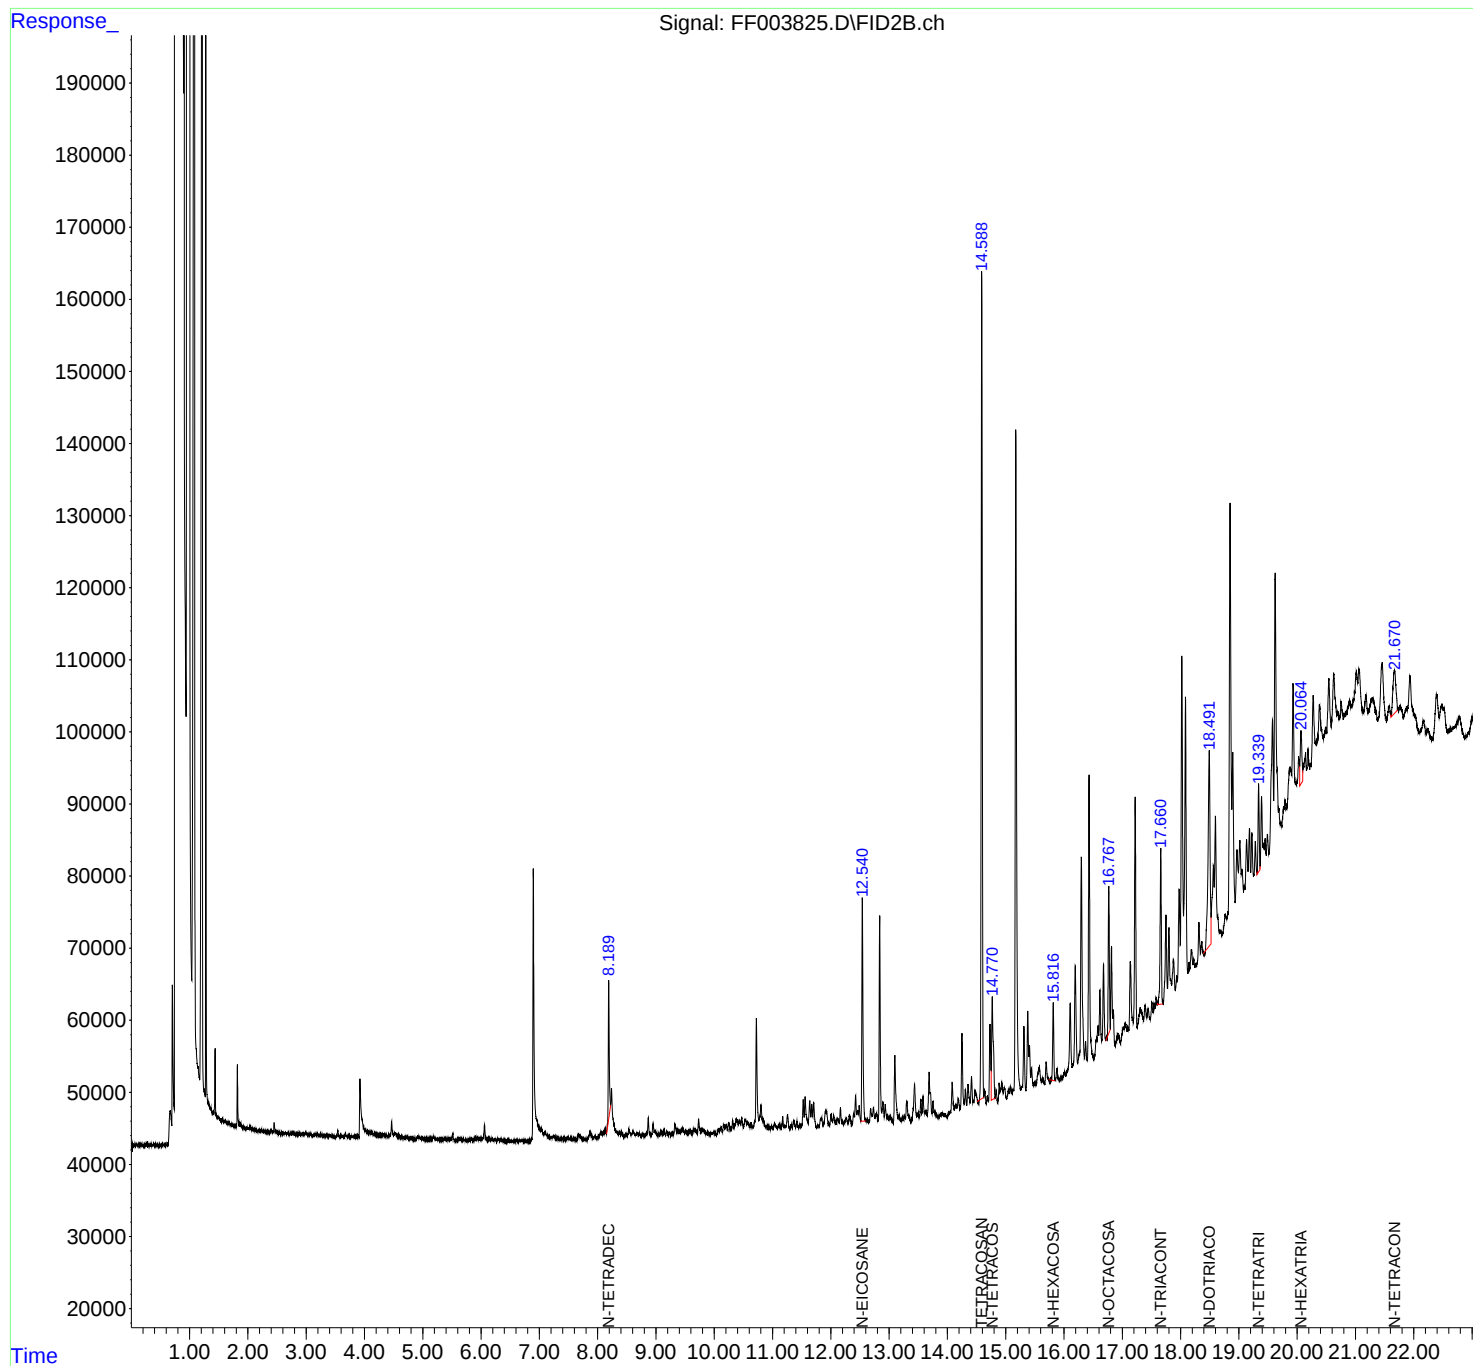


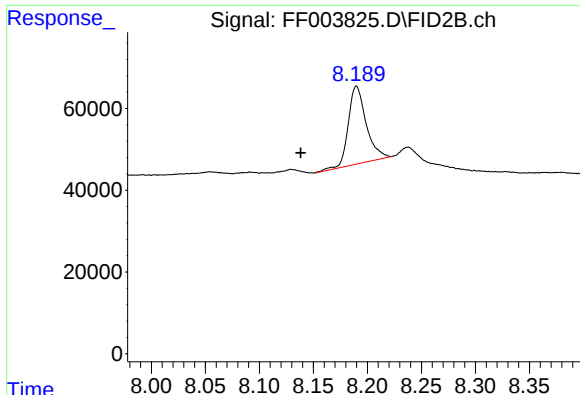

#4 N-TETRADECANE


R.T.: 8.190 min
Delta R.T.: 0.052 min
Response: 220833
Conc: 1.38 ug/ml

Instrument :
FID_F
ClientSampleId :
MR-MH-15-COMP

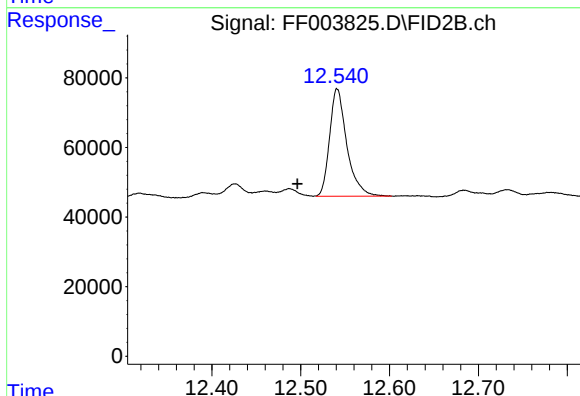


#7 N-EICOSANE

R.T.: 12.541 min
Delta R.T.: 0.045 min
Response: 415697
Conc: 2.54 ug/ml

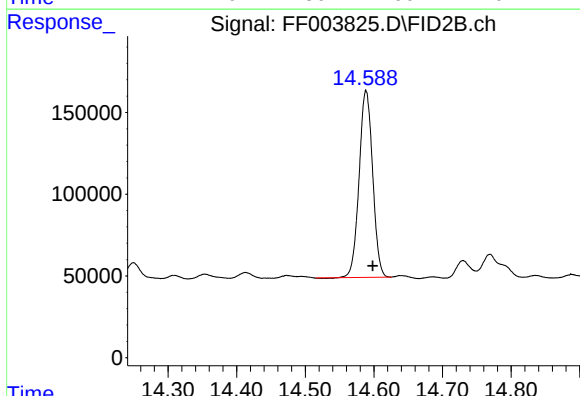


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.589 min
Delta R.T.: -0.010 min
Response: 1565407
Conc: 11.24 ug/ml

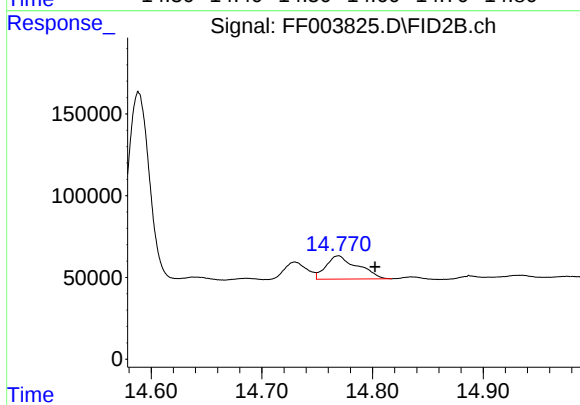

#10 N-TETRACOSANE


R.T.: 14.769 min
Delta R.T.: -0.033 min
Response: 283297
Conc: 1.79 ug/ml

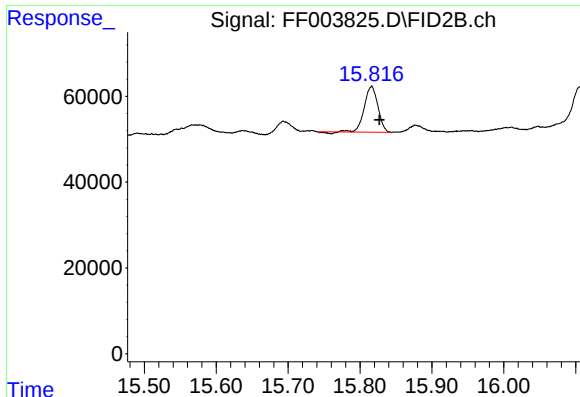

#11 N-HEXACOSANE


R.T.: 15.816 min
Delta R.T.: -0.011 min
Response: 139383
Conc: 0.90 ug/ml

Instrument :
FID_F
ClientSampleId :
MR-MH-15-COMP

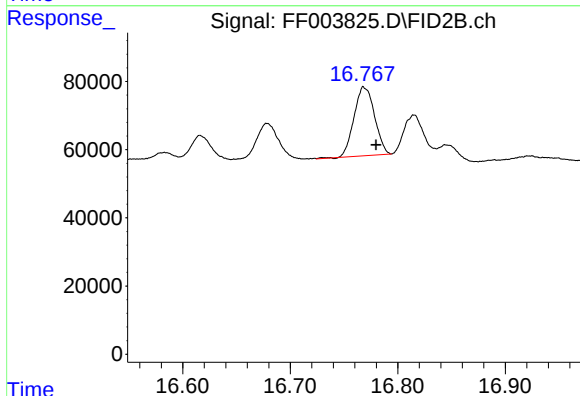


#12 N-OCTACOSANE

R.T.: 16.769 min
Delta R.T.: -0.011 min
Response: 267708
Conc: 1.77 ug/ml

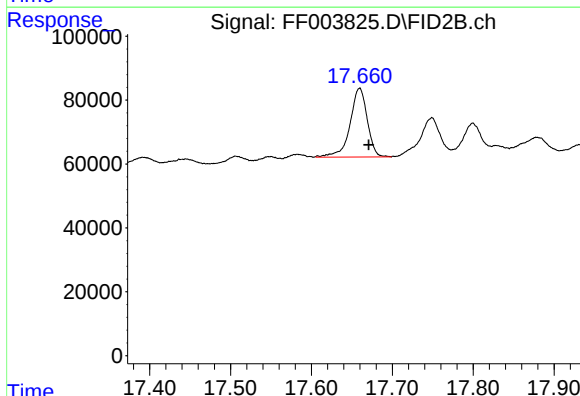


#13 N-TRIACONTANE

R.T.: 17.660 min
Delta R.T.: -0.011 min
Response: 317852
Conc: 2.16 ug/ml

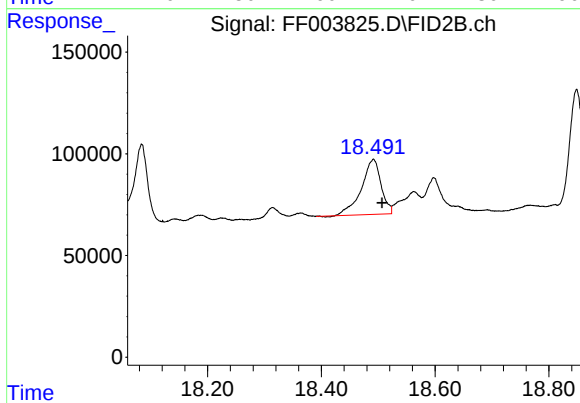

#14 N-DOTRIACONTANE


R.T.: 18.492 min
Delta R.T.: -0.015 min
Response: 646379
Conc: 4.55 ug/ml

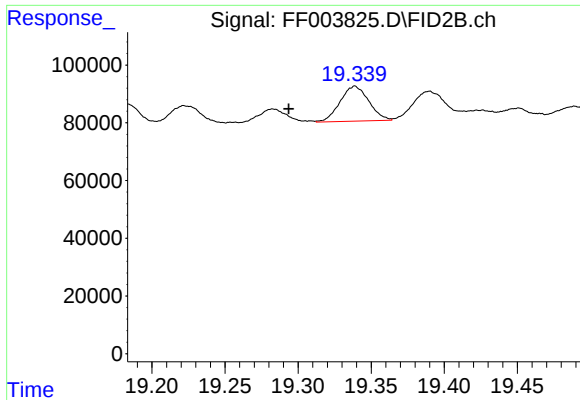

#15 N-TETRATRIACONTANE


R.T.: 19.339 min
Delta R.T.: 0.045 min
Response: 165565
Conc: 1.24 ug/ml

Instrument :
FID_F
ClientSampleId :
MR-MH-15-COMP

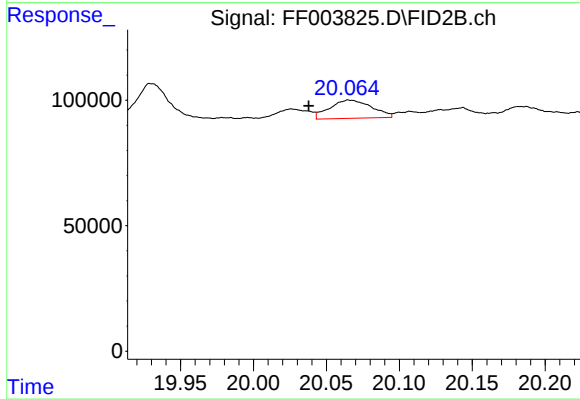

#16 N-HEXATRIACONTANE

R.T.: 20.066 min
Delta R.T.: 0.028 min
Response: 144675
Conc: 1.11 ug/ml

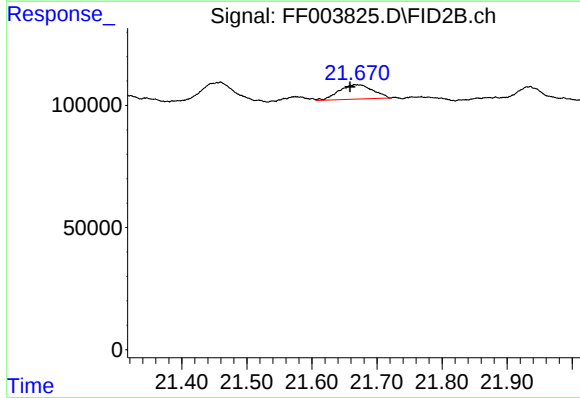

#18 N-TETRACONTANE

R.T.: 21.666 min
Delta R.T.: 0.007 min
Response: 213593
Conc: 1.72 ug/ml