

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
 Data File : FF003827.D
 Signal(s) : FID2B.ch
 Acq On : 13 Mar 2019 20:52
 Operator : AJ\SJ
 Sample : K1866-13
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 MR-MH-13-COMP

Integration File: autoint1.e
 Quant Time: Mar 14 01:05:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.590	1900258	13.649 ug/ml
Target Compounds			
4) N-TETRADECANE	8.191f	389264	2.428 ug/ml
11) N-HEXACOSANE	15.816	98326	0.637 ug/ml
12) N-OCTACOSANE	16.768	204499	1.353 ug/ml
13) N-TRIACONTANE	17.659	228777	1.555 ug/ml
14) N-DOTRIACONTANE	18.493	242782	1.707 ug/ml
16) N-HEXATRIACONTANE	20.067	622044	4.767 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
Data File : FF003827.D
Signal(s) : FID2B.ch
Acq On : 13 Mar 2019 20:52
Operator : AJ\SJ
Sample : K1866-13
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MR-MH-13-COMP

Integration File: autoint1.e
Quant Time: Mar 14 01:05:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

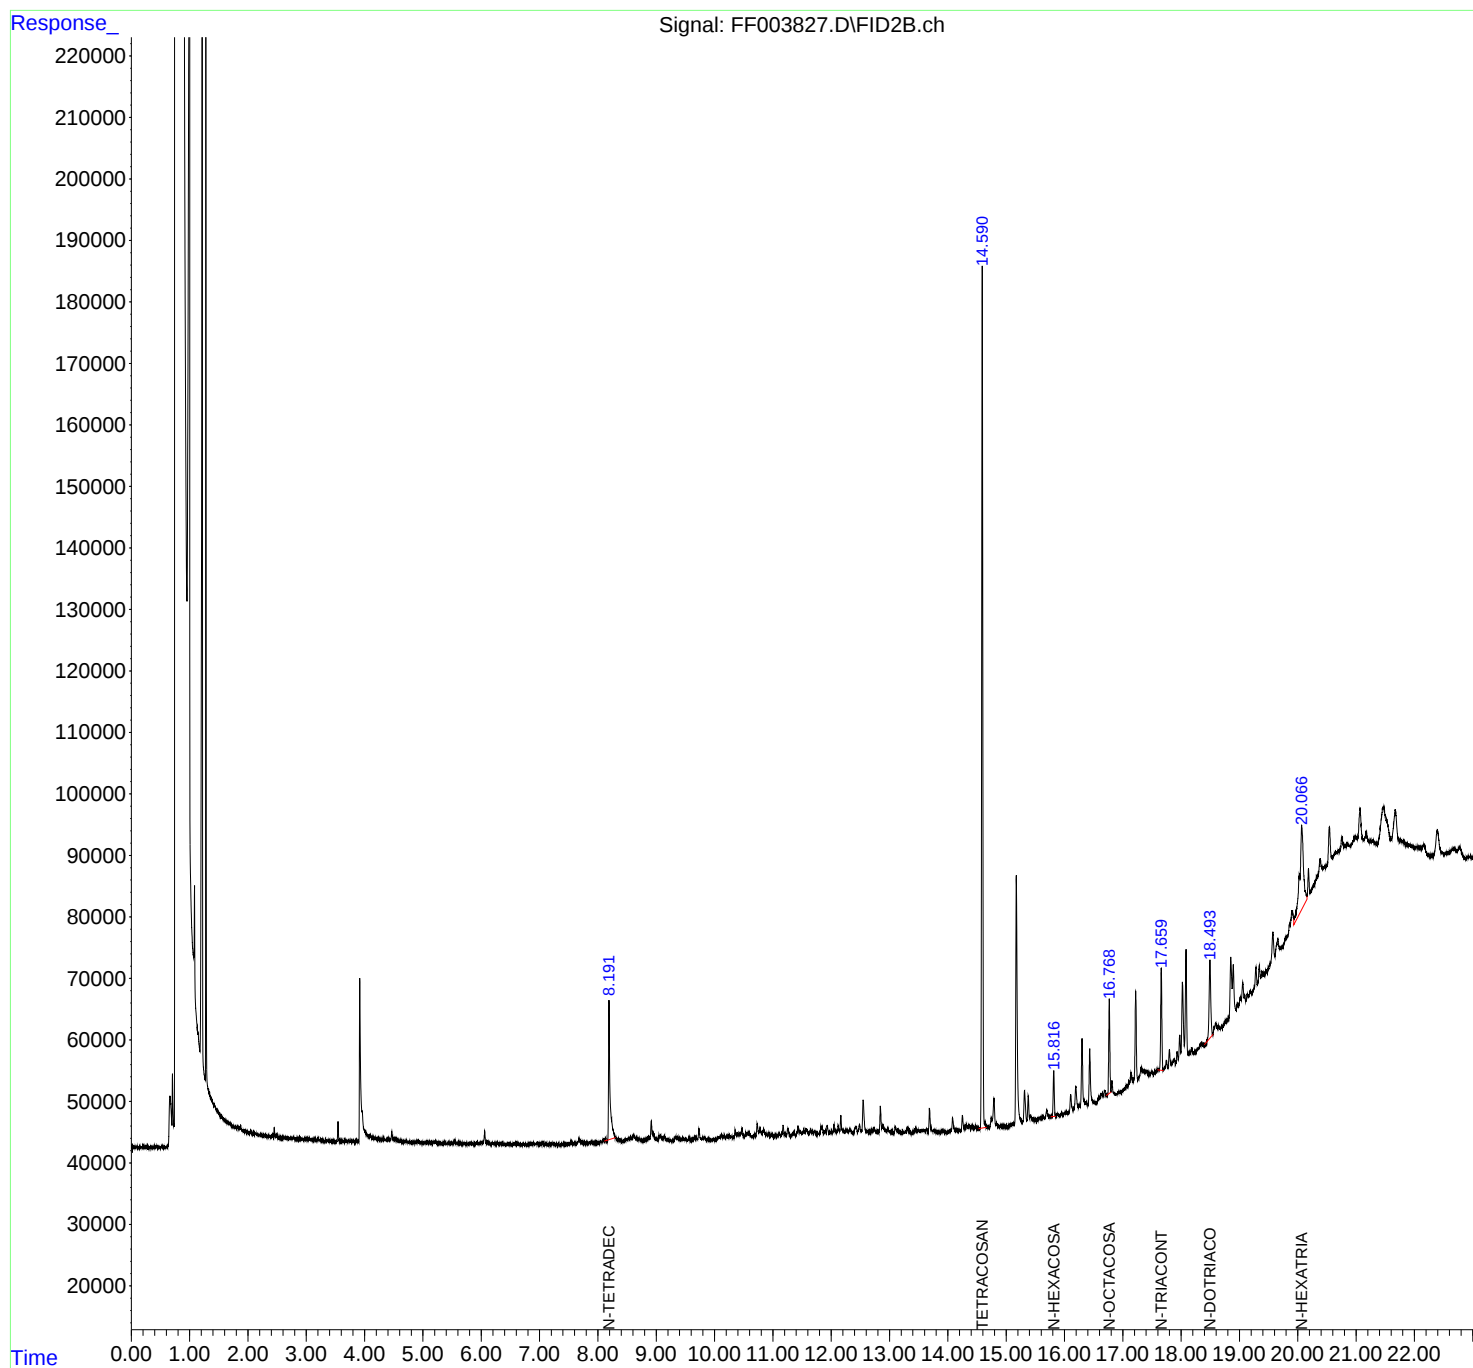


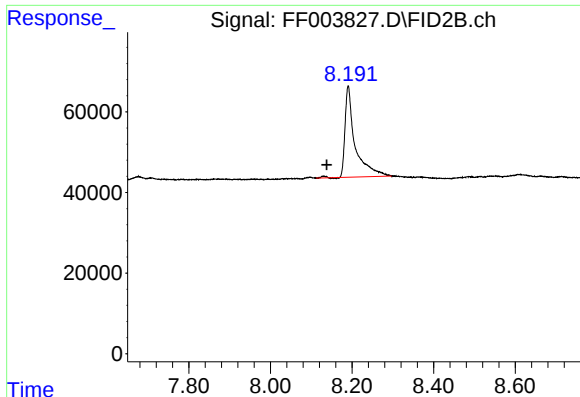

#4 N-TETRADECANE


R.T.: 8.191 min
Delta R.T.: 0.052 min
Response: 389264
Conc: 2.43 ug/ml

Instrument :
FID_F
ClientSampleId :
MR-MH-13-COMP

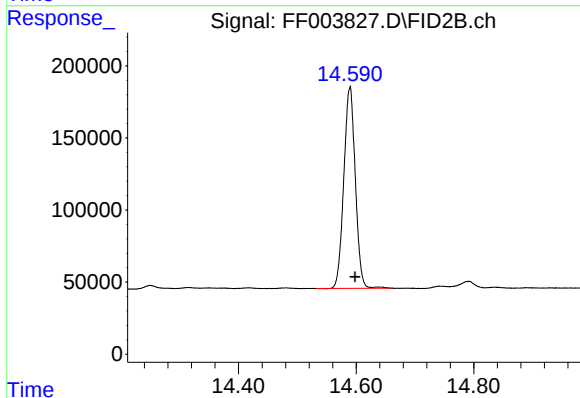


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.590 min
Delta R.T.: -0.009 min
Response: 1900258
Conc: 13.65 ug/ml

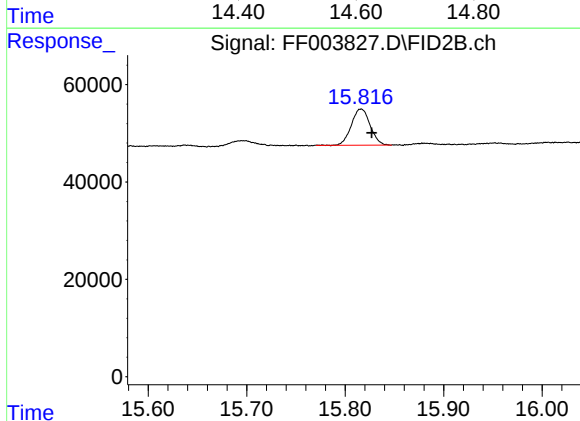


#11 N-HEXACOSANE

R.T.: 15.816 min
Delta R.T.: -0.011 min
Response: 98326
Conc: 0.64 ug/ml

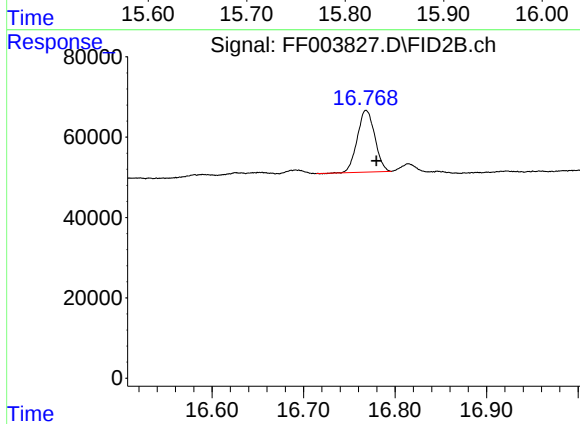

#12 N-OCTACOSANE


R.T.: 16.768 min
Delta R.T.: -0.011 min
Response: 204499
Conc: 1.35 ug/ml

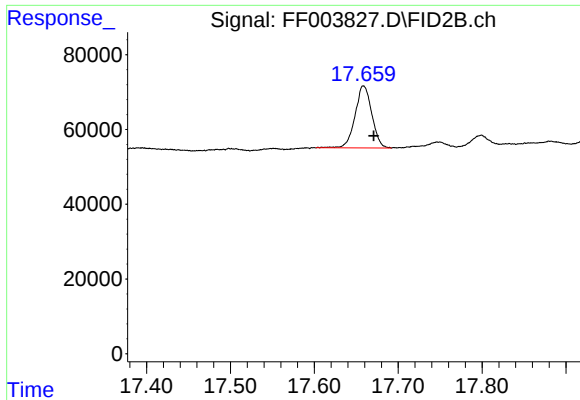

#13 N-TRIACONTANE


R.T.: 17.659 min
Delta R.T.: -0.012 min
Response: 228777
Conc: 1.56 ug/ml

Instrument :
FID_F
ClientSampleId :
MR-MH-13-COMP

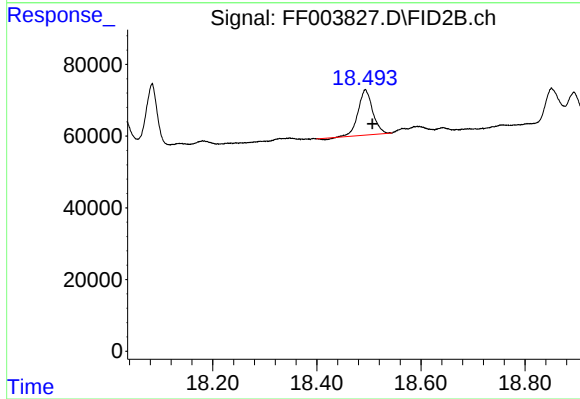

#14 N-DOTRIACONTANE

R.T.: 18.493 min
Delta R.T.: -0.014 min
Response: 242782
Conc: 1.71 ug/ml

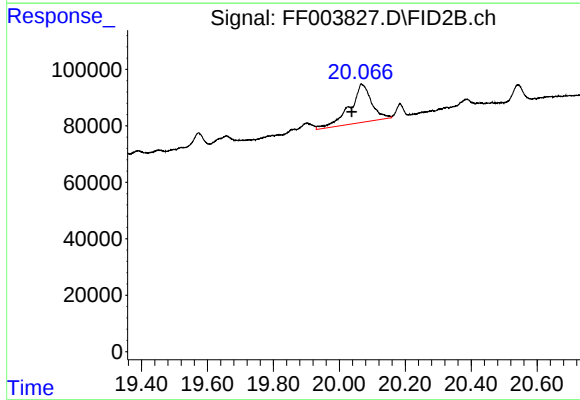

#16 N-HEXATRIACONTANE

R.T.: 20.067 min
Delta R.T.: 0.029 min
Response: 622044
Conc: 4.77 ug/ml