

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
 Data File : FF003829.D
 Signal(s) : FID2B.ch
 Acq On : 13 Mar 2019 21:53
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 14 01:05:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.589	2016738	14.485 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.660	107812	0.733 ug/ml
14) N-DOTRIACONTANE	18.495	209122	1.471 ug/ml
16) N-HEXATRIACONTANE	20.065	445237	3.412 ug/ml
18) N-TETRACONTANE	21.666	341399	2.744 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
Data File : FF003829.D
Signal(s) : FID2B.ch
Acq On : 13 Mar 2019 21:53
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 14 01:05:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

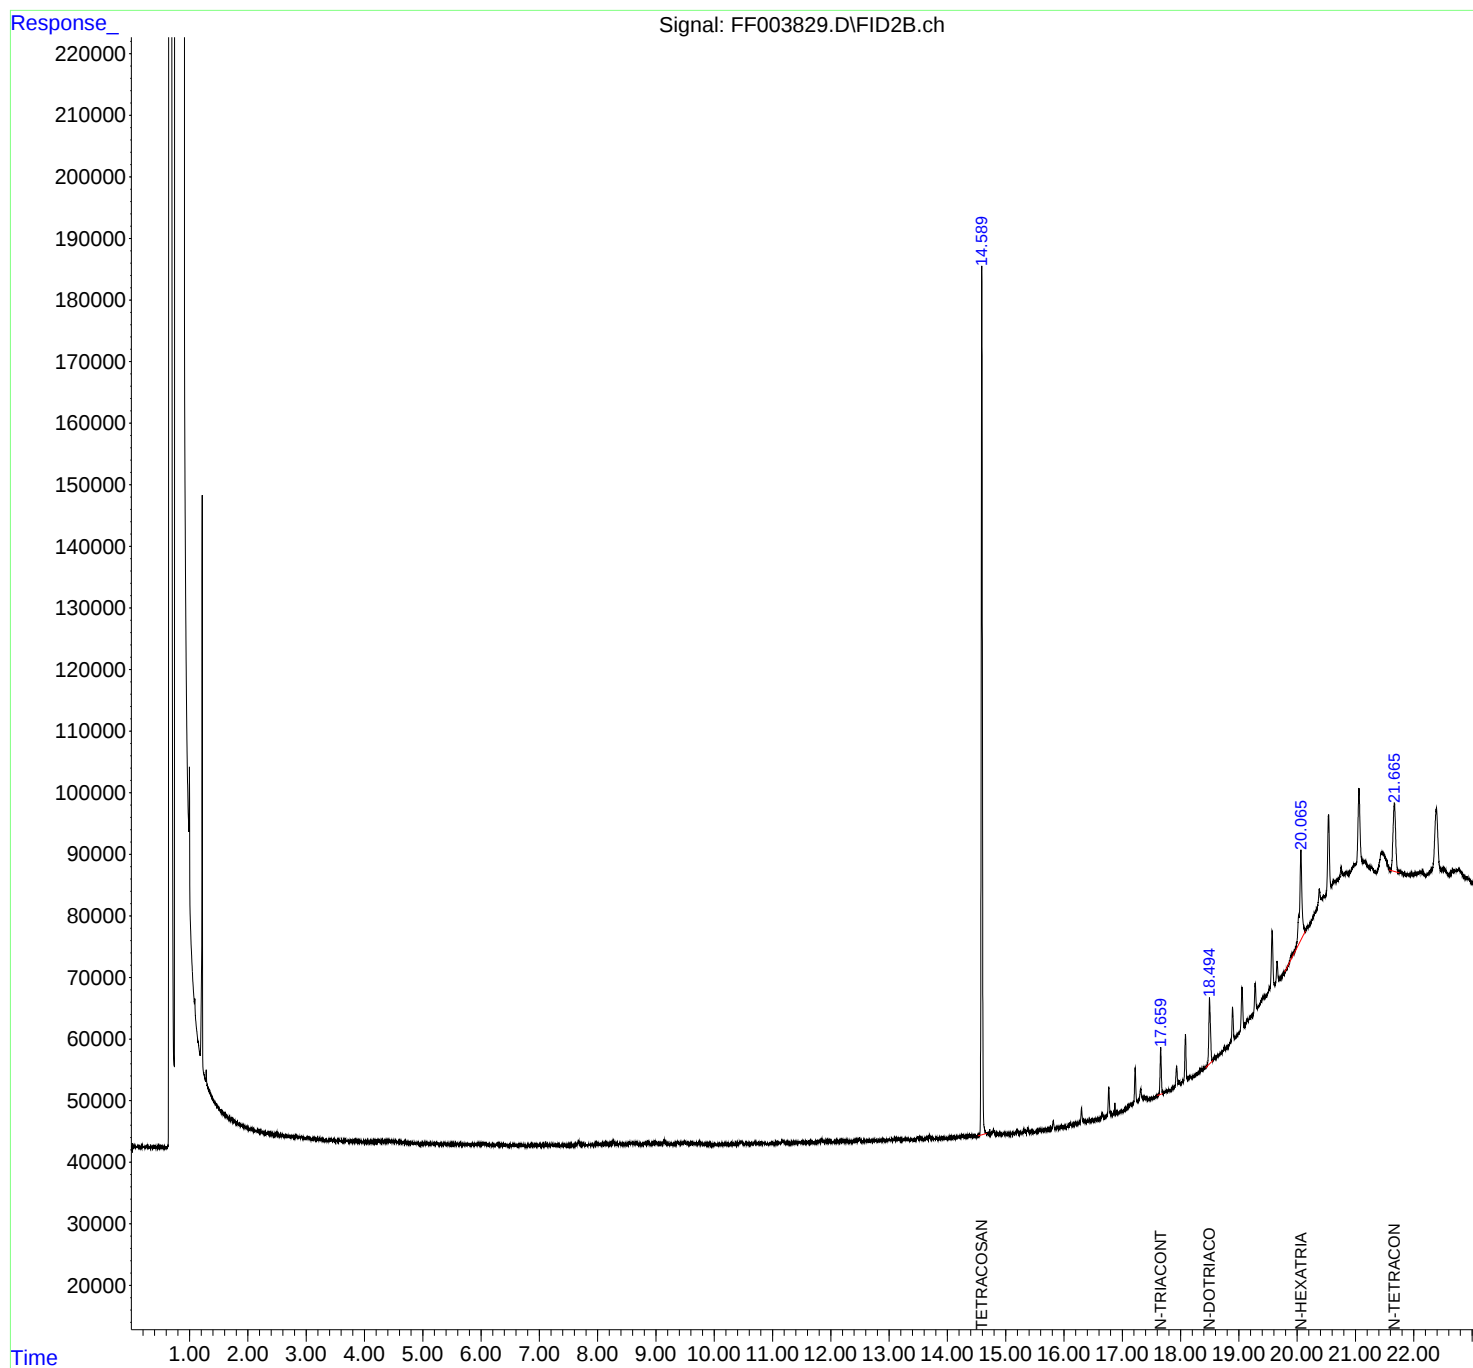


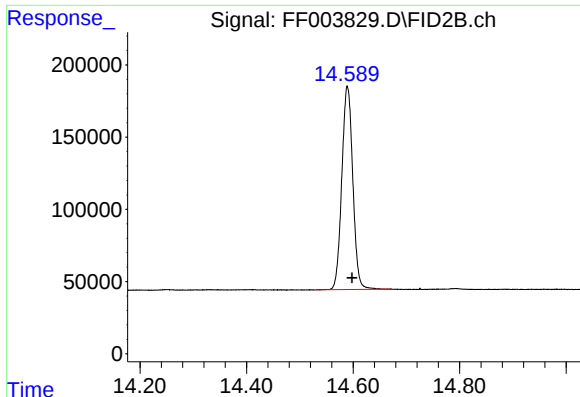

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.589 min
Delta R.T.: -0.009 min
Response: 2016738
Conc: 14.49 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

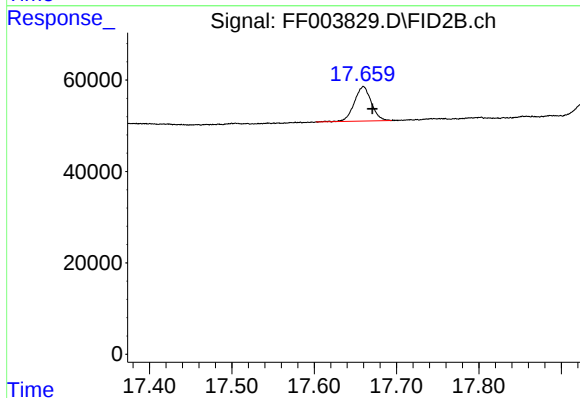


#13 N-TRIACONTANE

R.T.: 17.660 min
Delta R.T.: -0.011 min
Response: 107812
Conc: 0.73 ug/ml

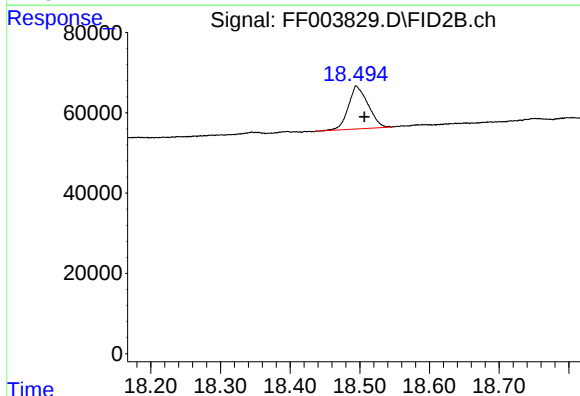


#14 N-DOTRIACONTANE

R.T.: 18.495 min
Delta R.T.: -0.012 min
Response: 209122
Conc: 1.47 ug/ml

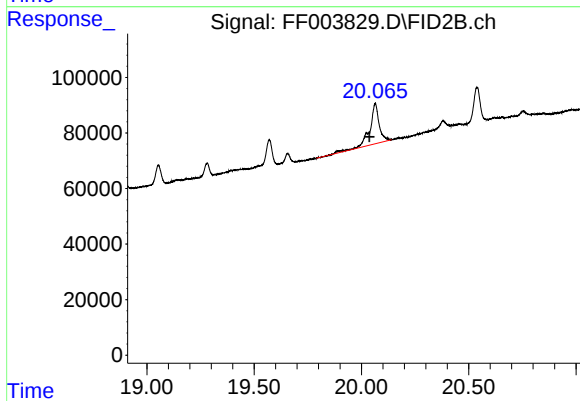

#16 N-HEXATRIACONTANE

R.T.: 20.065 min
Delta R.T.: 0.027 min
Response: 445237
Conc: 3.41 ug/ml

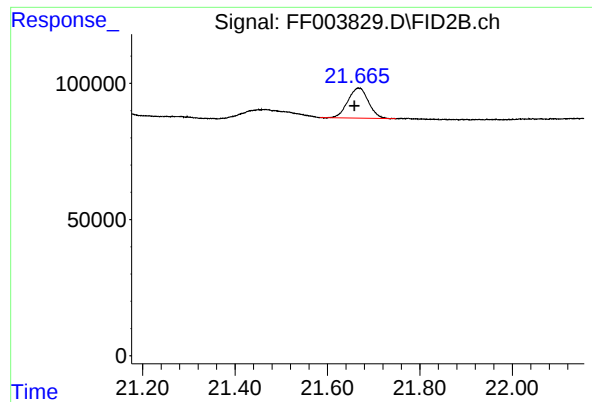

#18 N-TETRACONTANE

R.T.: 21.666 min
Delta R.T.: 0.008 min
Response: 341399
Conc: 2.74 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK