

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF031319\  
Data File : FF003810.D  
Signal(s) : FID2B.ch  
Acq On : 13 Mar 2019 09:04  
Operator : AJ\SJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Mar 14 00:58:52 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Quant Title :  
QLast Update : Mon Mar 04 08:35:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.590 | 1977239  | 14.201 ug/ml |

Target Compounds

-----

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF031319\  
Data File : FF003810.D  
Signal(s) : FID2B.ch  
Acq On : 13 Mar 2019 09:04  
Operator : AJ\SJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Mar 14 00:58:52 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Quant Title :  
QLast Update : Mon Mar 04 08:35:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

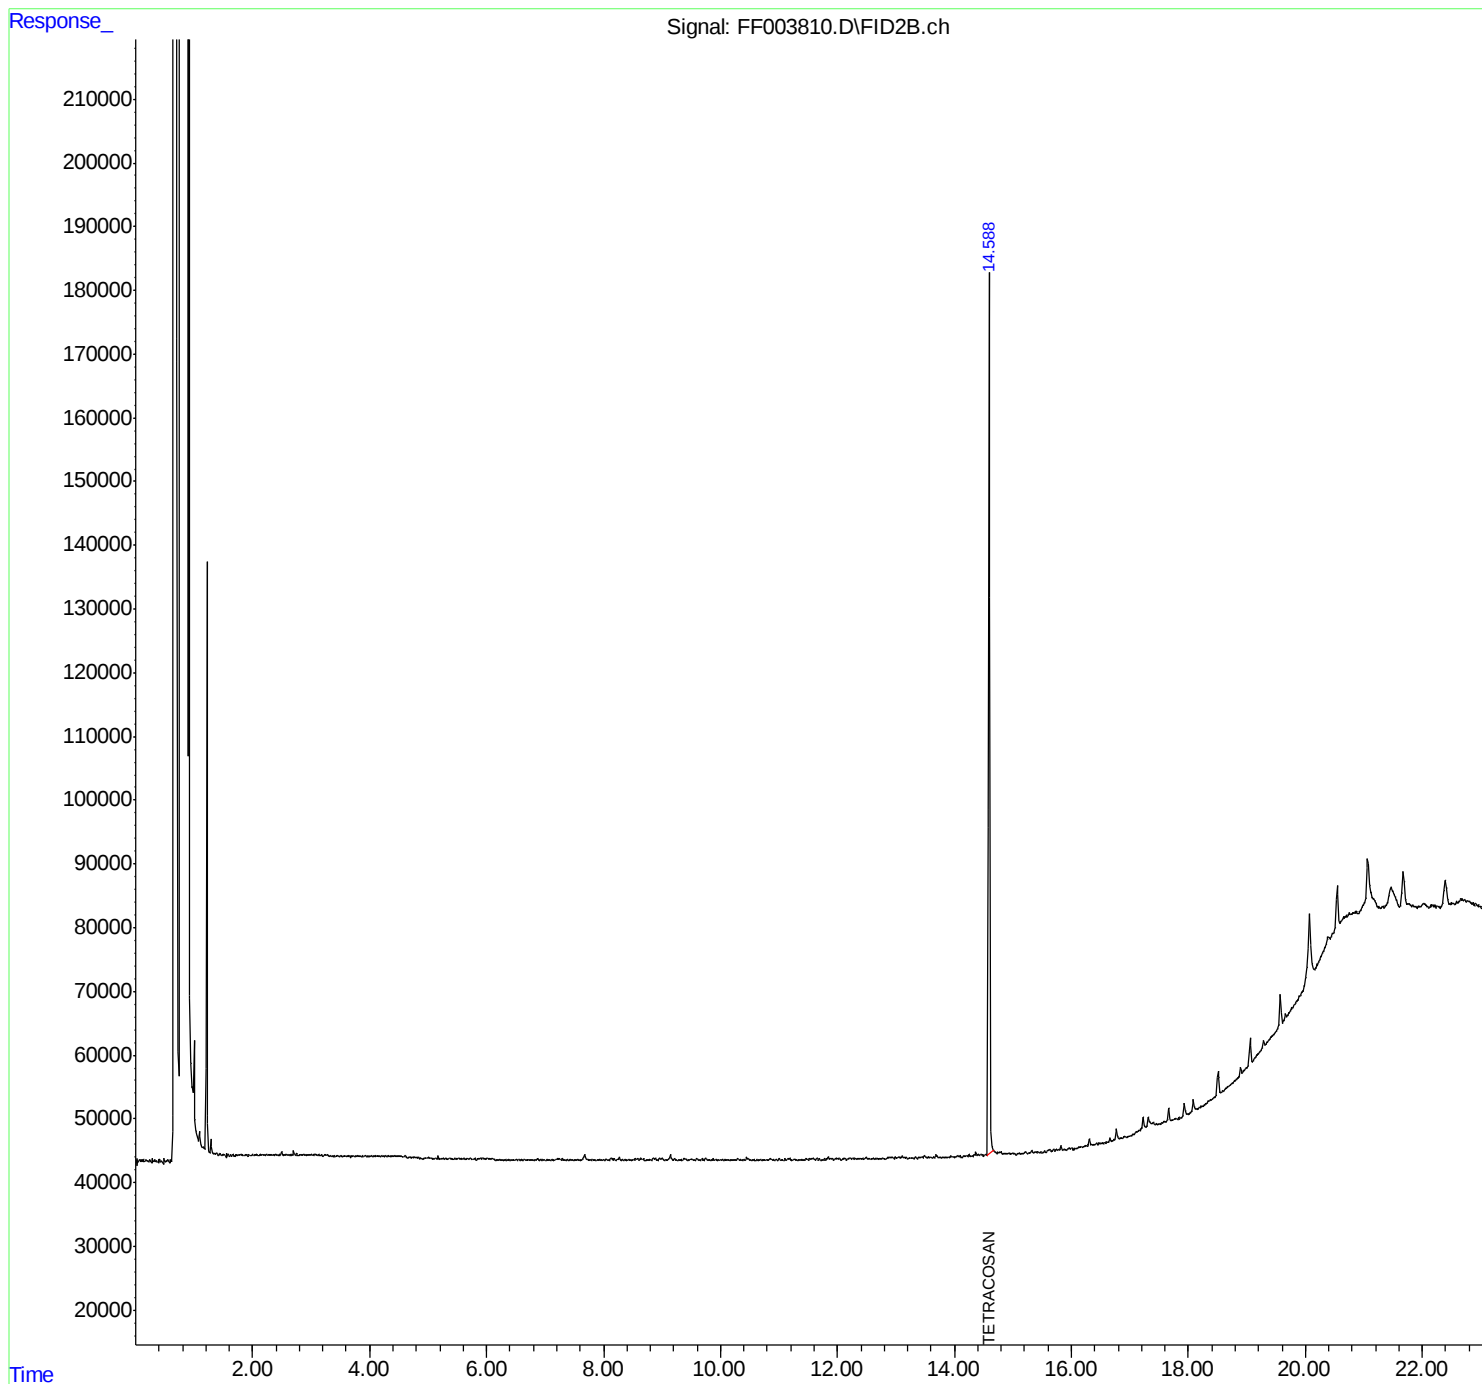

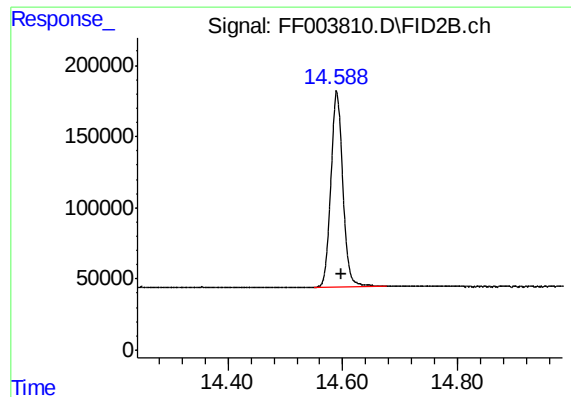

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.590 min  
Delta R.T.: -0.009 min  
Response: 1977239  
Conc: 14.20 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

rteres

# Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF031319\  
Data File : FF003810.D  
Signal(s) : FID2B.ch  
Acq On : 13 Mar 2019 09:04  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e

Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Title :

Signal : FID2B.ch

| peak<br>#               | R.T.<br>min | Start<br>min | End<br>min | PK<br>TY | peak<br>height | peak<br>area | peak<br>% max. | % of<br>total |
|-------------------------|-------------|--------------|------------|----------|----------------|--------------|----------------|---------------|
| 1                       | 14.590      | 14.551       | 14.674     | BB       | 137969         | 1977239      | 100.00%        | 100.000%      |
| Sum of corrected areas: |             |              |            |          |                | 1977239      |                |               |

FF030119.M Thu Mar 14 09:17:03 2019