

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
 Data File : FF003818.D
 Signal(s) : FID2B.ch
 Acq On : 13 Mar 2019 15:43
 Operator : AJ\SJ
 Sample : PB117871BS
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB117871BS

Integration File: autoint1.e
 Quant Time: Mar 14 01:03:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.590	1991291	14.302 ug/ml
Target Compounds			
2) N-DECANE	4.318	2732146	17.762 ug/ml
3) N-DODECANE	6.339	2760003	17.685 ug/ml
4) N-TETRADECANE	8.132	2746508	17.130 ug/ml
5) N-HEXADECANE	9.733	2703557	16.599 ug/ml
6) N-OCTADECANE	11.176	2642656	16.040 ug/ml
7) N-EICOSANE	12.487	2578085	15.759 ug/ml
8) N-DOCOSANE	13.687	2521059	15.621 ug/ml
10) N-TETRACOSANE	14.794	2488094	15.725 ug/ml
11) N-HEXACOSANE	15.818	2464805	15.970 ug/ml
12) N-OCTACOSANE	16.771	2488517	16.468 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031319\
Data File : FF03818.D
Signal(s) : FID2B.ch
Acq On : 13 Mar 2019 15:43
Operator : AJ\SJ
Sample : PB117871BS
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB117871BS

Integration File: autoint1.e
Quant Time: Mar 14 01:03:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

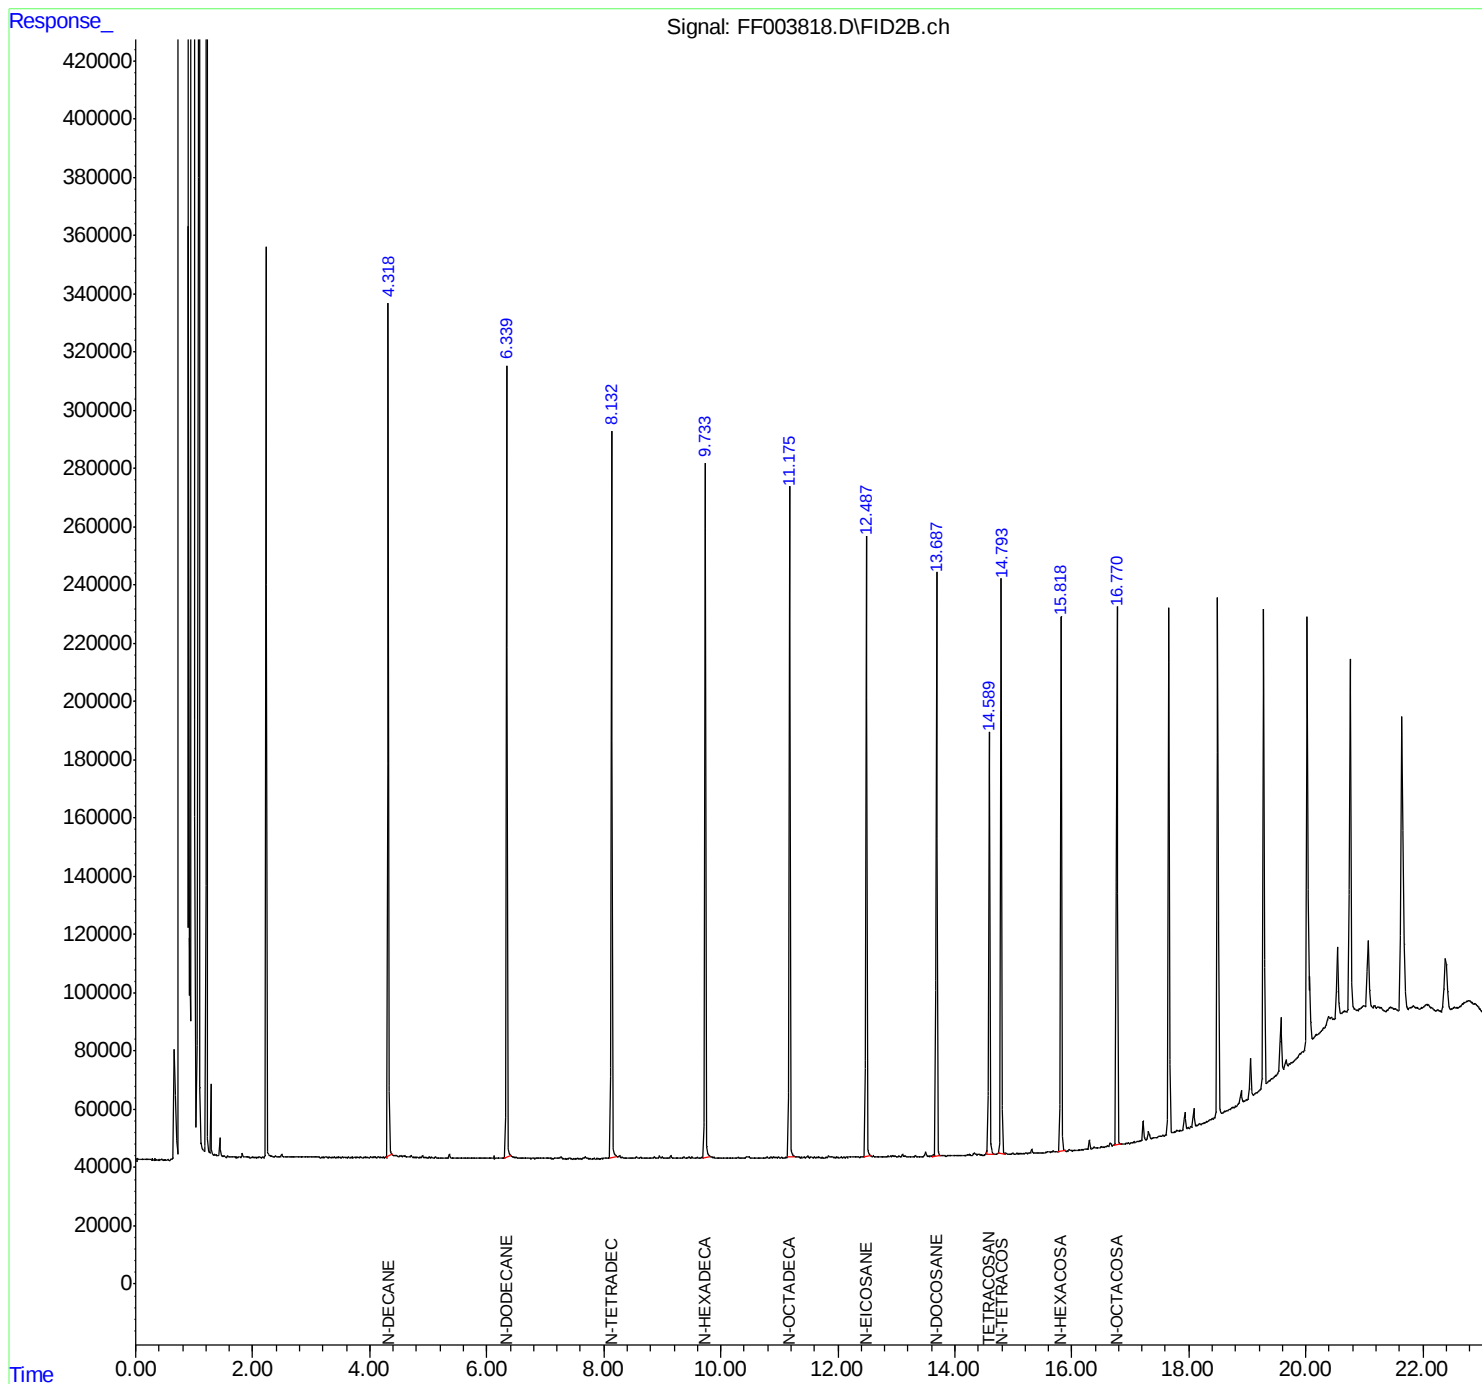


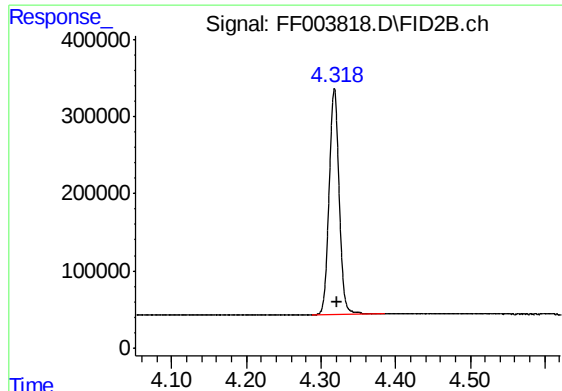

#2 N-DECANE


R.T.: 4.318 min
Delta R.T.: -0.003 min
Response: 2732146
Conc: 17.76 ug/ml

Instrument :
FID_F
ClientSampleId :
PB117871BS

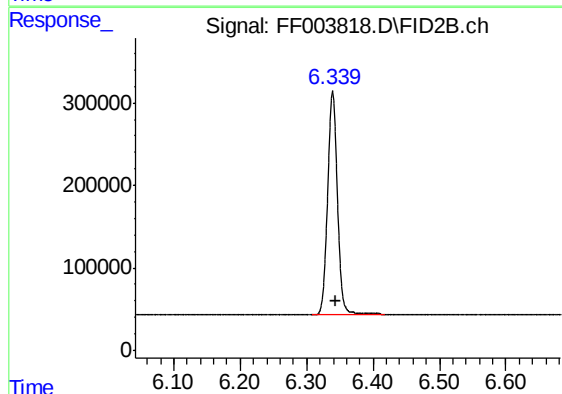


#3 N-DODECANE

R.T.: 6.339 min
Delta R.T.: -0.005 min
Response: 2760003
Conc: 17.69 ug/ml

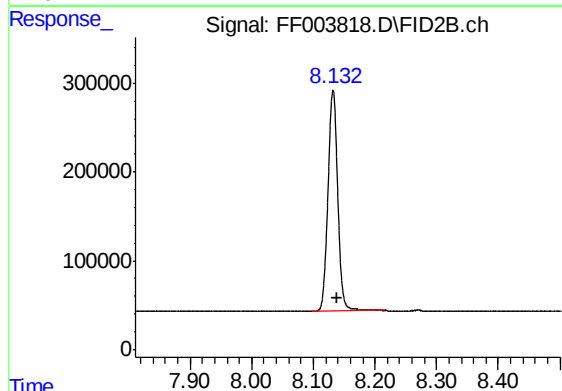


#4 N-TETRADECANE

R.T.: 8.132 min
Delta R.T.: -0.006 min
Response: 2746508
Conc: 17.13 ug/ml

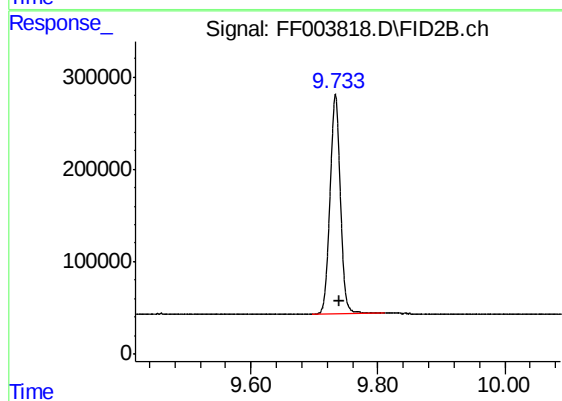

#5 N-HEXADECANE


R.T.: 9.733 min
Delta R.T.: -0.007 min
Response: 2703557
Conc: 16.60 ug/ml

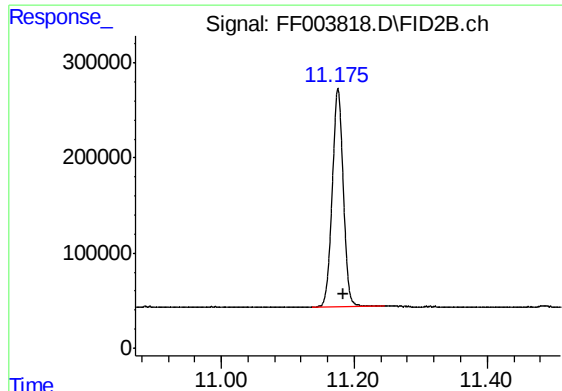

#6 N-OCTADECANE


R.T.: 11.176 min
Delta R.T.: -0.008 min
Response: 2642656
Conc: 16.04 ug/ml

Instrument :
FID_F
ClientSampleId :
PB117871BS

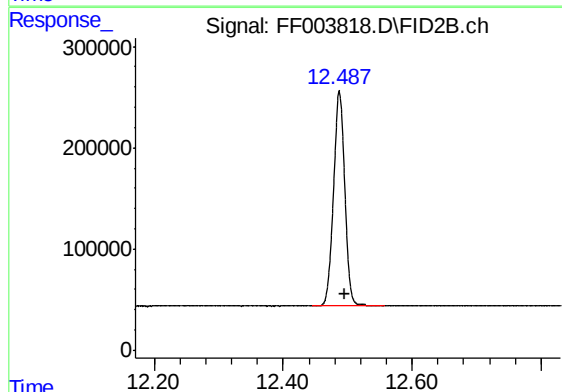


#7 N-EICOSANE

R.T.: 12.487 min
Delta R.T.: -0.009 min
Response: 2578085
Conc: 15.76 ug/ml

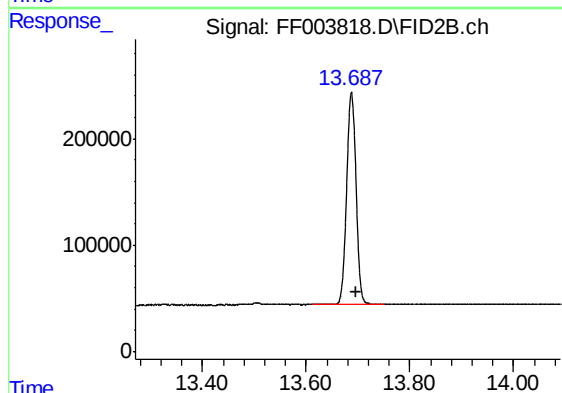


#8 N-DOCOSANE

R.T.: 13.687 min
Delta R.T.: -0.009 min
Response: 2521059
Conc: 15.62 ug/ml

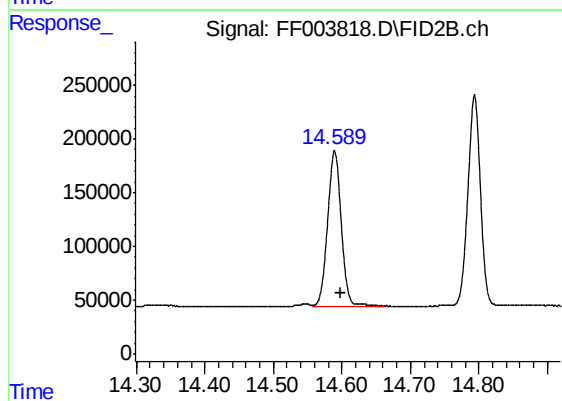

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.590 min
Delta R.T.: -0.009 min
Response: 1991291
Conc: 14.30 ug/ml

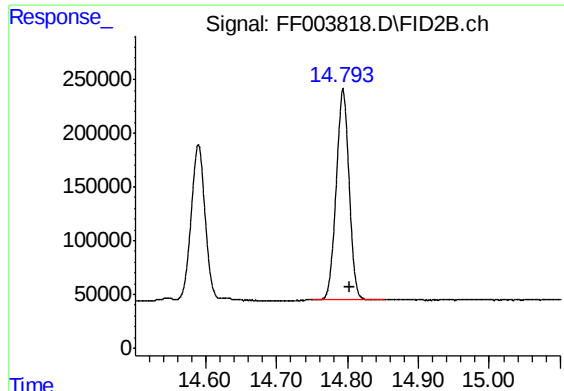

#10 N-TETRACOSANE


R.T.: 14.794 min
Delta R.T.: -0.009 min
Response: 2488094
Conc: 15.73 ug/ml

Instrument :
FID_F
ClientSampleId :
PB117871BS

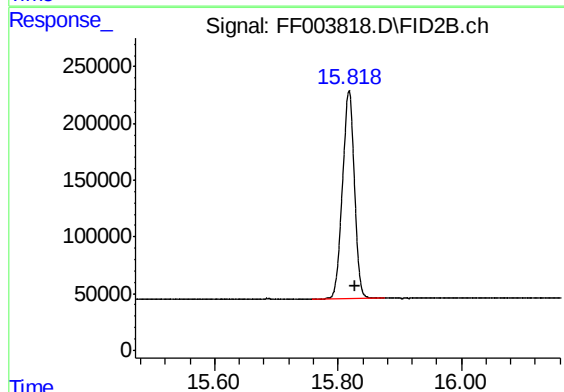

#11 N-HEXACOSANE

R.T.: 15.818 min
Delta R.T.: -0.009 min
Response: 2464805
Conc: 15.97 ug/ml

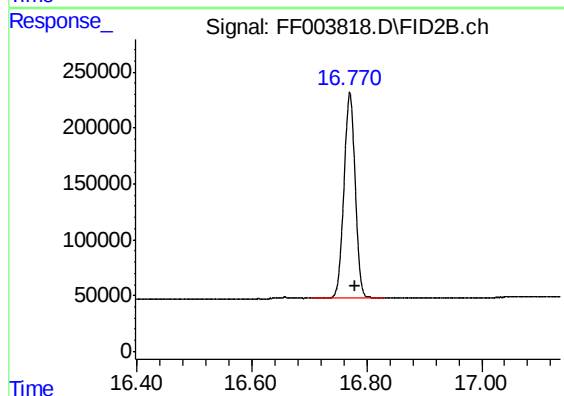

#12 N-OCTACOSANE

R.T.: 16.771 min
Delta R.T.: -0.009 min
Response: 2488517
Conc: 16.47 ug/ml