

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031320\
 Data File : FF006557.D
 Signal(s) : FID2B.ch
 Acq On : 13 Mar 2020 19:09
 Operator : DD\AJ
 Sample : L1907-06
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 13 23:05:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.582	2039768	15.849 ug/ml
Target Compounds			
4) N-TETRADECANE	8.223f	638486	4.464 ug/ml
12) N-OCTACOSANE	16.744	149615	1.045 ug/ml
13) N-TRIACONTANE	17.627	207040	1.463 ug/ml
14) N-DOTRIACONTANE	18.453	260559	1.933 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031320\
Data File : FF006557.D
Signal(s) : FID2B.ch
Acq On : 13 Mar 2020 19:09
Operator : DD\AJ
Sample : L1907-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 13 23:05:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

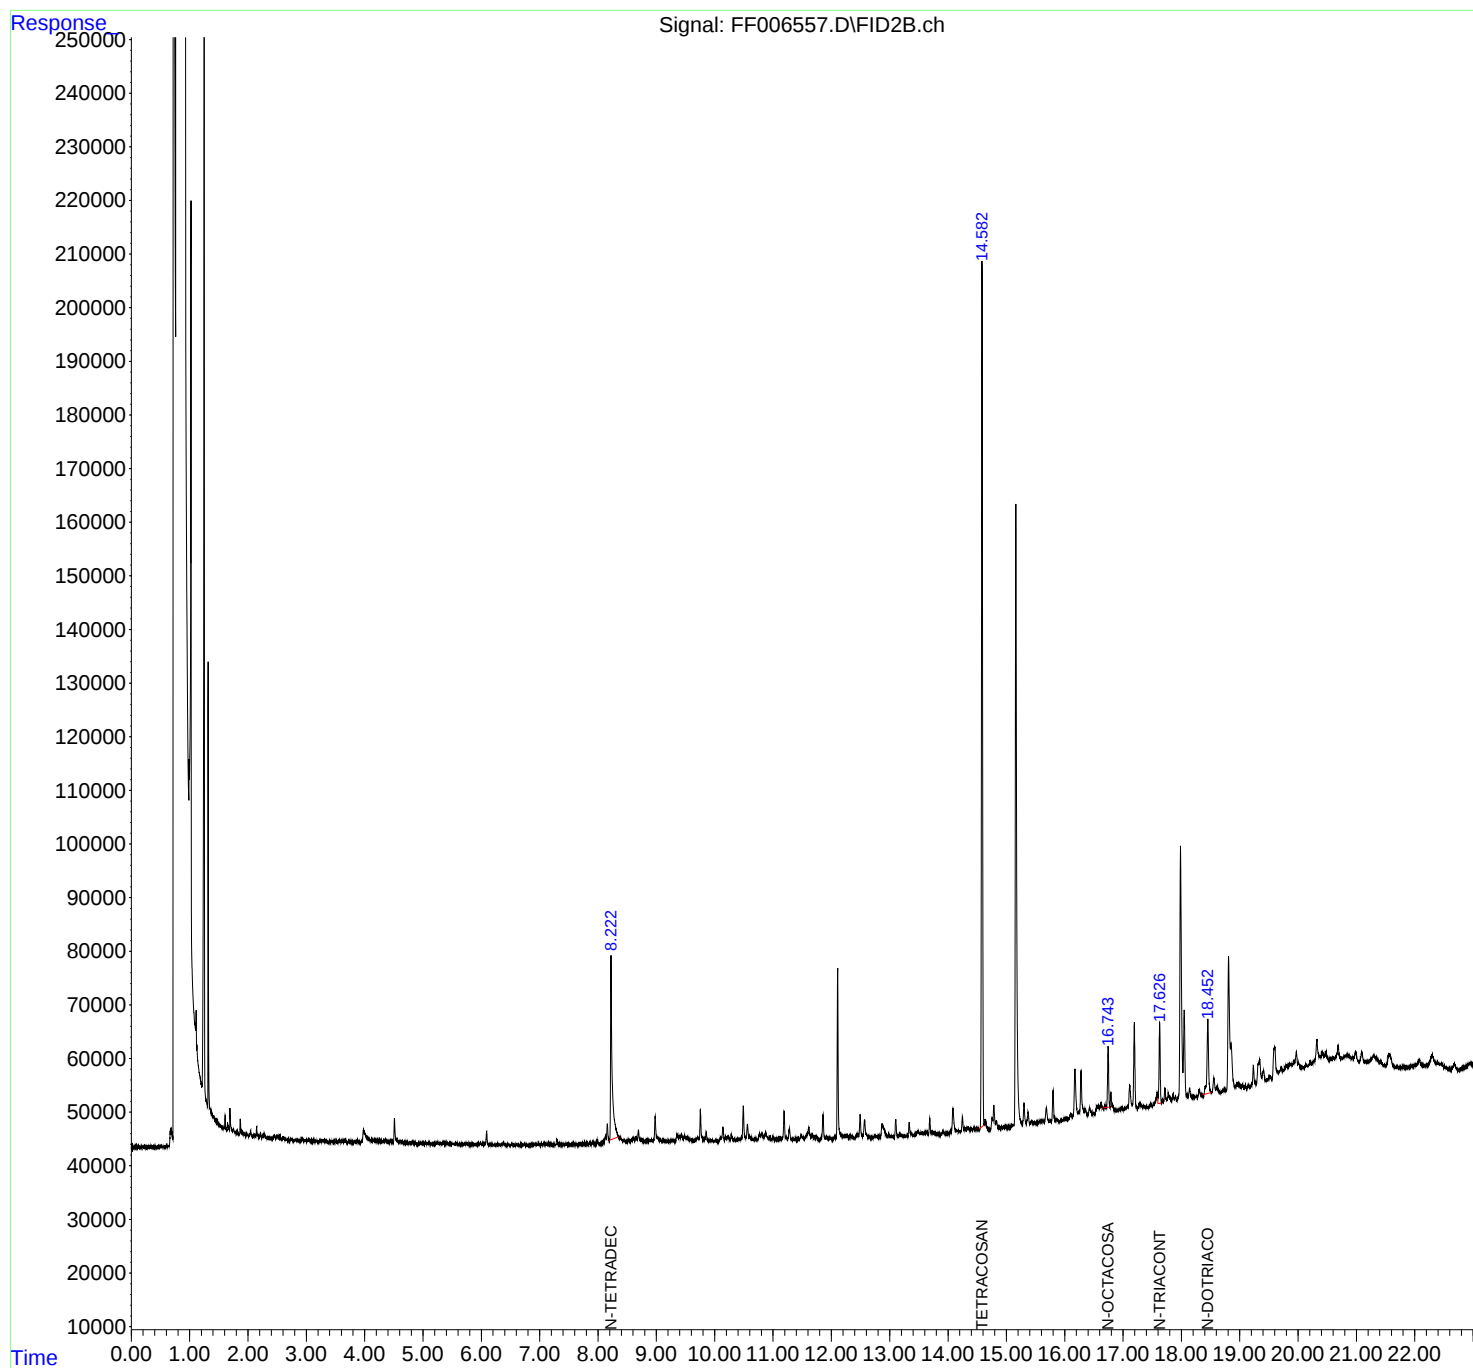

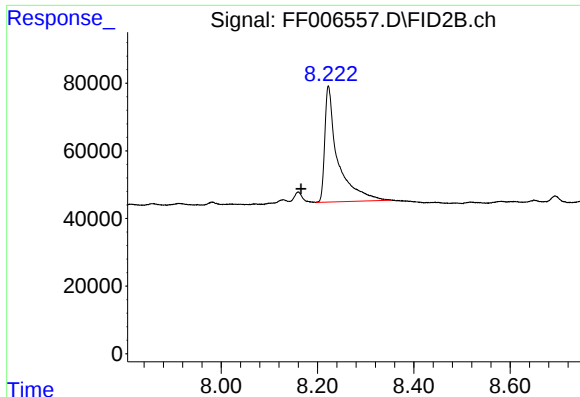


#4 N-TETRADECANE

R.T.: 8.223 min
Delta R.T.: 0.057 min
Response: 638486
Conc: 4.46 ug/ml

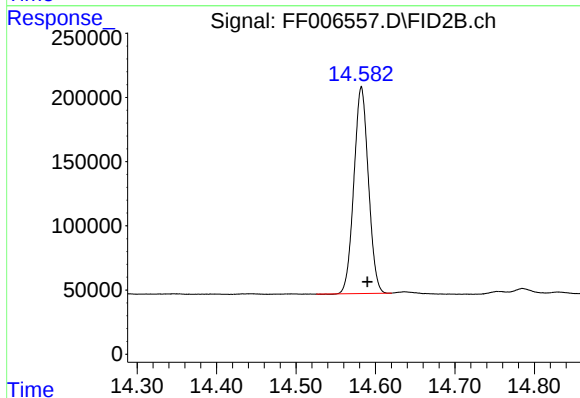


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.582 min
Delta R.T.: -0.007 min
Response: 2039768
Conc: 15.85 ug/ml

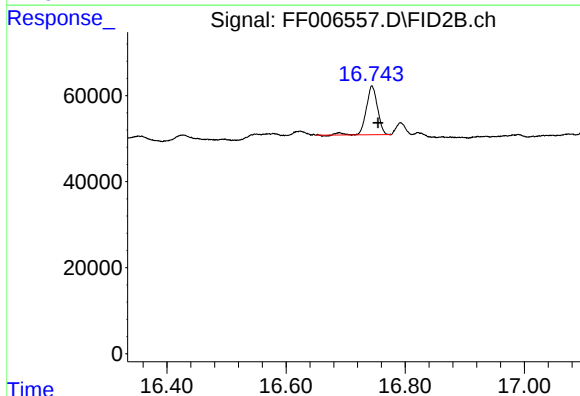


#12 N-OCTACOSANE

R.T.: 16.744 min
Delta R.T.: -0.010 min
Response: 149615
Conc: 1.04 ug/ml

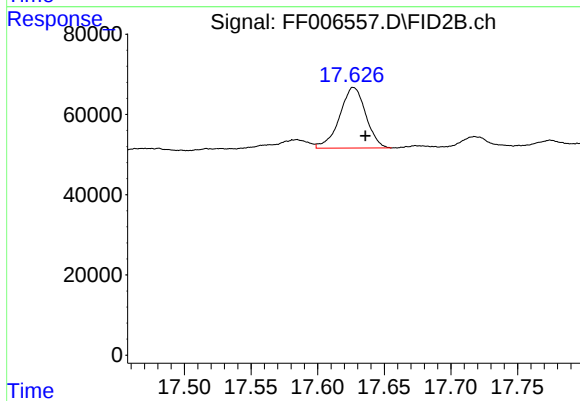

#13 N-TRIACONTANE

R.T.: 17.627 min
Delta R.T.: -0.009 min
Response: 207040
Conc: 1.46 ug/ml

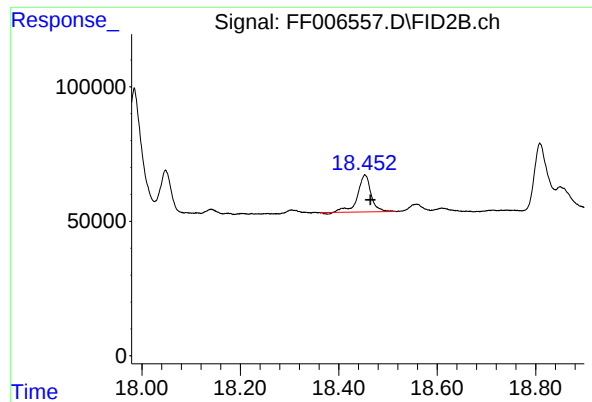

#14 N-DOTRIACONTANE

R.T.: 18.453 min
Delta R.T.: -0.011 min
Response: 260559
Conc: 1.93 ug/ml