

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031320\
 Data File : FF006562.D
 Signal(s) : FID2B.ch
 Acq On : 13 Mar 2020 22:13
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 13 23:06:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.586	2256039	17.529 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.462	123239	0.914 ug/ml
16) N-HEXATRIACONTANE	19.972	430041	4.682 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031320\
 Data File : FF006562.D
 Signal(s) : FID2B.ch
 Acq On : 13 Mar 2020 22:13
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 13 23:06:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

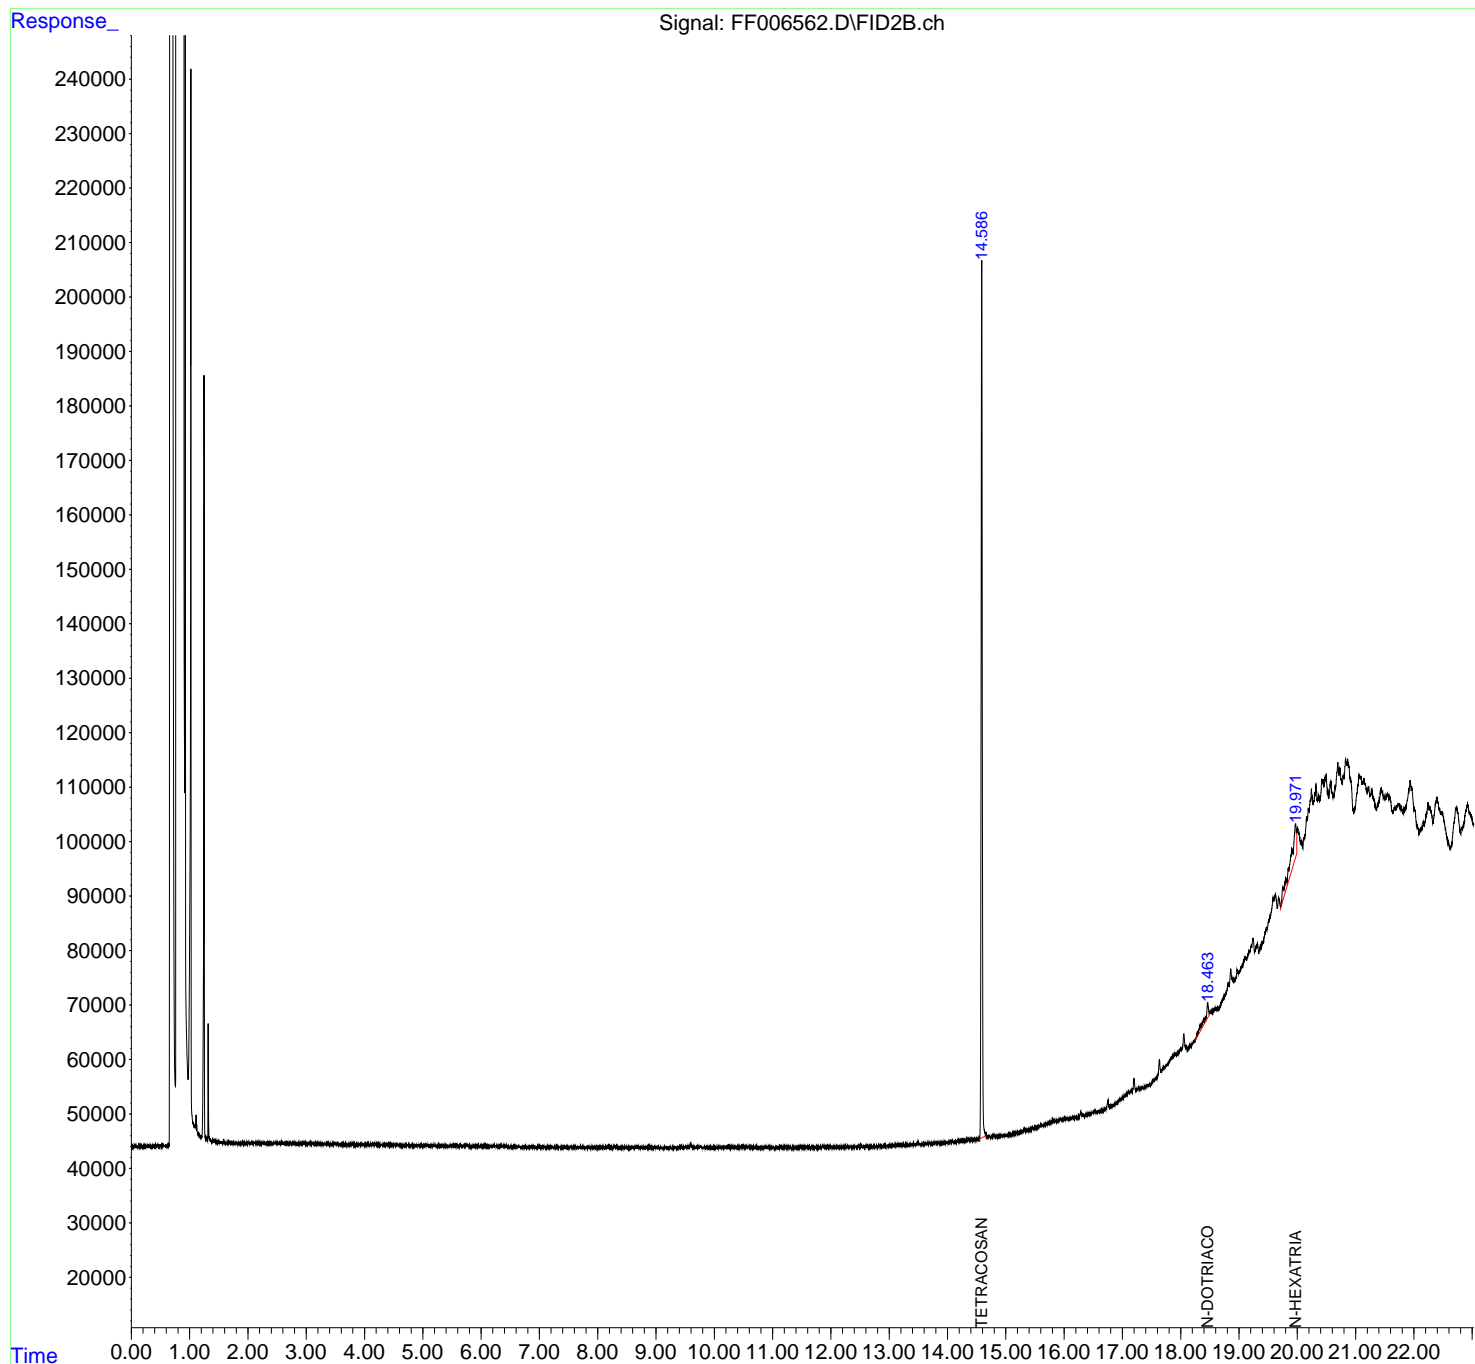

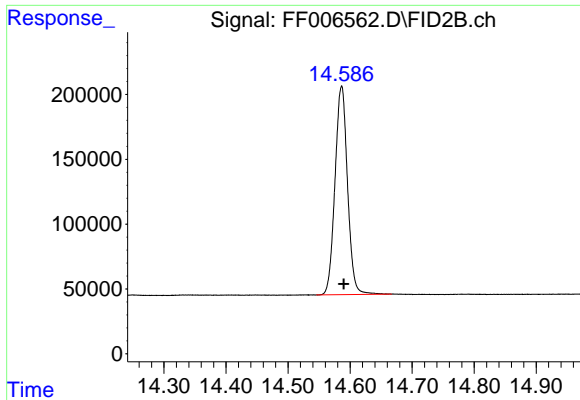


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.586 min
 Delta R.T.: -0.003 min
 Response: 2256039
 Conc: 17.53 ug/ml

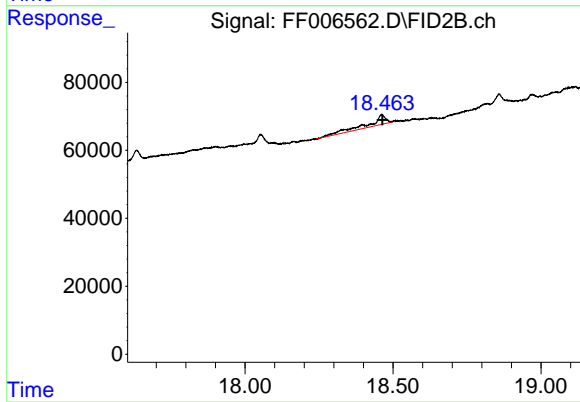

#14 N-DOTRIACONTANE

R.T.: 18.462 min
 Delta R.T.: -0.002 min
 Response: 123239
 Conc: 0.91 ug/ml

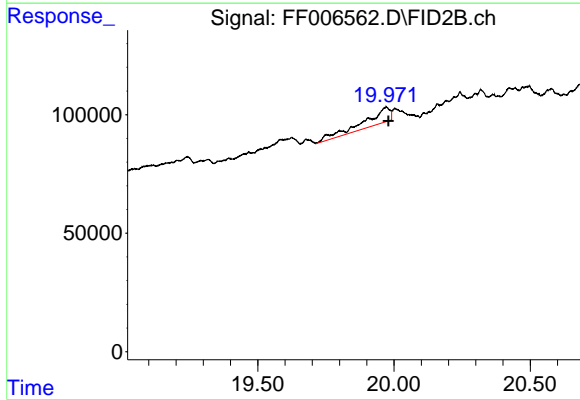

#16 N-HEXATRIACONTANE

R.T.: 19.972 min
 Delta R.T.: -0.007 min
 Response: 430041
 Conc: 4.68 ug/ml