

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031420\
 Data File : FF006572.D
 Signal(s) : FID2B.ch
 Acq On : 14 Mar 2020 13:16
 Operator : DD\AJ
 Sample : L1761-06 20X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 16 00:51:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.373	101290	0.718 ug/ml
4) N-TETRADECANE	8.161	291480	2.038 ug/ml
5) N-HEXADECANE	9.756	411209	2.805 ug/ml
6) N-OCTADECANE	11.193	297893	2.016 ug/ml
7) N-EICOSANE	12.498	296906	1.998 ug/ml
8) N-DOCOSANE	13.691	121145	0.816 ug/ml
10) N-TETRACOSANE	14.774	773281	5.232 ug/ml
11) N-HEXACOSANE	15.806	89717	0.619 ug/ml
12) N-OCTACOSANE	16.768	260019	1.815 ug/ml
13) N-TRIACONTANE	17.633	237383	1.677 ug/ml
14) N-DOTRIACONTANE	18.461	161545	1.198 ug/ml
16) N-HEXATRIACONTANE	19.979	190599	2.075 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031420\
Data File : FF006572.D
Signal(s) : FID2B.ch
Acq On : 14 Mar 2020 13:16
Operator : DD\AJ
Sample : L1761-06 20X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 16 00:51:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

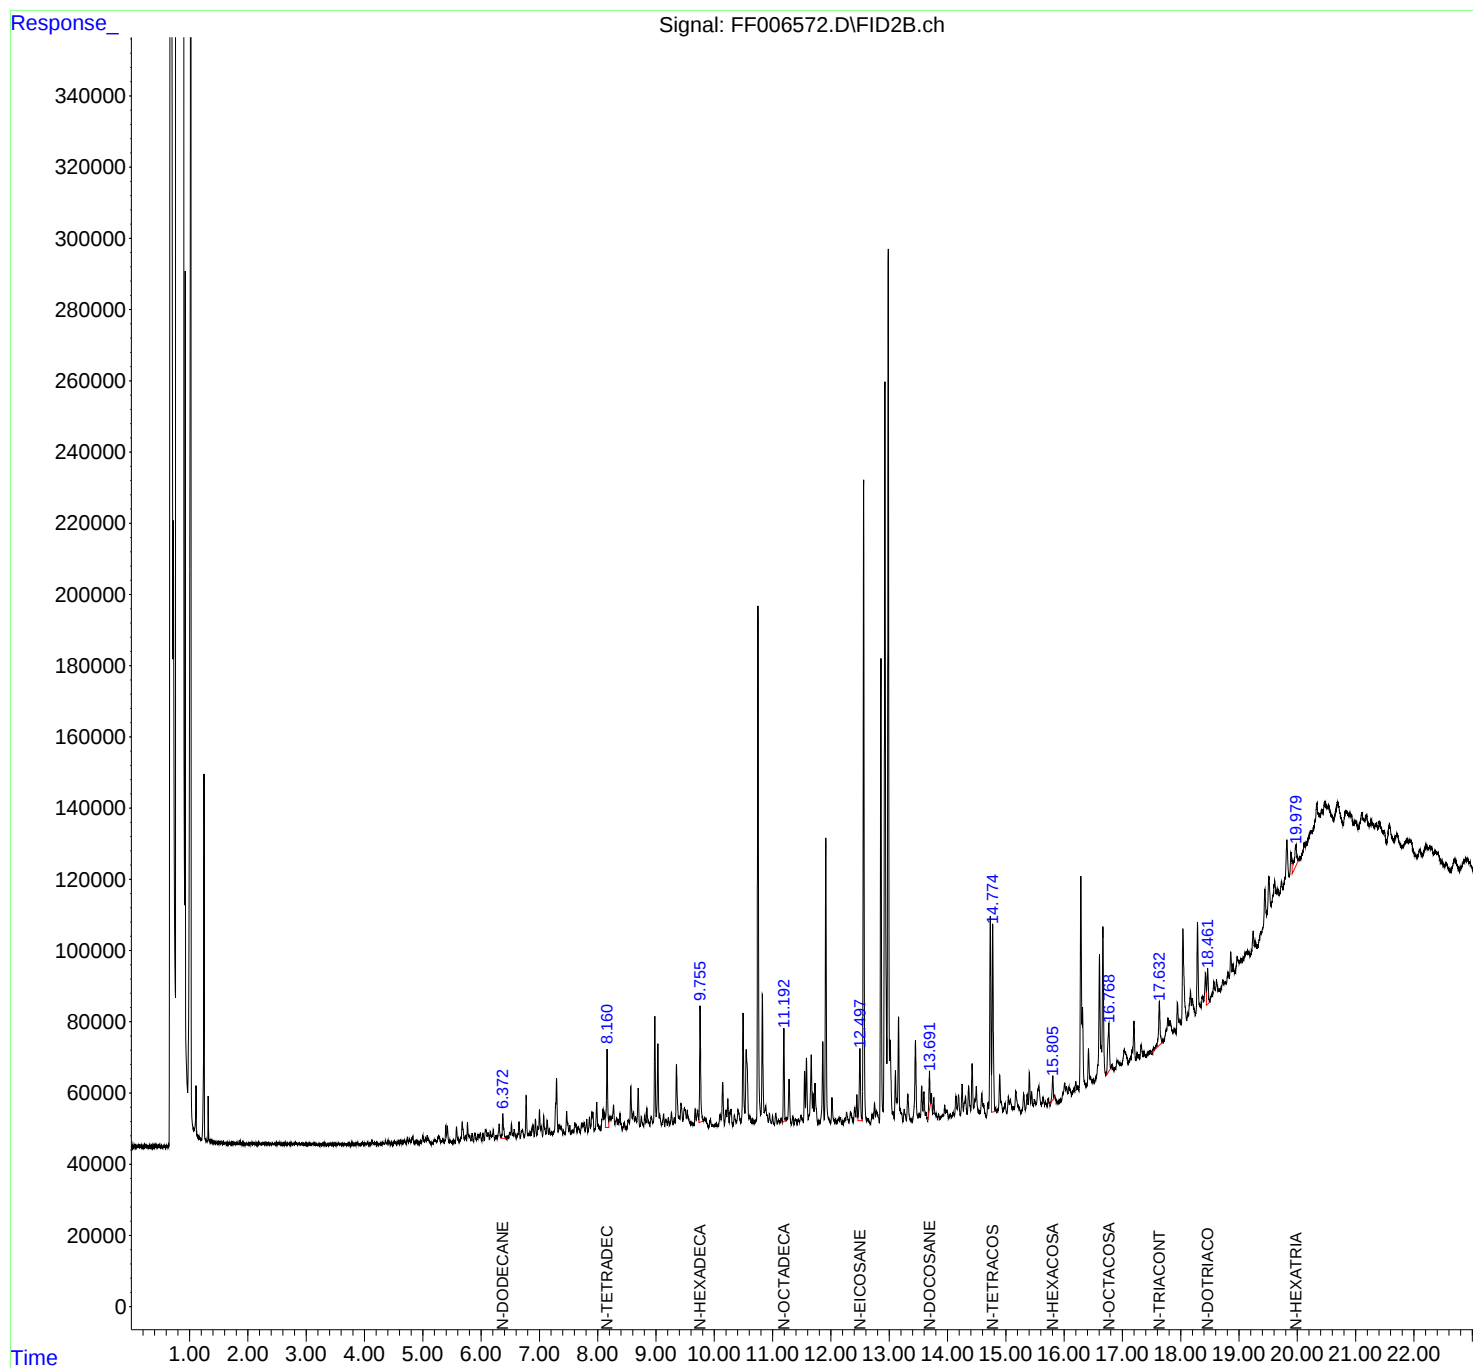

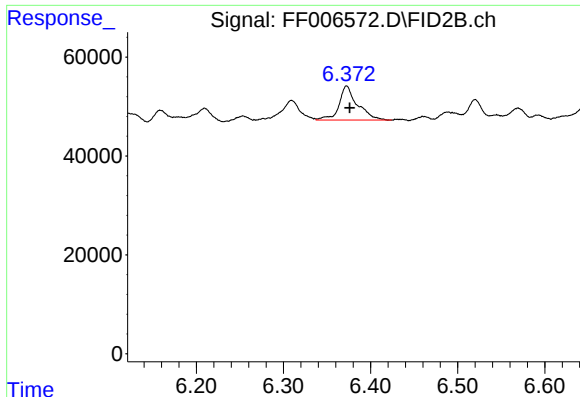


#3 N-DODECANE

R.T.: 6.373 min
Delta R.T.: -0.004 min
Response: 101290
Conc: 0.72 ug/ml

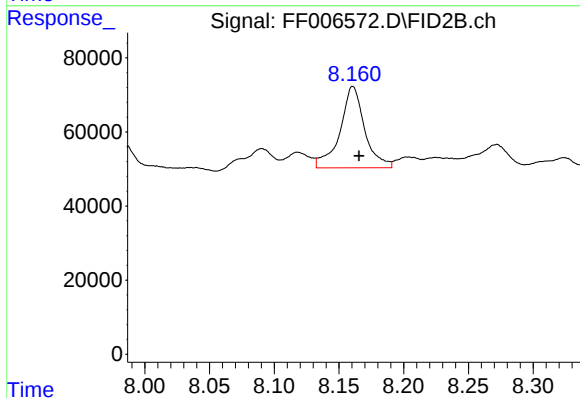


#4 N-TETRADECANE

R.T.: 8.161 min
Delta R.T.: -0.005 min
Response: 291480
Conc: 2.04 ug/ml

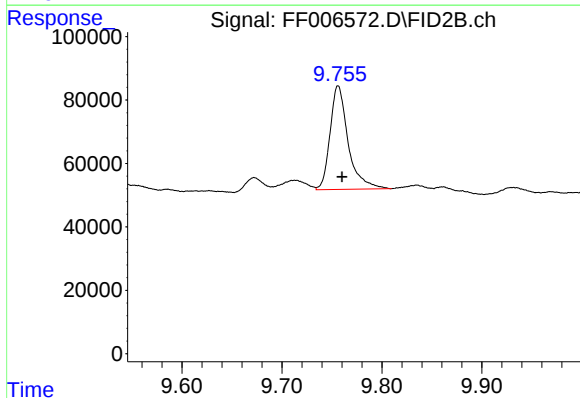


#5 N-HEXADECANE

R.T.: 9.756 min
Delta R.T.: -0.004 min
Response: 411209
Conc: 2.81 ug/ml

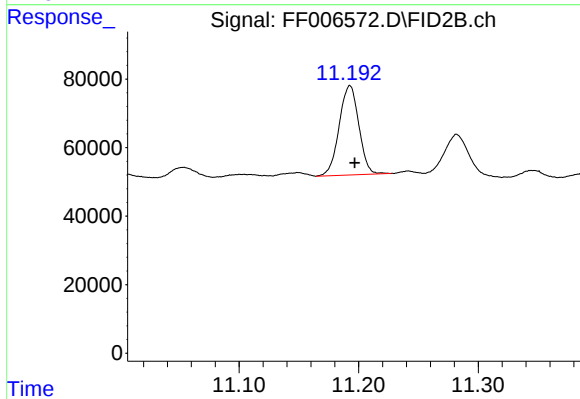


#6 N-OCTADECANE

R.T.: 11.193 min
Delta R.T.: -0.004 min
Response: 297893
Conc: 2.02 ug/ml

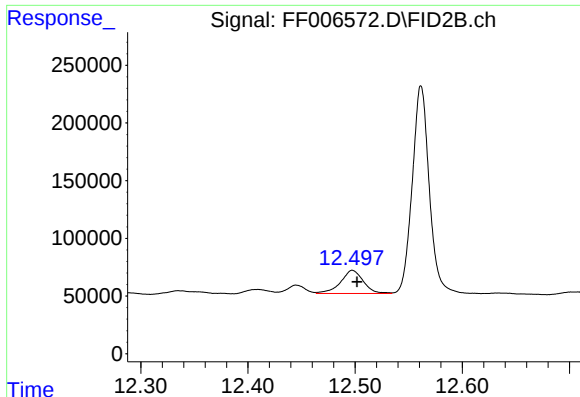


#7 N-EICOSANE

R.T.: 12.498 min
Delta R.T.: -0.004 min
Response: 296906
Conc: 2.00 ug/ml

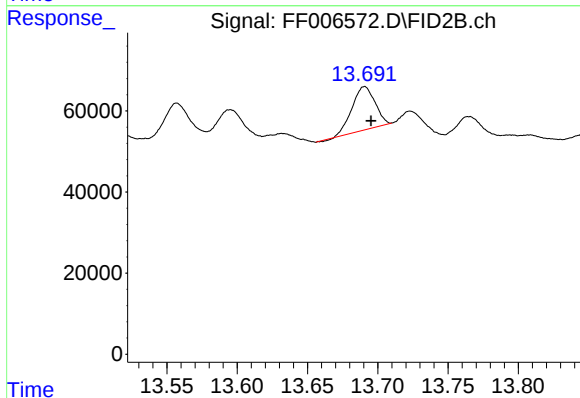


#8 N-DOCOSANE

R.T.: 13.691 min
Delta R.T.: -0.005 min
Response: 121145
Conc: 0.82 ug/ml

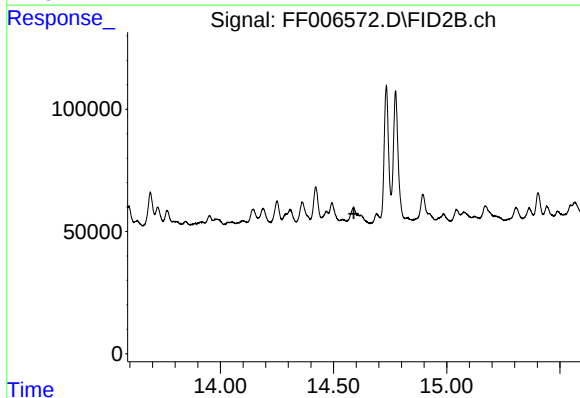


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.590 min
Response: 0
Conc: N.D.

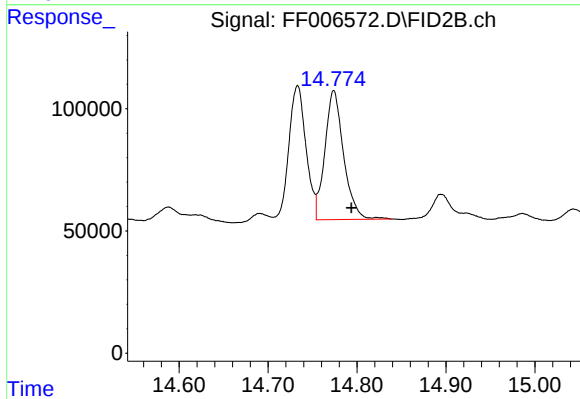


#10 N-TETRACOSANE

R.T.: 14.774 min
Delta R.T.: -0.020 min
Response: 773281
Conc: 5.23 ug/ml

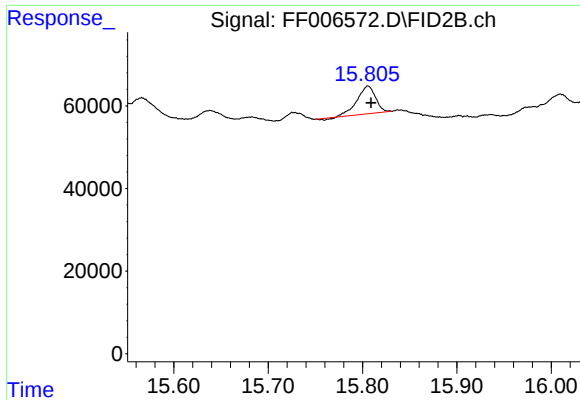


#11 N-HEXACOSANE

R.T.: 15.806 min
Delta R.T.: -0.003 min
Response: 89717
Conc: 0.62 ug/ml

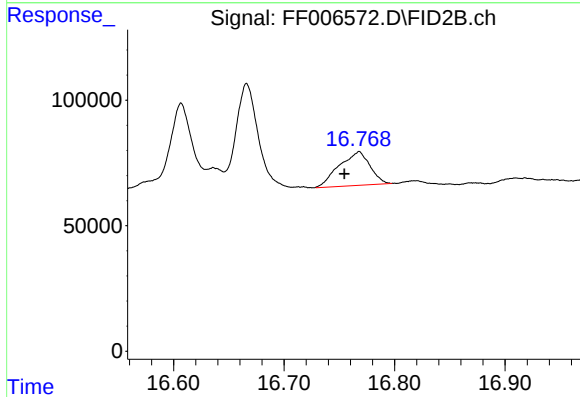


#12 N-OCTACOSANE

R.T.: 16.768 min
Delta R.T.: 0.013 min
Response: 260019
Conc: 1.82 ug/ml

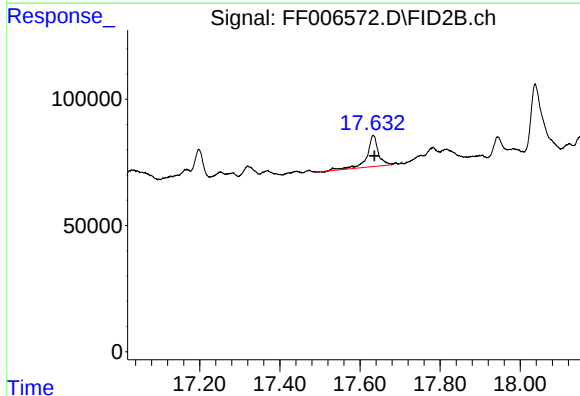


#13 N-TRIACONTANE

R.T.: 17.633 min
Delta R.T.: -0.003 min
Response: 237383
Conc: 1.68 ug/ml

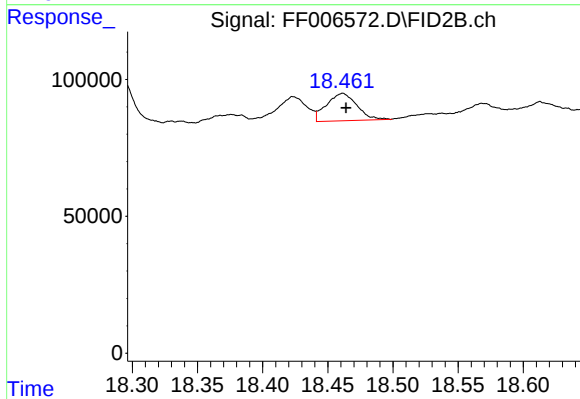

#14 N-DOTRIACONTANE

R.T.: 18.461 min
Delta R.T.: -0.003 min
Response: 161545
Conc: 1.20 ug/ml

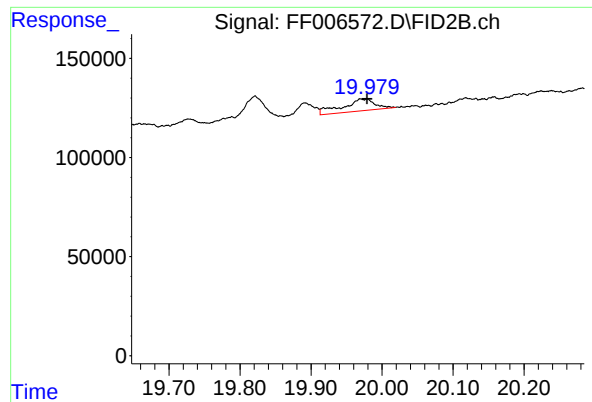

#16 N-HEXATRIACONTANE

R.T.: 19.979 min
Delta R.T.: 0.000 min
Response: 190599
Conc: 2.08 ug/ml