

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031420\
Data File : FF006574.D
Signal(s) : FID2B.ch
Acq On : 14 Mar 2020 14:46
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 16 00:52:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.587	2410354	18.728 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.633	95870	0.677 ug/ml
14) N-DOTRIACONTANE	18.461	112037	0.831 ug/ml
15) N-TETRATRIACONTANE	19.240	108769	0.963 ug/ml
16) N-HEXATRIACONTANE	19.978	54432	0.593 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031420\
Data File : FF006574.D
Signal(s) : FID2B.ch
Acq On : 14 Mar 2020 14:46
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 16 00:52:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

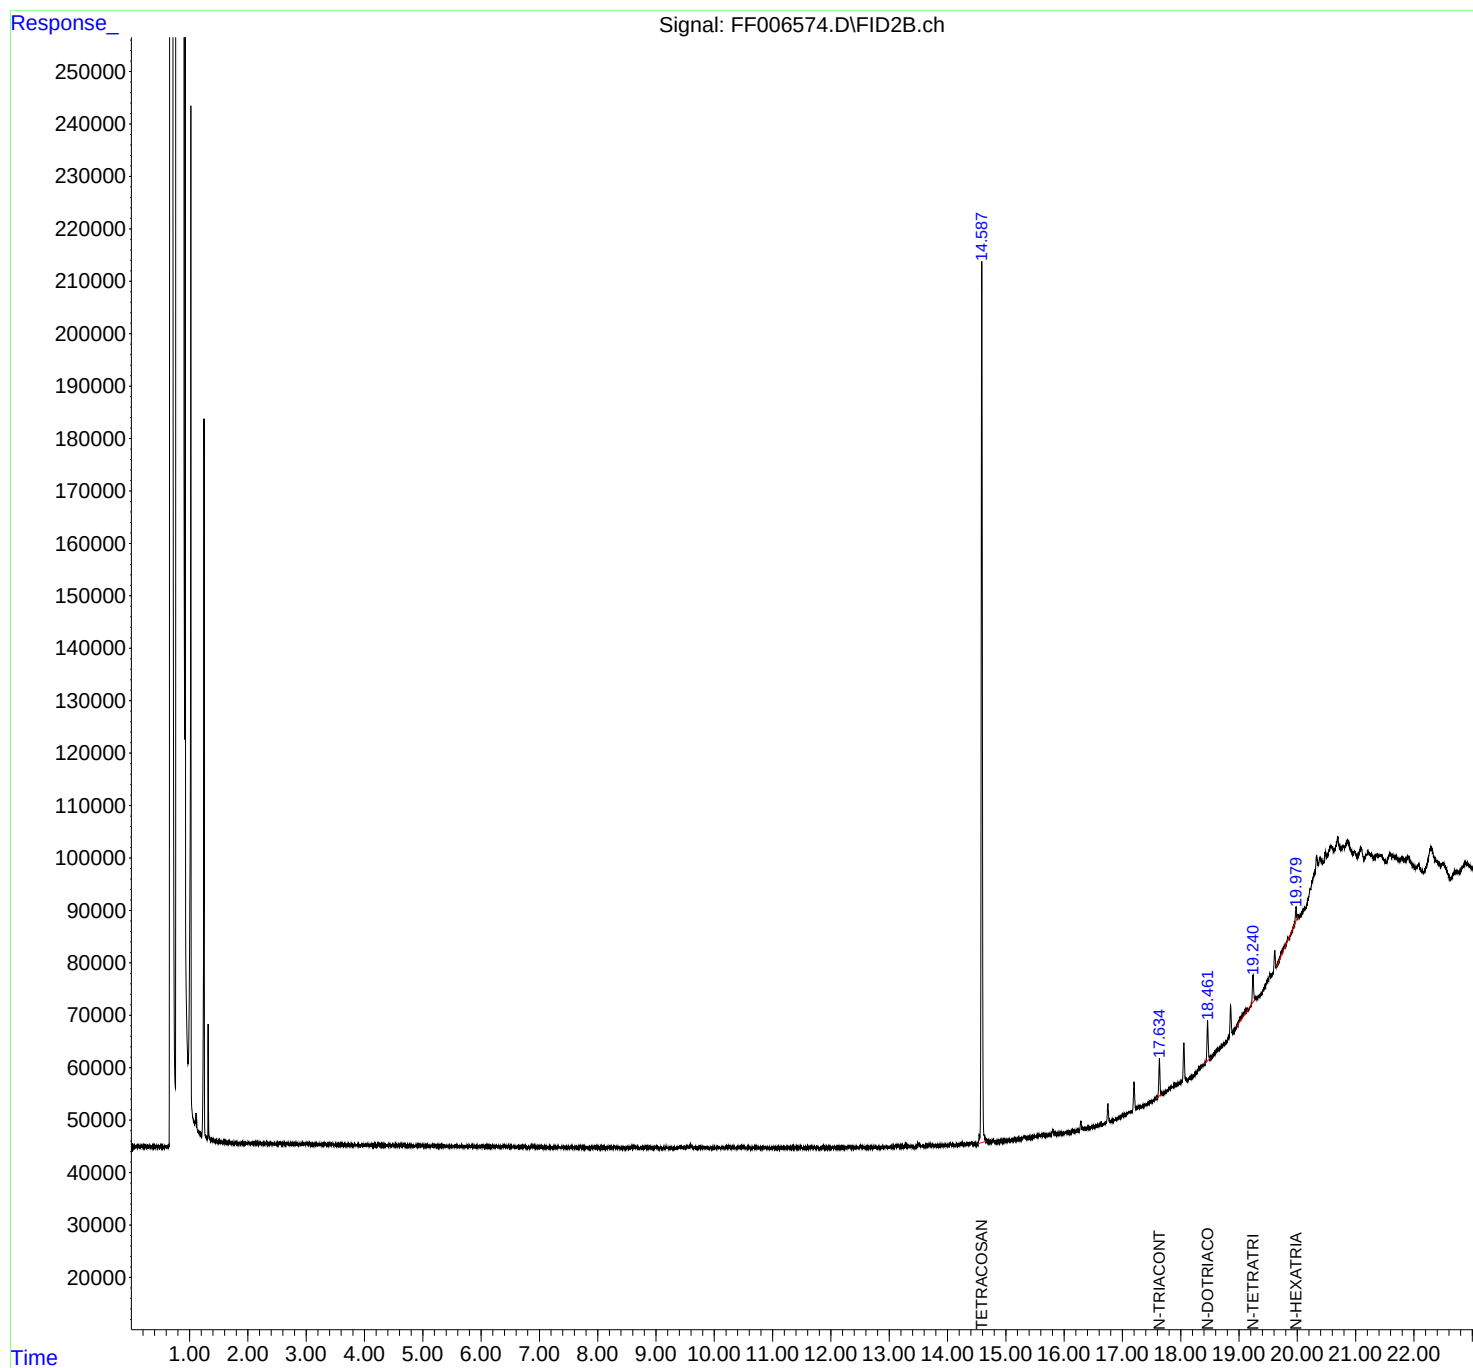

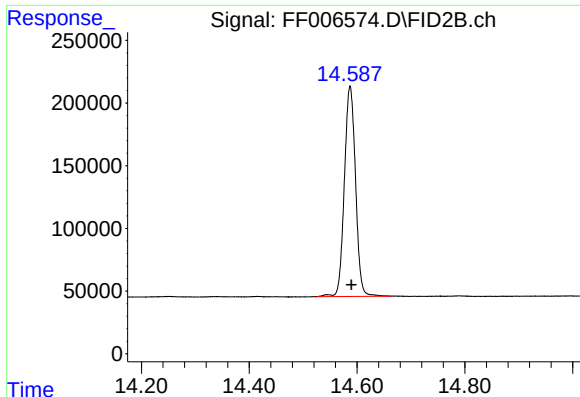


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.587 min
Delta R.T.: -0.003 min
Response: 2410354
Conc: 18.73 ug/ml

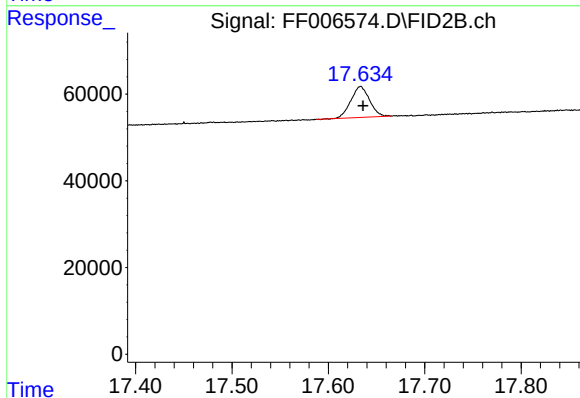


#13 N-TRIACONTANE

R.T.: 17.633 min
Delta R.T.: -0.003 min
Response: 95870
Conc: 0.68 ug/ml

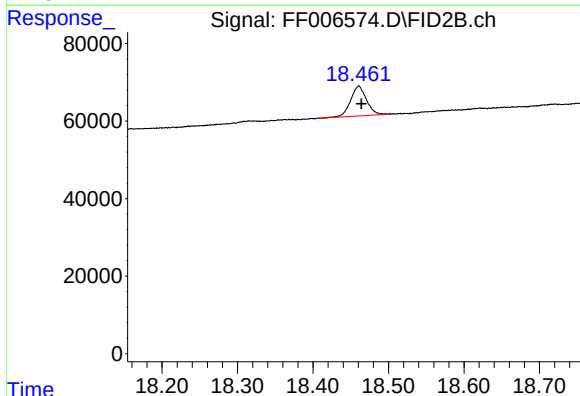


#14 N-DOTRIACONTANE

R.T.: 18.461 min
Delta R.T.: -0.003 min
Response: 112037
Conc: 0.83 ug/ml

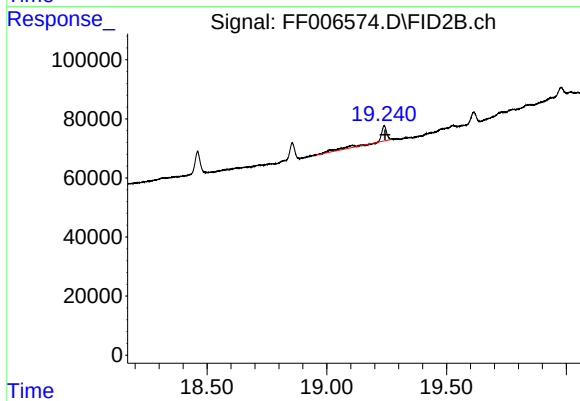

#15 N-TETRATRIACONTANE

R.T.: 19.240 min
Delta R.T.: -0.004 min
Response: 108769
Conc: 0.96 ug/ml

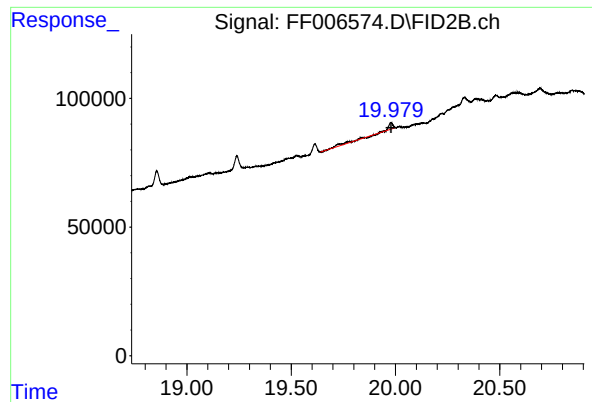

#16 N-HEXATRIACONTANE

R.T.: 19.978 min
Delta R.T.: 0.000 min
Response: 54432
Conc: 0.59 ug/ml