

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031423\
 Data File : FF012262.D
 Signal(s) : FID2B.ch
 Acq On : 14 Mar 2023 13:01
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 15 04:29:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
 Quant Title :
 QLast Update : Tue Feb 21 16:12:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.752	2111161	15.539 ug/ml
12) N-OCTACOSANE	17.199	2236806	18.224 ug/ml
13) N-TRIACONTANE	18.088	96356	0.825 ug/ml
14) N-DOTRIACONTANE	18.918	57970	0.521 ug/ml
16) N-HEXATRIACONTANE	20.449	59172	0.624 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031423\
Data File : FF012262.D
Signal(s) : FID2B.ch
Acq On : 14 Mar 2023 13:01
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 15 04:29:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

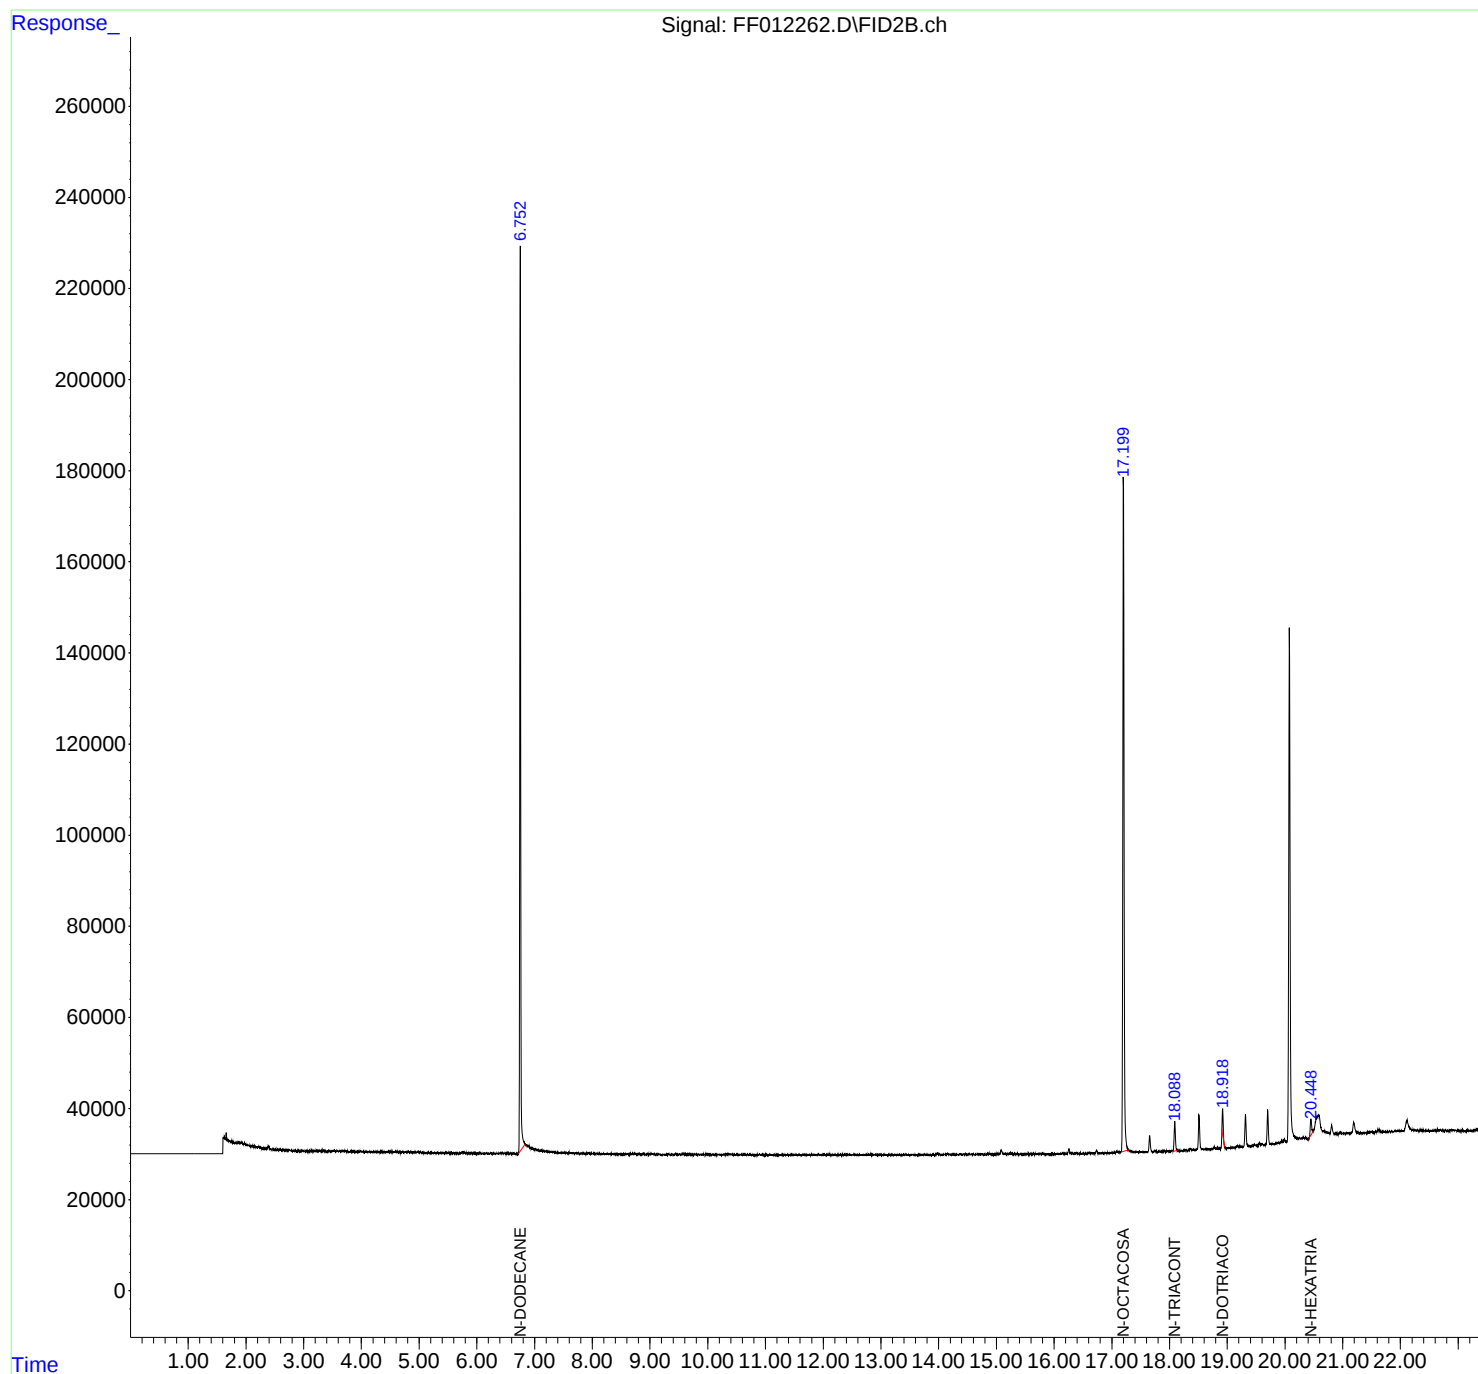


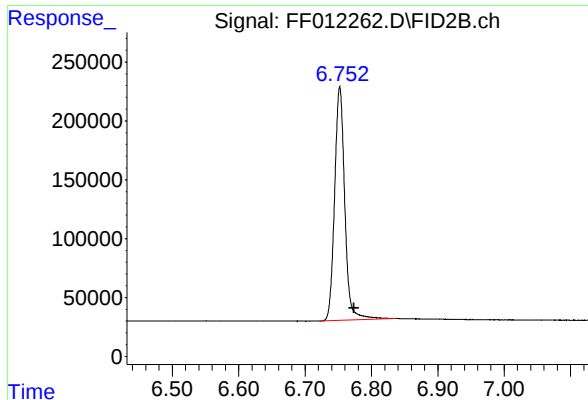

#3 N-DODECANE


R.T.: 6.752 min
Delta R.T.: -0.021 min
Response: 2111161
Conc: 15.54 ug/ml

Instrument :
FID_F
ClientSampleId :

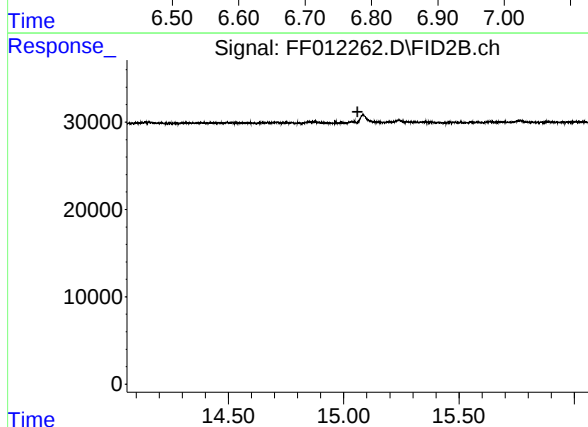


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.060 min
Response: 0
Conc: N.D.

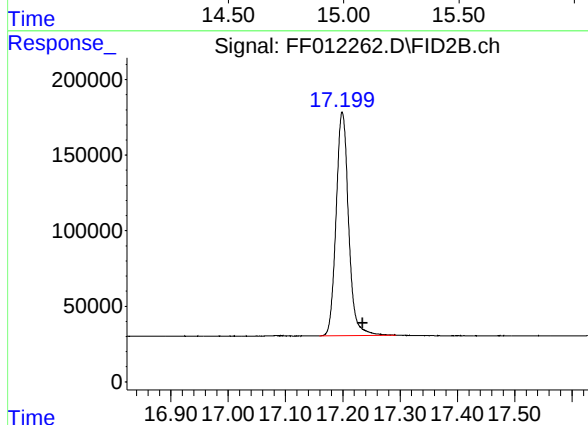


#12 N-OCTACOSANE

R.T.: 17.199 min
Delta R.T.: -0.035 min
Response: 2236806
Conc: 18.22 ug/ml

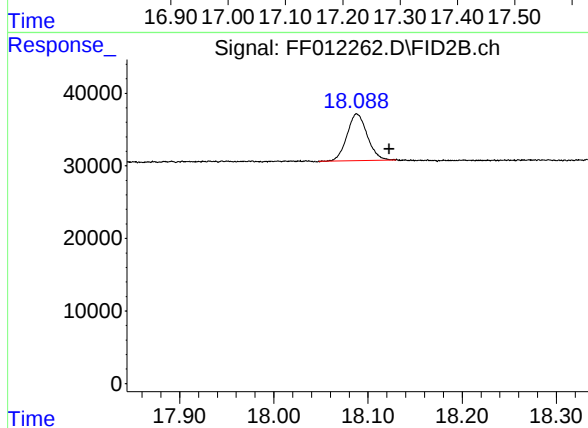

#13 N-TRIACONTANE


R.T.: 18.088 min
Delta R.T.: -0.034 min
Response: 96356
Conc: 0.83 ug/ml

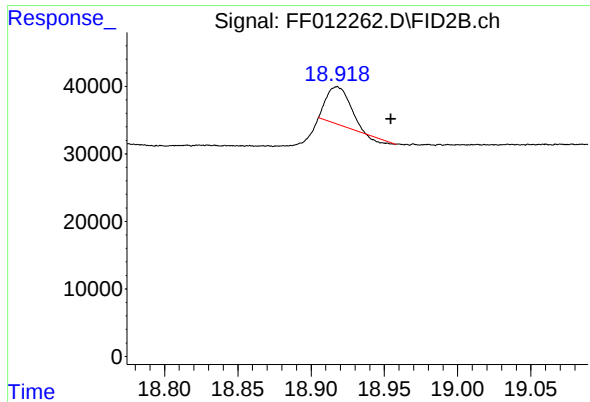

#14 N-DOTRIACONTANE

R.T.: 18.918 min
Delta R.T.: -0.037 min
Response: 57970
Conc: 0.52 ug/ml

Instrument :
FID_F
ClientSampleId :

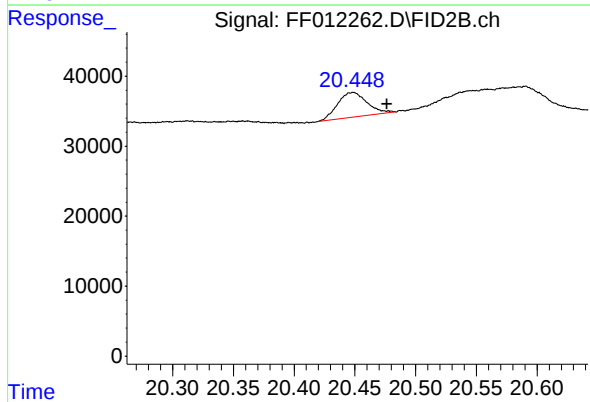

#16 N-HEXATRIACONTANE

R.T.: 20.449 min
Delta R.T.: -0.028 min
Response: 59172
Conc: 0.62 ug/ml