

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031523\
Data File : FF012275.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2023 08:44
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 15 14:30:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.924	77182	0.693 ug/ml
16)	N-HEXATRIACONTANE	20.474	124132	1.309 ug/ml
18)	N-TETRACONTANE	22.117	122607	1.346 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031523\
Data File : FF012275.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2023 08:44
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 15 14:30:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

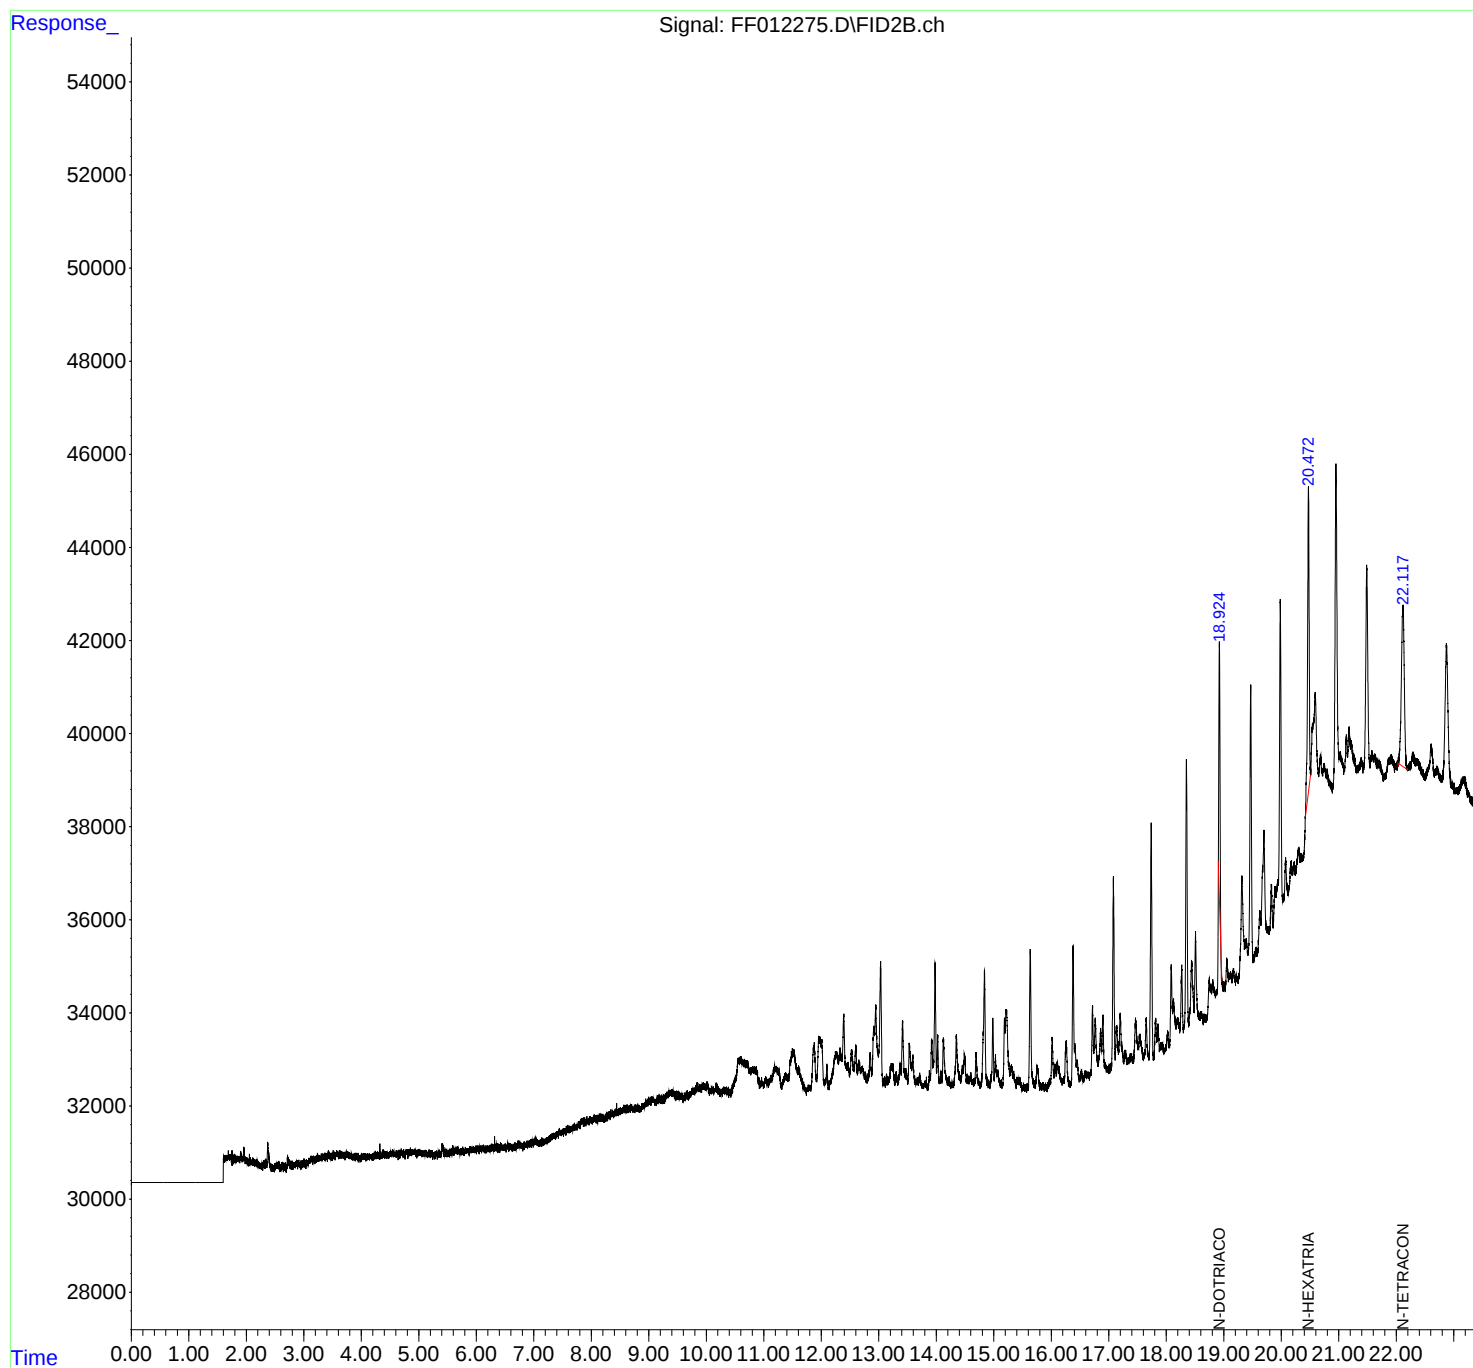


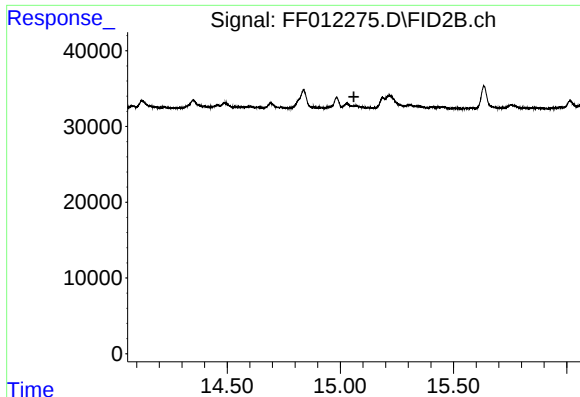

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.060 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

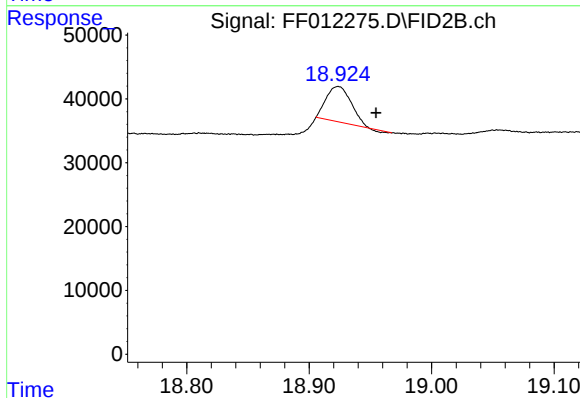


#14 N-DOTRIACONTANE

R.T.: 18.924 min
Delta R.T.: -0.031 min
Response: 77182
Conc: 0.69 ug/ml

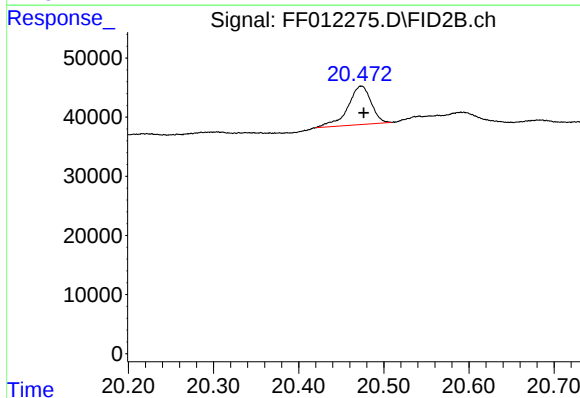

#16 N-HEXATRIACONTANE

R.T.: 20.474 min
Delta R.T.: -0.003 min
Response: 124132
Conc: 1.31 ug/ml

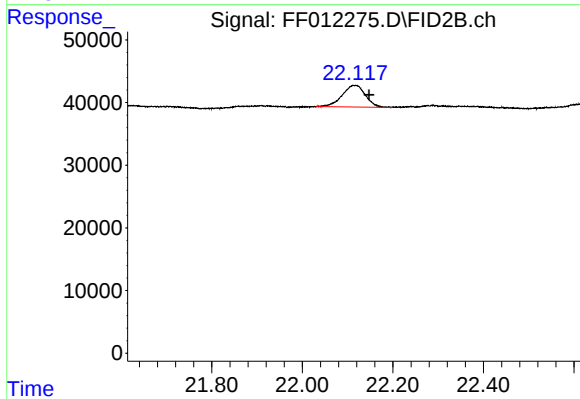

#18 N-TETRACONTANE

R.T.: 22.117 min
Delta R.T.: -0.031 min
Response: 122607
Conc: 1.35 ug/ml