

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031523\
 Data File : FF012278.D
 Signal(s) : FID2B.ch
 Acq On : 15 Mar 2023 10:16
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 15 14:30:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
 Quant Title :
 QLast Update : Tue Feb 21 16:12:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.749	2032512	14.960 ug/ml
12)	N-OCTACOSANE	17.198	2167198	17.657 ug/ml
13)	N-TRIACONTANE	18.085	113606	0.973 ug/ml
14)	N-DOTRIACONTANE	18.915	26960	0.242 ug/ml
16)	N-HEXATRIACONTANE	20.443	60146	0.634 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031523\
Data File : FF012278.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2023 10:16
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 15 14:30:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

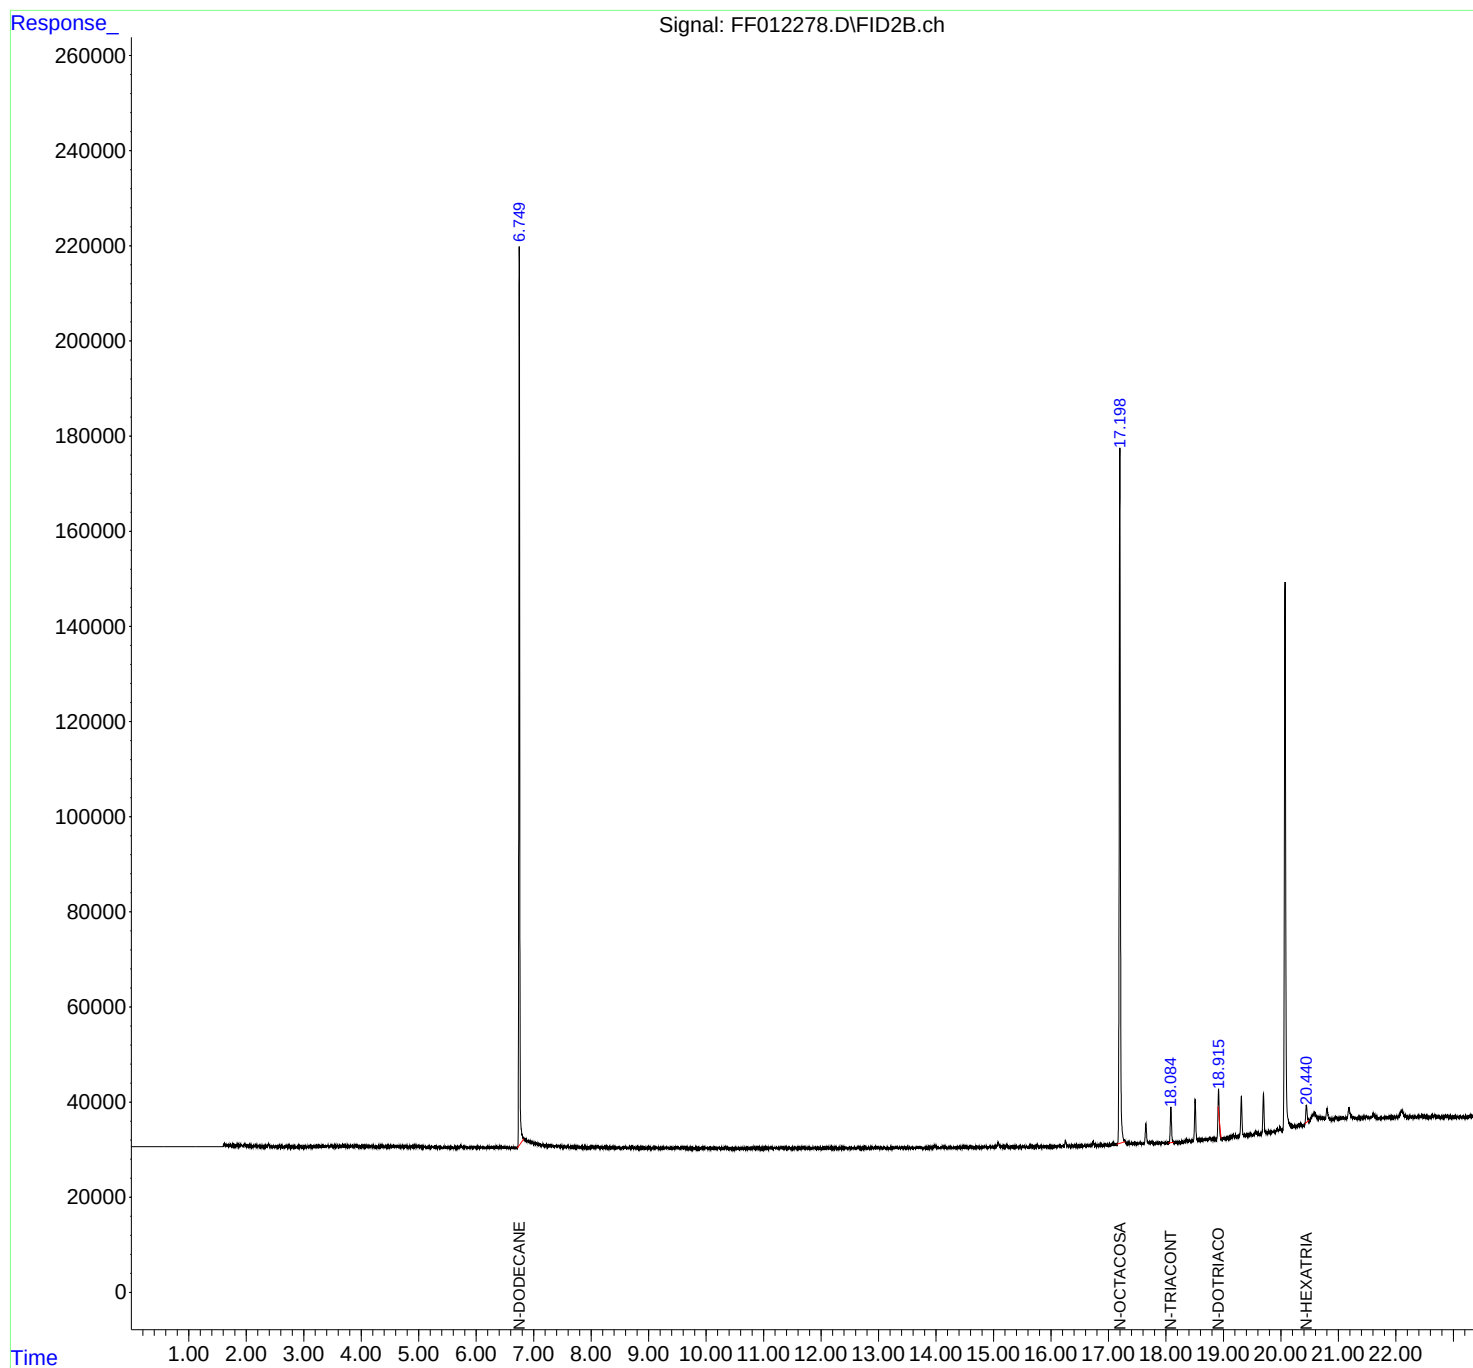


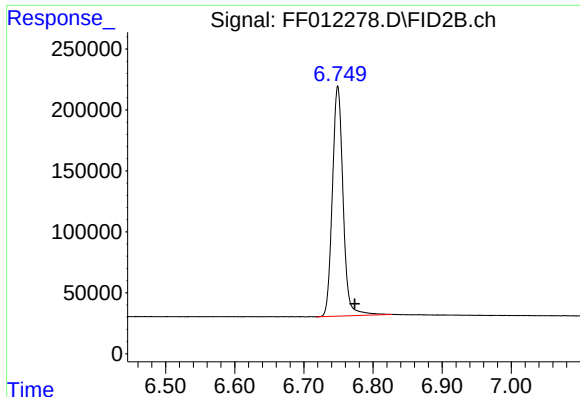

#3 N-DODECANE


R.T.: 6.749 min
Delta R.T.: -0.025 min
Response: 2032512
Conc: 14.96 ug/ml

Instrument :
FID_F
ClientSampleId :

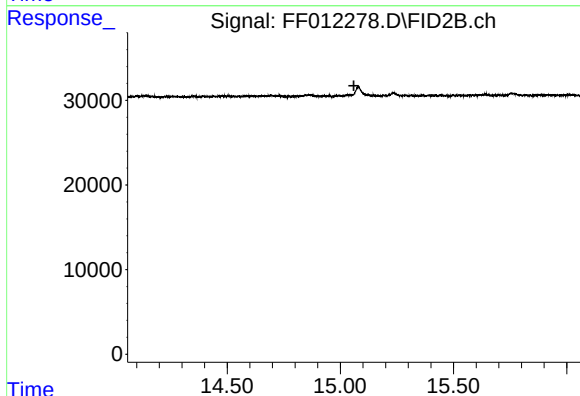


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.060 min
Response: 0
Conc: N.D.

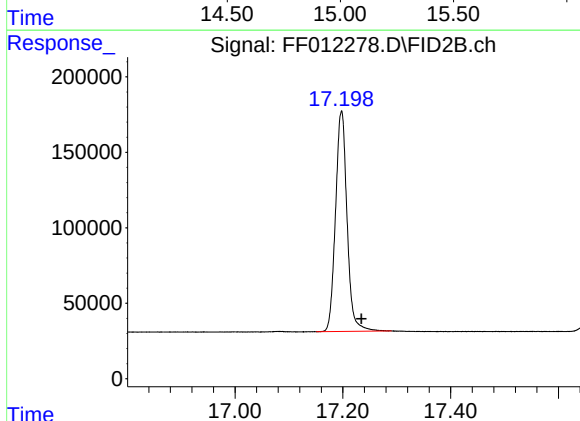


#12 N-OCTACOSANE

R.T.: 17.198 min
Delta R.T.: -0.037 min
Response: 2167198
Conc: 17.66 ug/ml

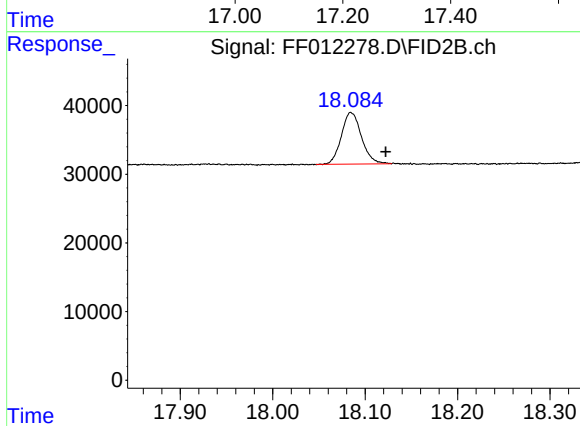

#13 N-TRIACONTANE


R.T.: 18.085 min
Delta R.T.: -0.038 min
Response: 113606
Conc: 0.97 ug/ml

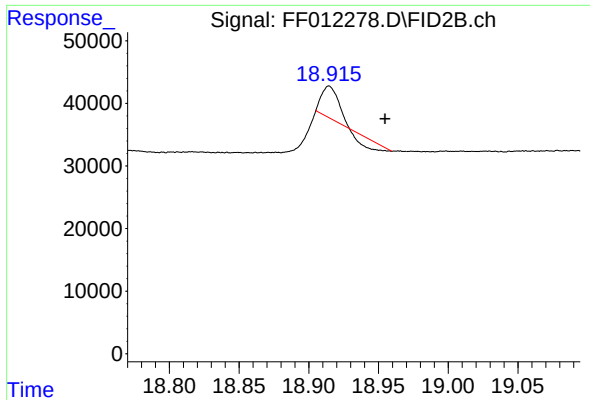

#14 N-DOTRIACONTANE

R.T.: 18.915 min
Delta R.T.: -0.040 min
Response: 26960
Conc: 0.24 ug/ml

Instrument :
FID_F
ClientSampleId :

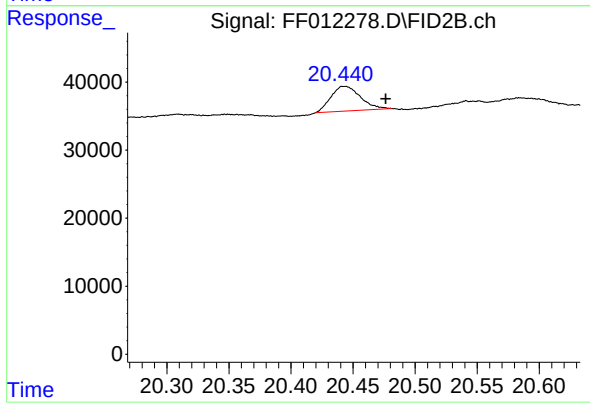

#16 N-HEXATRIACONTANE

R.T.: 20.443 min
Delta R.T.: -0.034 min
Response: 60146
Conc: 0.63 ug/ml