

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031524\
 Data File : FF014080.D
 Signal(s) : FID2B.ch
 Acq On : 15 Mar 2024 09:32
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 15 13:45:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031524.M
 Quant Title :
 QLast Update : Fri Mar 15 13:45:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.945	2027148	16.915 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.012	108923	0.863 ug/ml
14) N-DOTRIACONTANE	18.866	249455	1.974 ug/ml
16) N-HEXATRIACONTANE	20.420f	210836	2.880 ug/ml
18) N-TETRACONTANE	22.034	157004	2.555 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031524\
Data File : FF014080.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2024 09:32
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 15 13:45:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031524.M
Quant Title :
QLast Update : Fri Mar 15 13:45:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

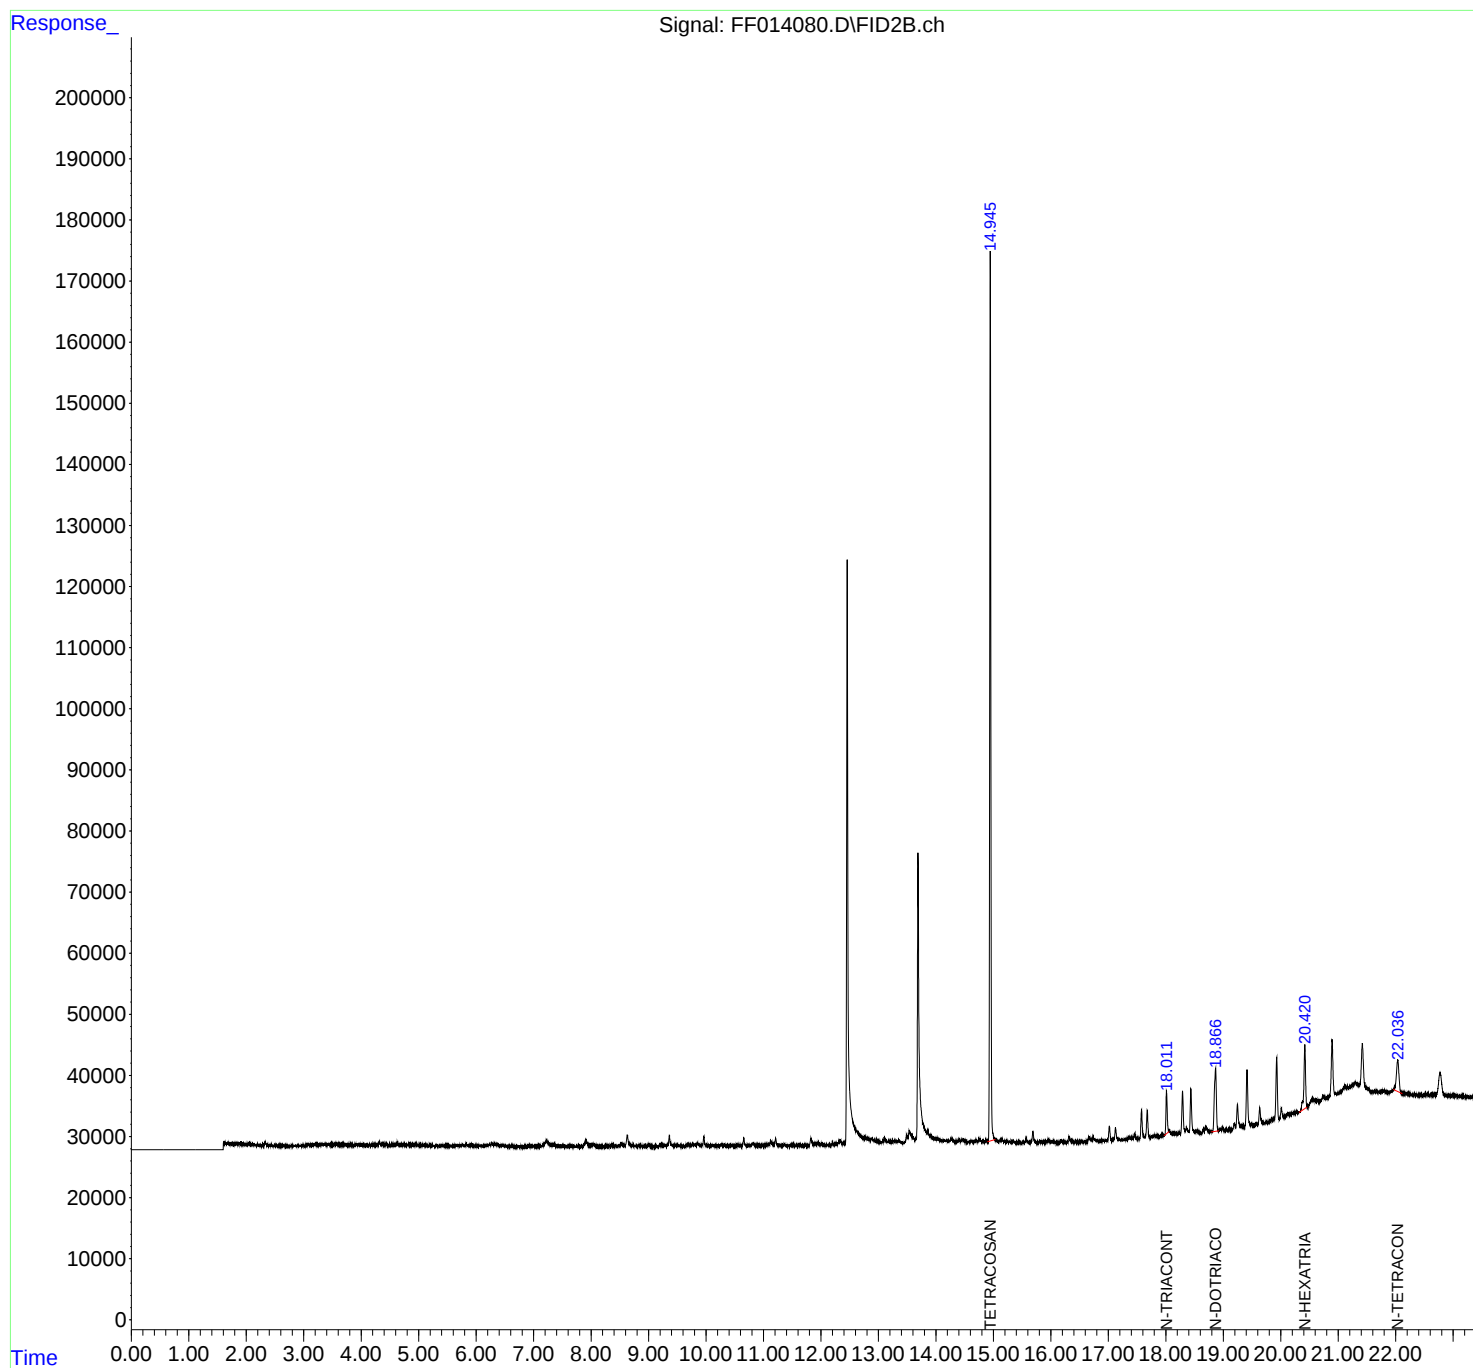

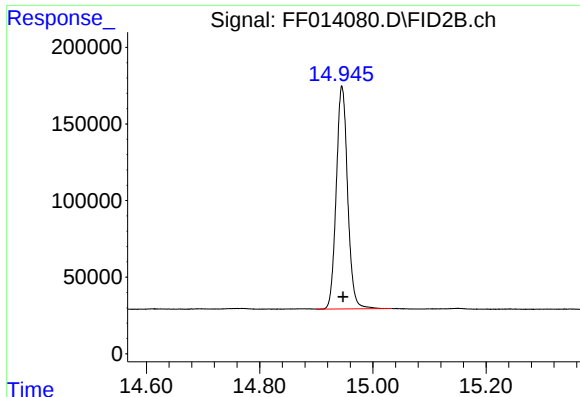


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.945 min
Delta R.T.: -0.002 min
Response: 2027148
Conc: 16.92 ug/ml

Instrument :


FID_F

ClientSampleId :

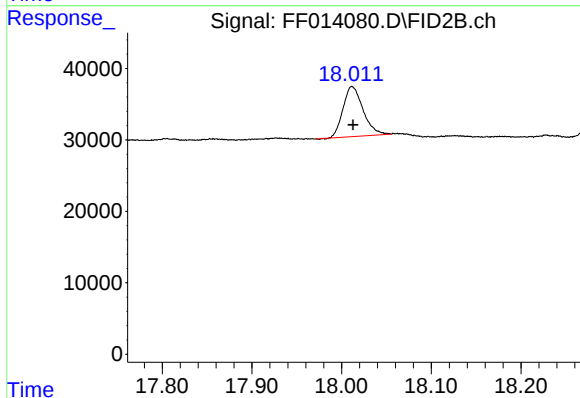


#13 N-TRIACONTANE

R.T.: 18.012 min
Delta R.T.: -0.001 min
Response: 108923
Conc: 0.86 ug/ml

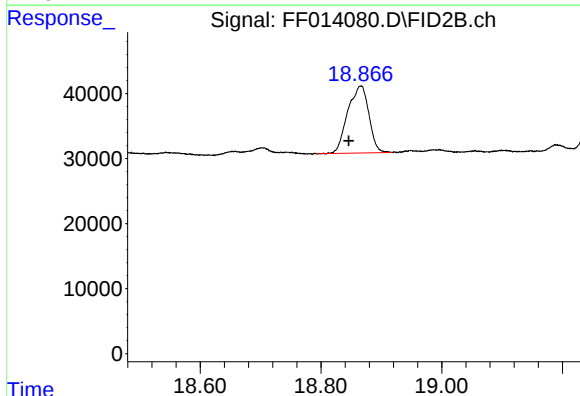


#14 N-DOTRIACONTANE

R.T.: 18.866 min
Delta R.T.: 0.020 min
Response: 249455
Conc: 1.97 ug/ml

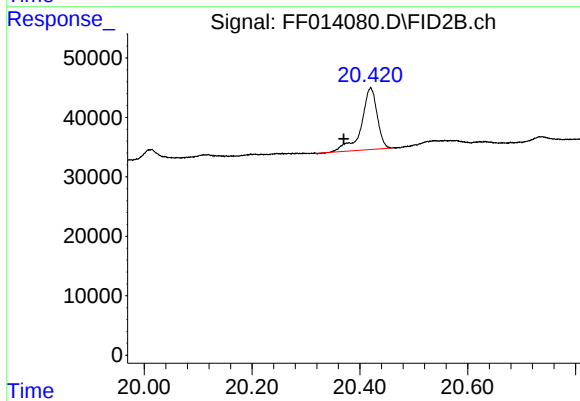

#16 N-HEXATRIACONTANE

R.T.: 20.420 min
Delta R.T.: 0.050 min
Response: 210836
Conc: 2.88 ug/ml

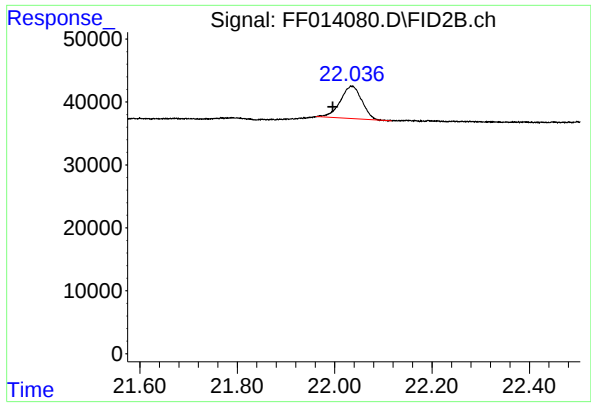

#18 N-TETRACONTANE

R.T.: 22.034 min
Delta R.T.: 0.038 min
Response: 157004
Conc: 2.55 ug/ml

Instrument :
FID_F
ClientSampleId :