

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031619\
 Data File : FF003850.D
 Signal(s) : FID2B.ch
 Acq On : 15 Mar 2019 13:18
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 15 22:54:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.585	2130390	15.301 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.492	140730	0.990 ug/ml
16) N-HEXATRIACONTANE	20.064	546376	4.187 ug/ml
18) N-TETRACONTANE	21.665	214214	1.722 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031619\
Data File : FF003850.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2019 13:18
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 15 22:54:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

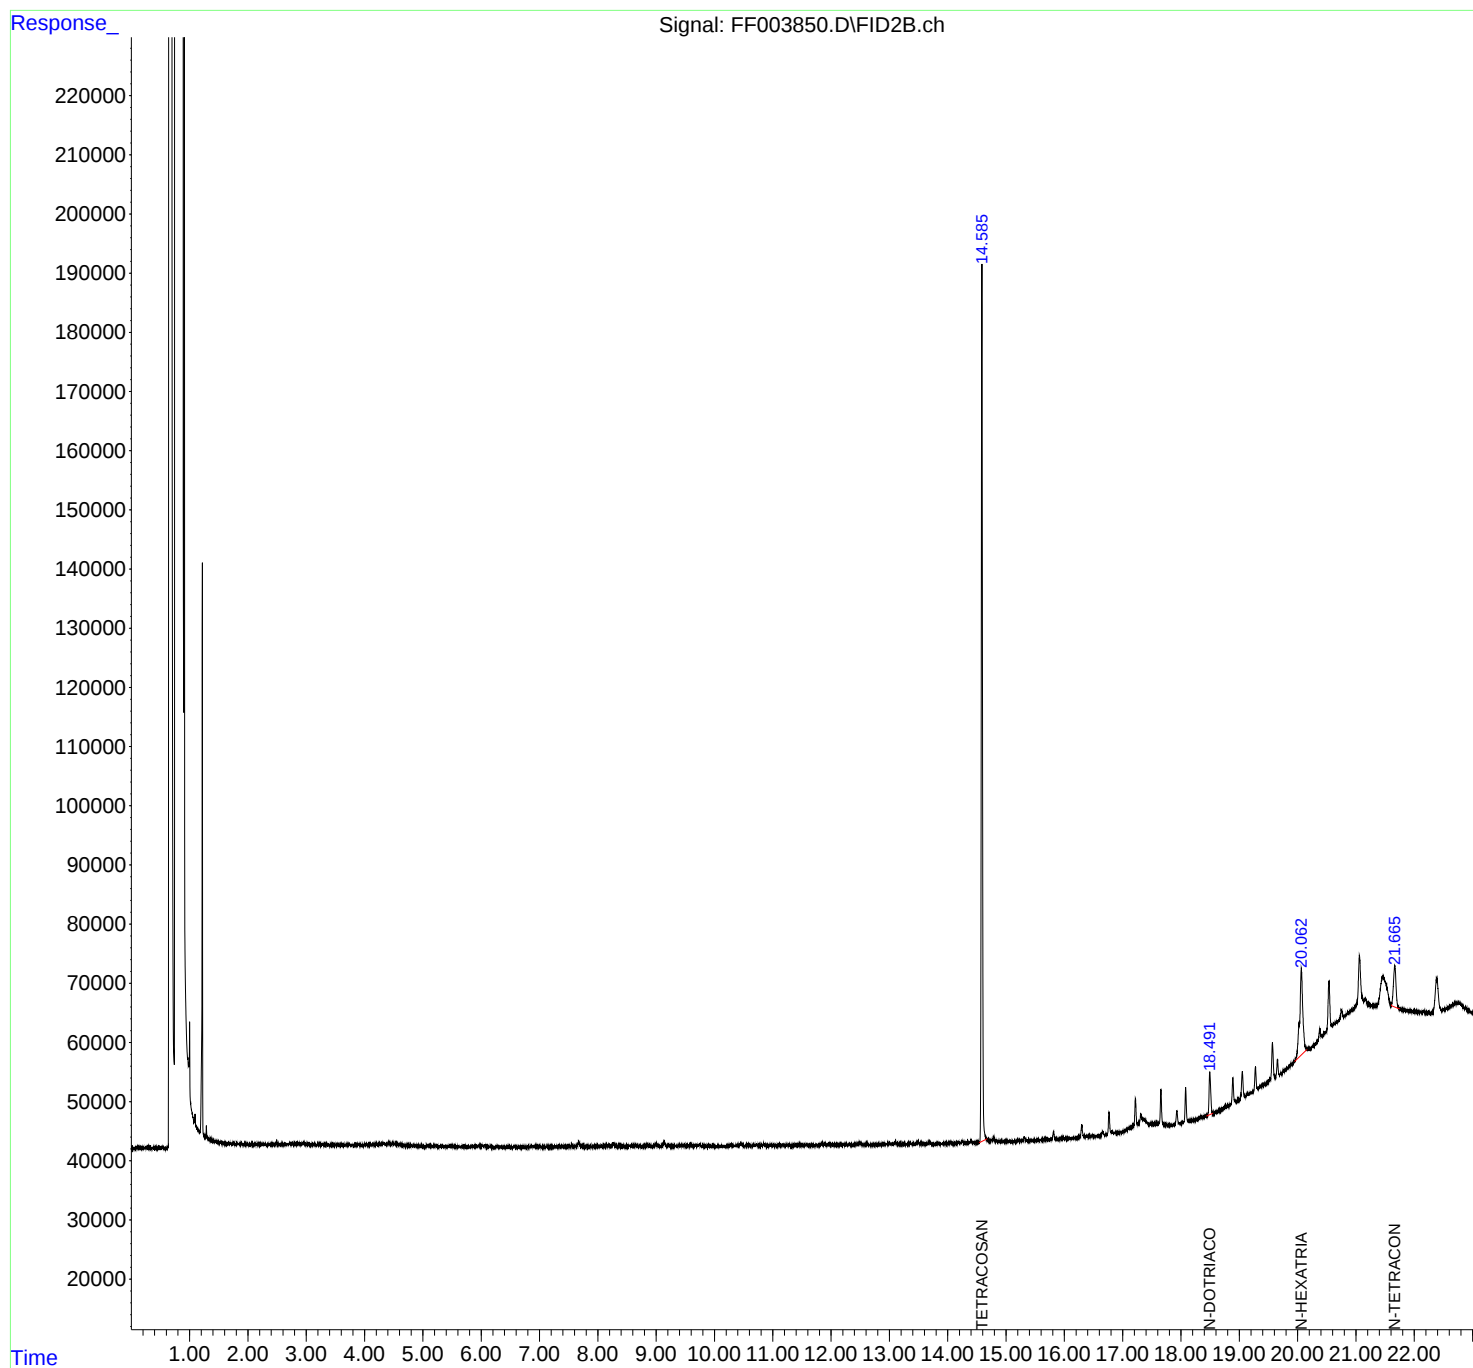


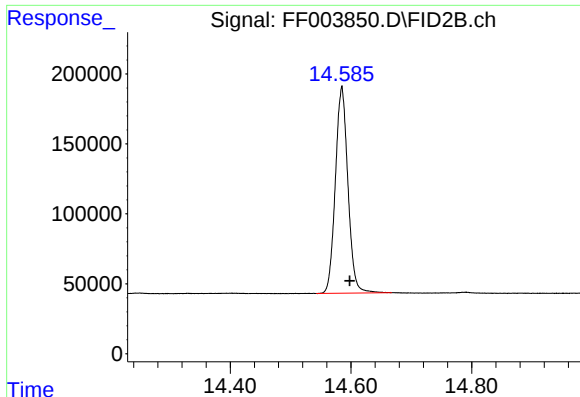

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.585 min
Delta R.T.: -0.013 min
Response: 2130390
Conc: 15.30 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

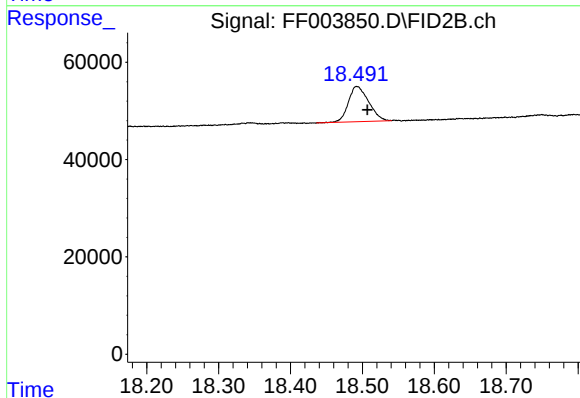


#14 N-DOTRIACONTANE

R.T.: 18.492 min
Delta R.T.: -0.014 min
Response: 140730
Conc: 0.99 ug/ml

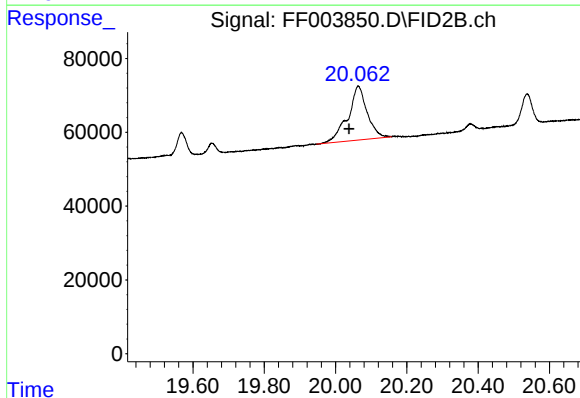

#16 N-HEXATRIACONTANE

R.T.: 20.064 min
Delta R.T.: 0.026 min
Response: 546376
Conc: 4.19 ug/ml

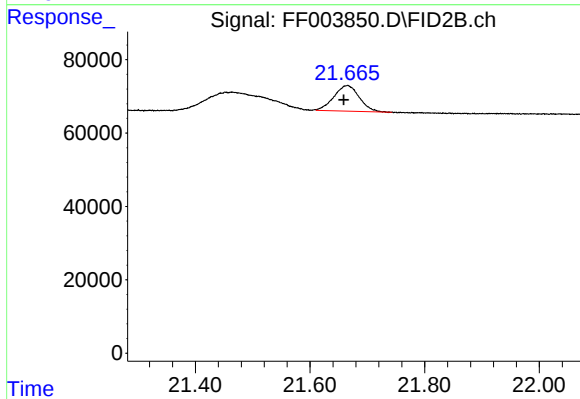

#18 N-TETRACONTANE

R.T.: 21.665 min
Delta R.T.: 0.006 min
Response: 214214
Conc: 1.72 ug/ml