

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031619\
 Data File : FF003852.D
 Signal(s) : FID2B.ch
 Acq On : 15 Mar 2019 14:19
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Mar 15 22:55:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.335	3642371	23.339 ug/ml
12) N-OCTACOSANE	16.766	3403211	22.521 ug/ml
13) N-TRIACONTANE	17.653	372566	2.533 ug/ml
14) N-DOTRIACONTANE	18.490	450573	3.168 ug/ml
15) N-TETRATRIACONTANE	19.275	303580	2.267 ug/ml
16) N-HEXATRIACONTANE	20.019	72274	0.554 ug/ml
17) N-OCTATRIACONTANE	20.752	113969	0.987 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031619\
Data File : FF003852.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2019 14:19
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 15 22:55:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

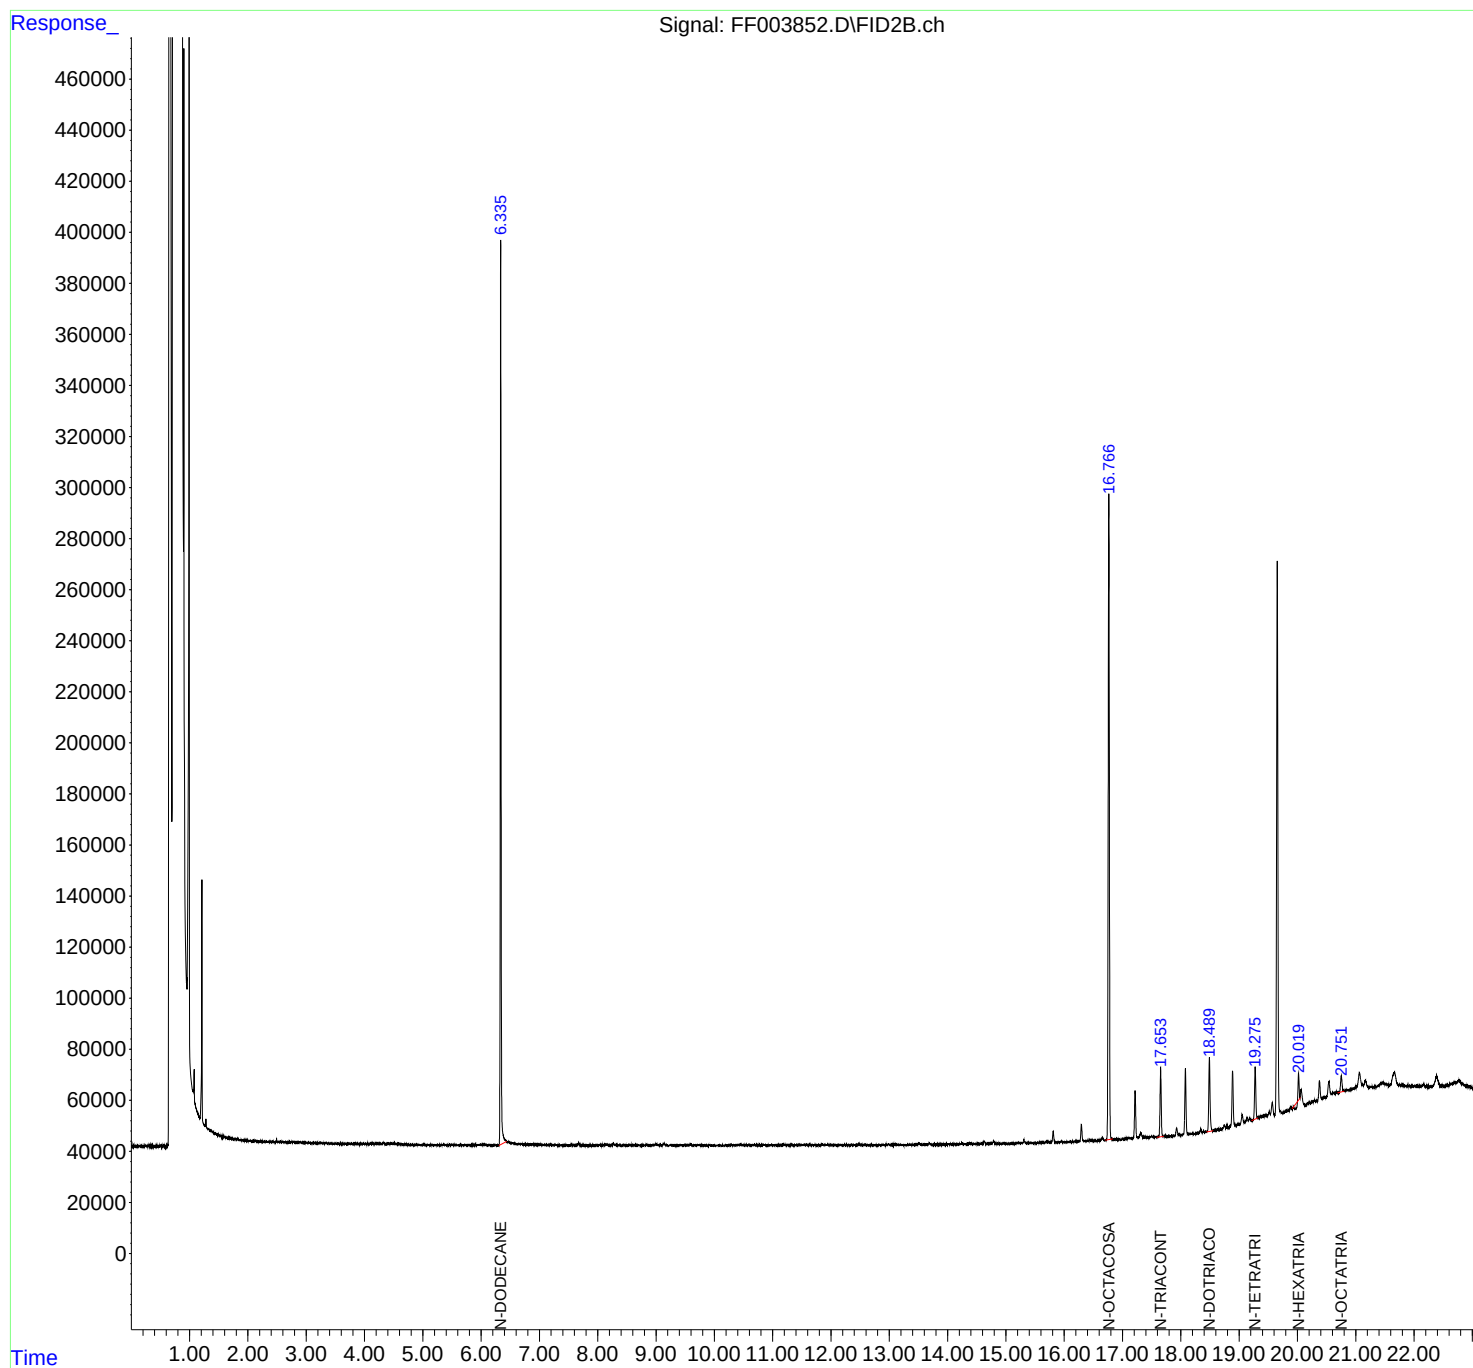


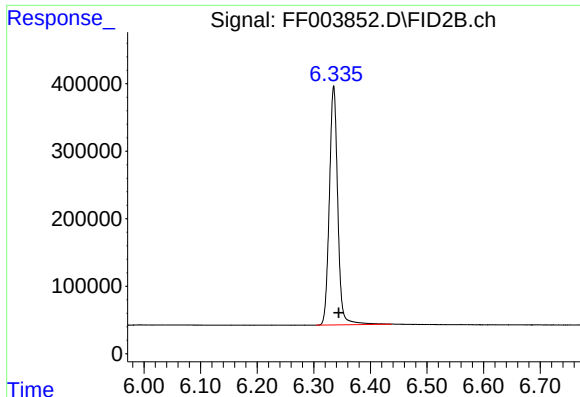

#3 N-DODECANE


R.T.: 6.335 min
Delta R.T.: -0.009 min
Response: 3642371
Conc: 23.34 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

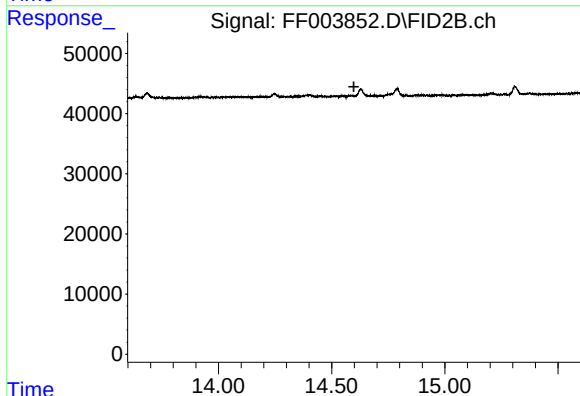


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.598 min
Response: 0
Conc: N.D.

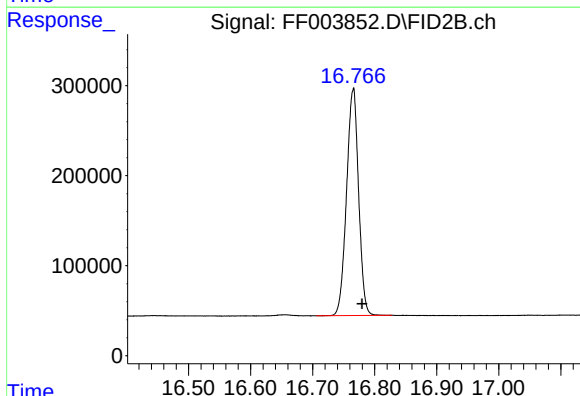


#12 N-OCTACOSANE

R.T.: 16.766 min
Delta R.T.: -0.014 min
Response: 3403211
Conc: 22.52 ug/ml

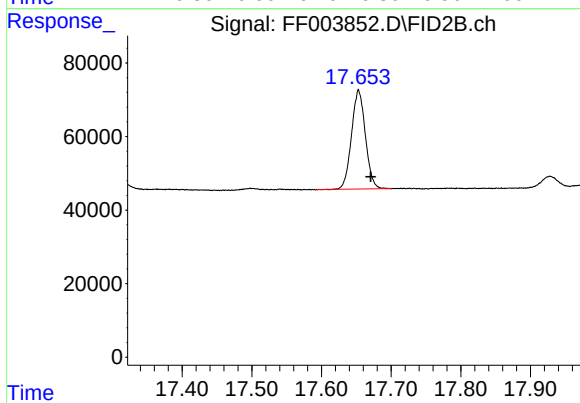

#13 N-TRIACONTANE


R.T.: 17.653 min
Delta R.T.: -0.018 min
Response: 372566
Conc: 2.53 ug/ml

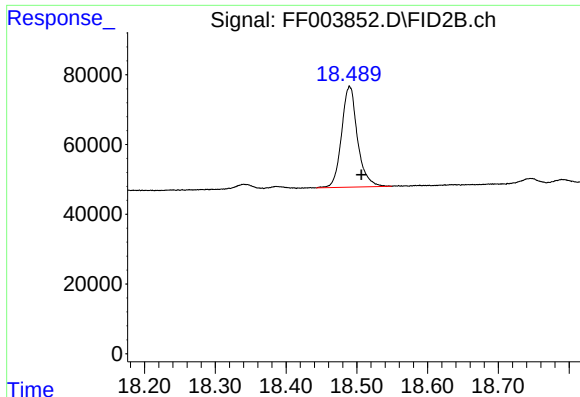

#14 N-DOTRIACONTANE


R.T.: 18.490 min
Delta R.T.: -0.017 min
Response: 450573
Conc: 3.17 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

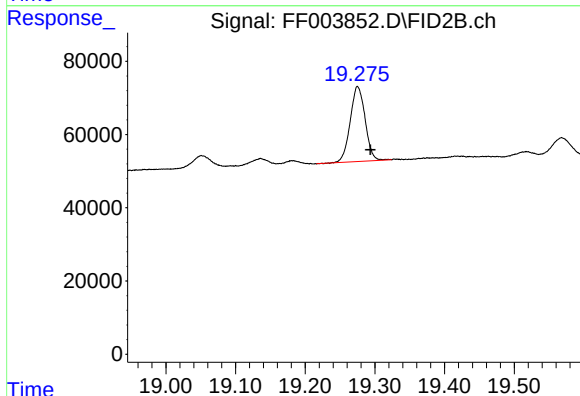


#15 N-TETRATRIACONTANE

R.T.: 19.275 min
Delta R.T.: -0.018 min
Response: 303580
Conc: 2.27 ug/ml

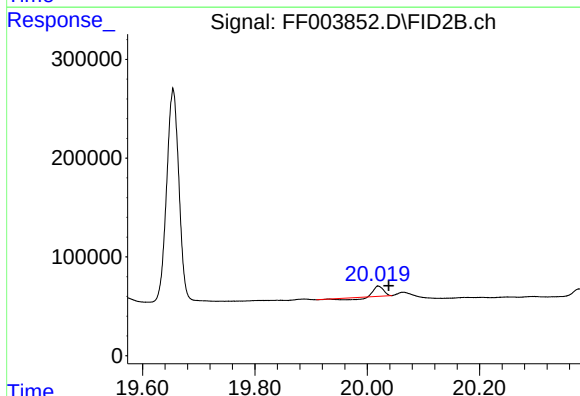

#16 N-HEXATRIACONTANE

R.T.: 20.019 min
Delta R.T.: -0.019 min
Response: 72274
Conc: 0.55 ug/ml

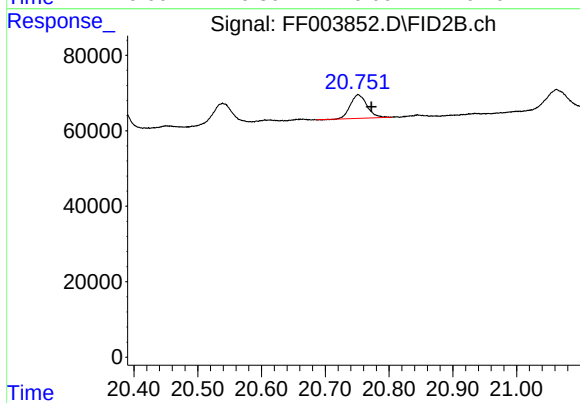

#17 N-OCTATRIACONTANE

R.T.: 20.752 min
Delta R.T.: -0.021 min
Response: 113969
Conc: 0.99 ug/ml