

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031619\
Data File : FF003853.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2019 14:58
Operator : AJ\SJ
Sample : PB117957BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB117957BL

Integration File: autoint1.e
Quant Time: Mar 15 22:55:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.584	1558227	11.192 ug/ml
Target Compounds				
16)	N-HEXATRIACONTANE	20.067	215582	1.652 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031619\
Data File : FF003853.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2019 14:58
Operator : AJ\SJ
Sample : PB117957BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB117957BL

Integration File: autoint1.e
Quant Time: Mar 15 22:55:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

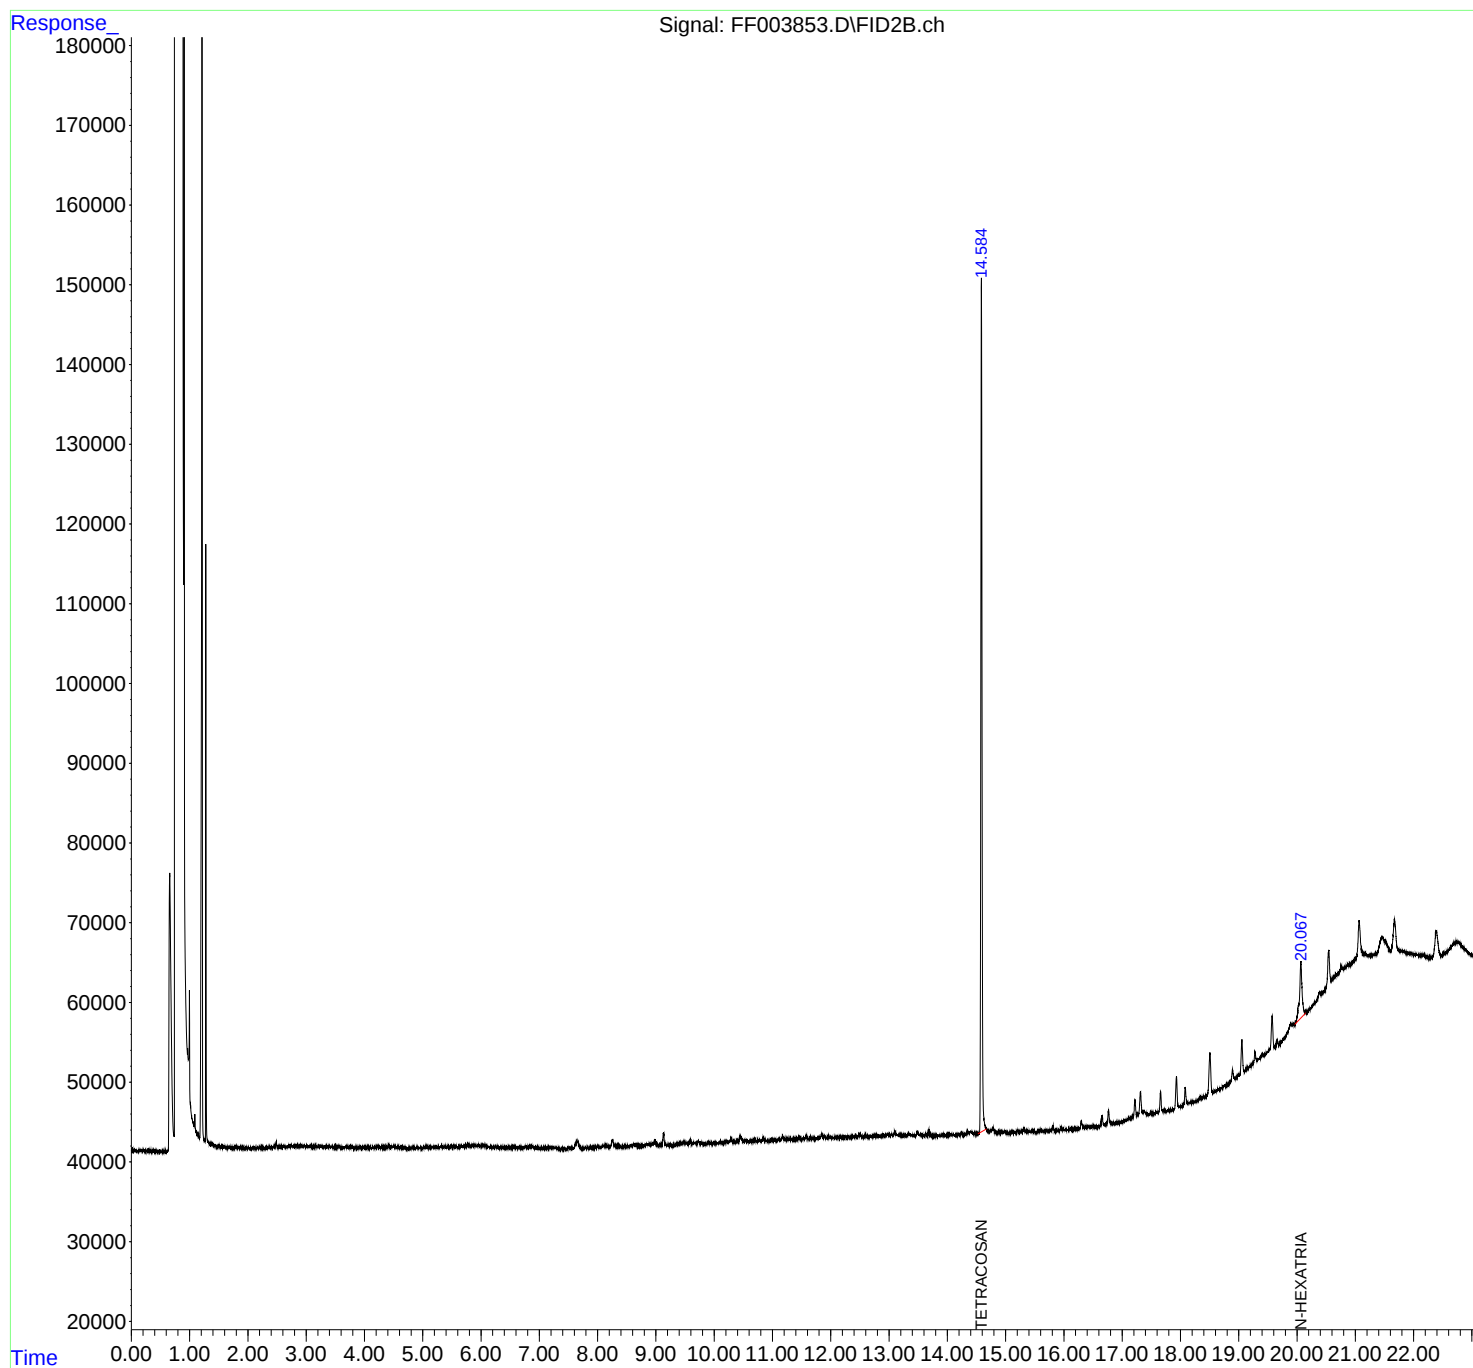


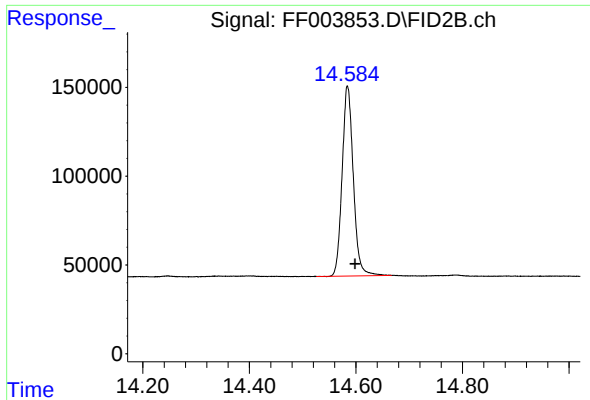

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.584 min
Delta R.T.: -0.014 min
Response: 1558227
Conc: 11.19 ug/ml

Instrument :
FID_F
ClientSampleId :
PB117957BL

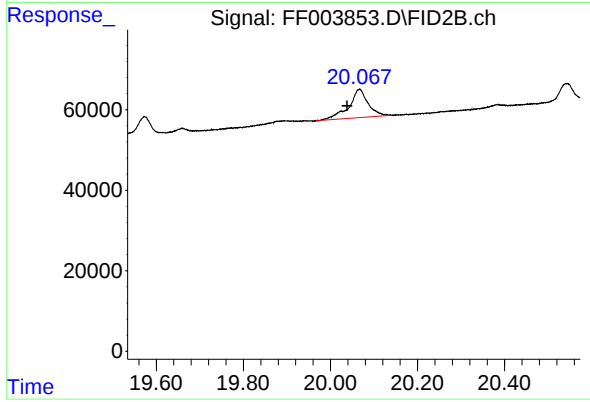

#16 N-HEXATRIACONTANE

R.T.: 20.067 min
Delta R.T.: 0.029 min
Response: 215582
Conc: 1.65 ug/ml