

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031619\
 Data File : FF003857.D
 Signal(s) : FID2B.ch
 Acq On : 15 Mar 2019 17:00
 Operator : AJ\SJ
 Sample : K1908-05
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 93-94

Integration File: autoint1.e
 Quant Time: Mar 15 23:00:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.587	1279095	9.187 ug/ml
Target Compounds			
4) N-TETRADECANE	8.191f	164724	1.027 ug/ml
11) N-HEXACOSANE	15.814	89925	0.583 ug/ml
12) N-OCTACOSANE	16.768	184627	1.222 ug/ml
13) N-TRIACONTANE	17.659	327450	2.226 ug/ml
14) N-DOTRIACONTANE	18.494	337661	2.374 ug/ml
15) N-TETRATRIACONTANE	19.272	84319	0.630 ug/ml
16) N-HEXATRIACONTANE	20.026	127946	0.981 ug/ml
18) N-TETRACONTANE	21.675	236035	1.897 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031619\
Data File : FF003857.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2019 17:00
Operator : AJ\SJ
Sample : K1908-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
93-94

Integration File: autoint1.e
Quant Time: Mar 15 23:00:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

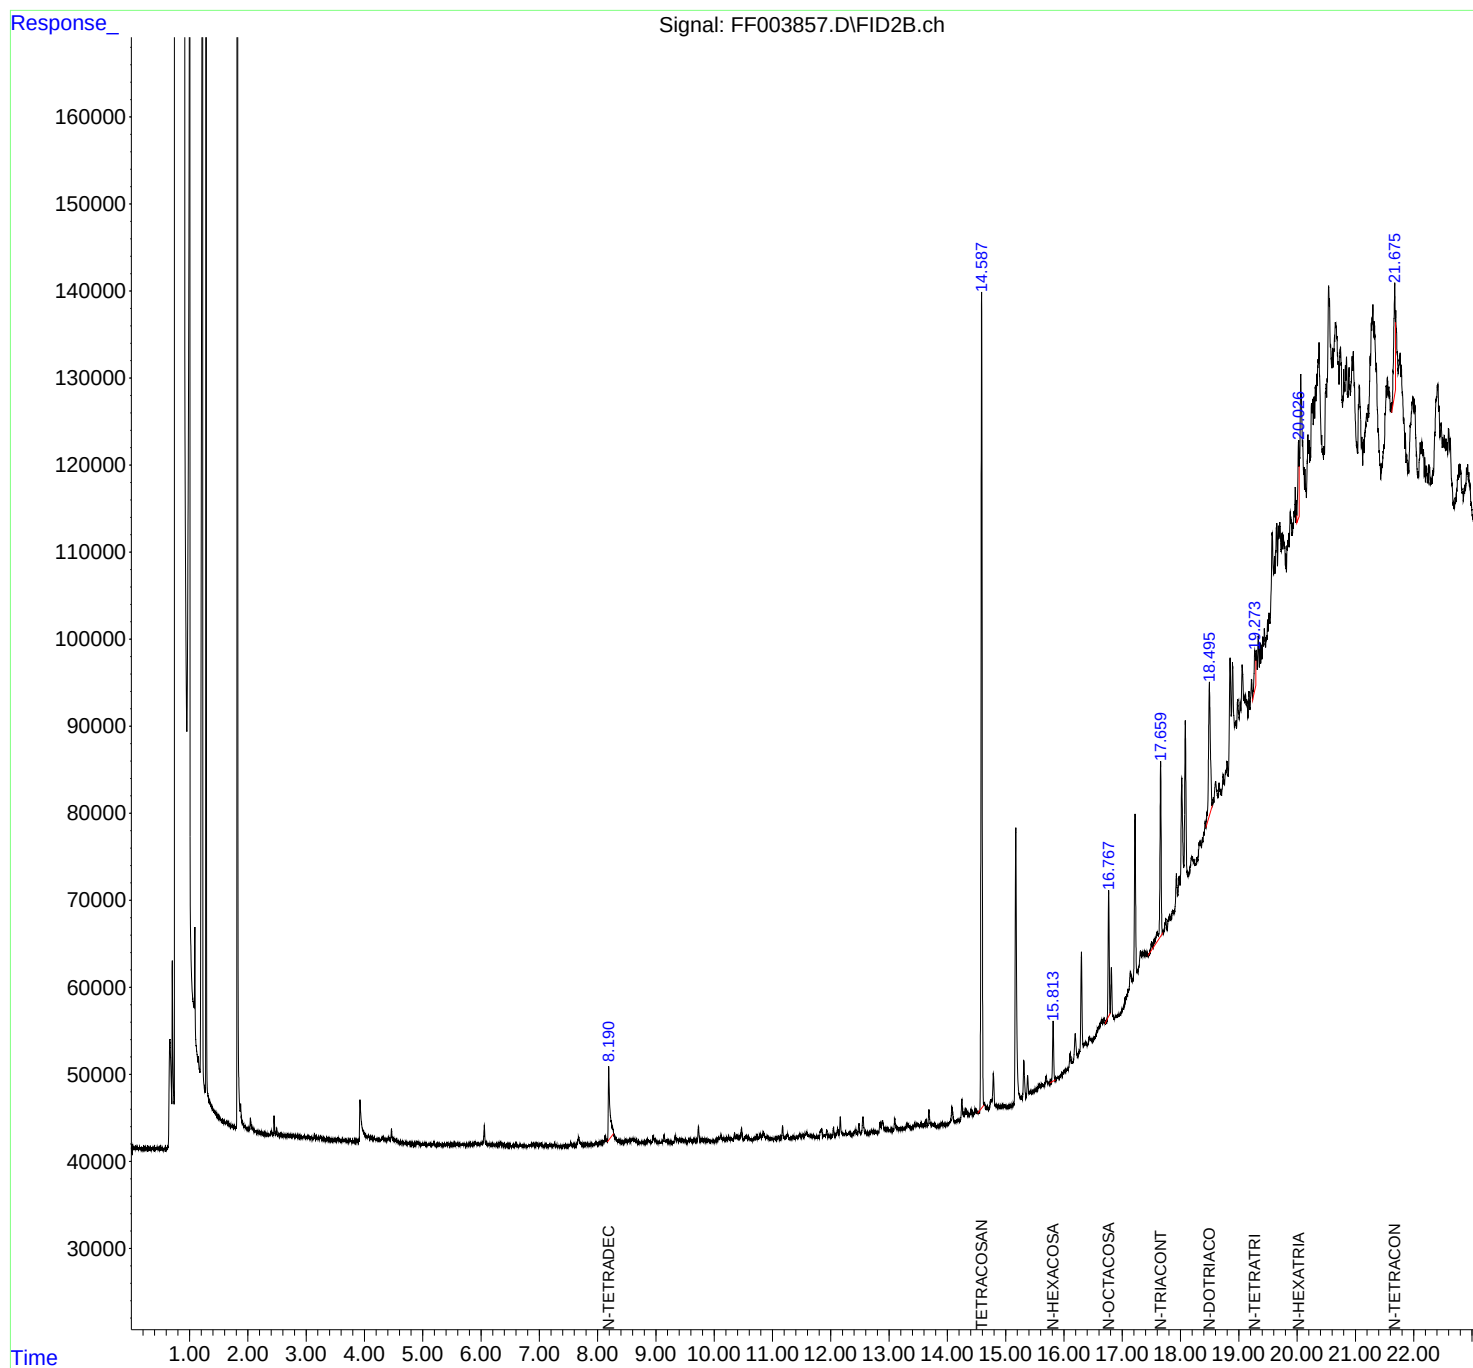


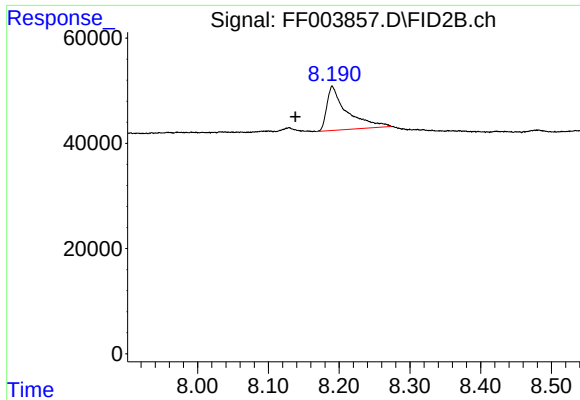

#4 N-TETRADECANE


R.T.: 8.191 min
Delta R.T.: 0.052 min
Response: 164724
Conc: 1.03 ug/ml

Instrument :
FID_F
ClientSampleId :
93-94

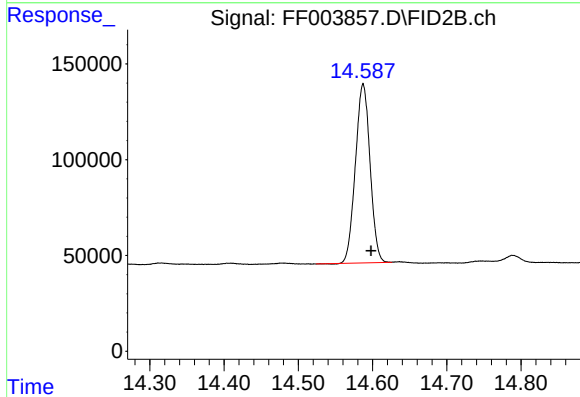


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.587 min
Delta R.T.: -0.011 min
Response: 1279095
Conc: 9.19 ug/ml

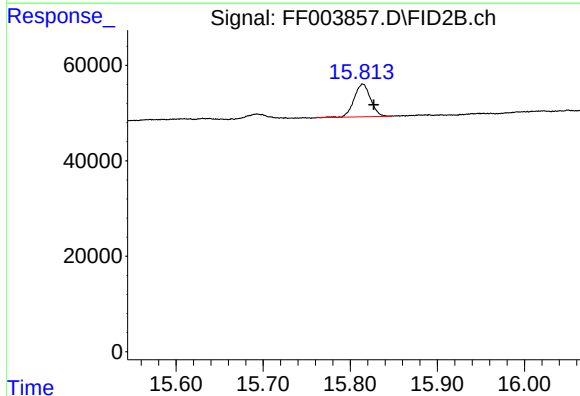


#11 N-HEXACOSANE

R.T.: 15.814 min
Delta R.T.: -0.012 min
Response: 89925
Conc: 0.58 ug/ml

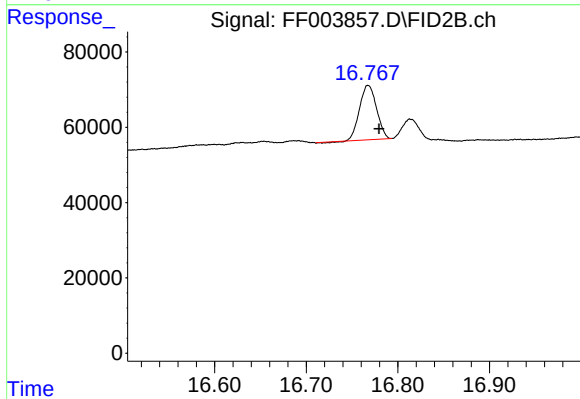

#12 N-OCTACOSANE


R.T.: 16.768 min
Delta R.T.: -0.012 min
Response: 184627
Conc: 1.22 ug/ml

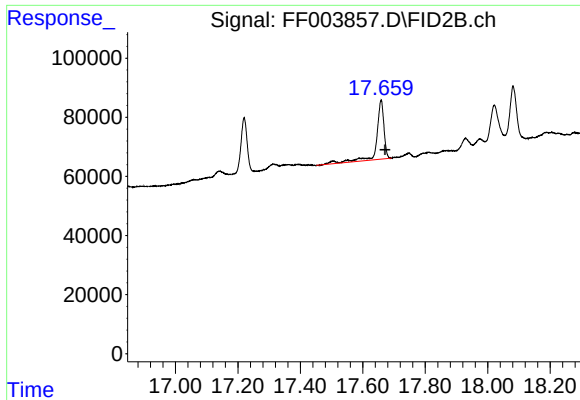

#13 N-TRIACONTANE


R.T.: 17.659 min
Delta R.T.: -0.012 min
Response: 327450
Conc: 2.23 ug/ml

Instrument :
FID_F
ClientSampleId :
93-94

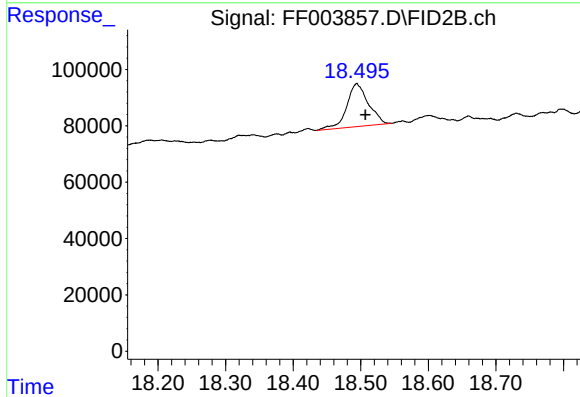


#14 N-DOTRIACONTANE

R.T.: 18.494 min
Delta R.T.: -0.013 min
Response: 337661
Conc: 2.37 ug/ml

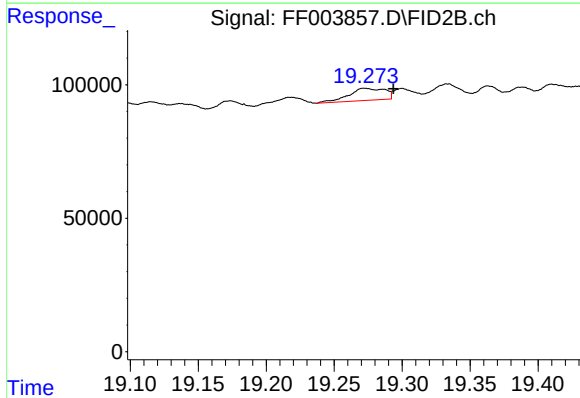


#15 N-TETRATRIACONTANE

R.T.: 19.272 min
Delta R.T.: -0.021 min
Response: 84319
Conc: 0.63 ug/ml

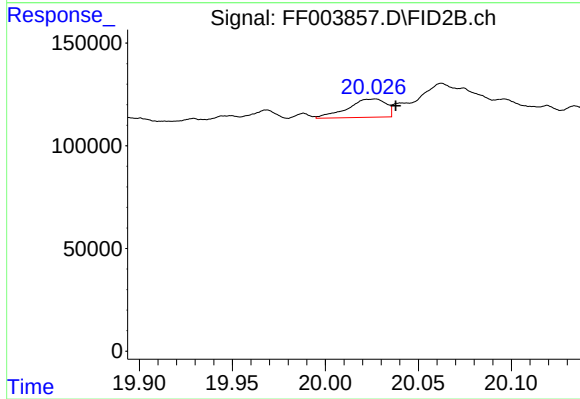

#16 N-HEXATRIACONTANE

R.T.: 20.026 min
Delta R.T.: -0.011 min
Response: 127946
Conc: 0.98 ug/ml

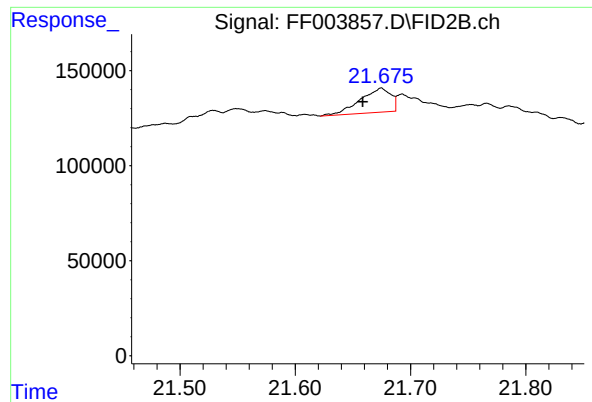

#18 N-TETRACONTANE

R.T.: 21.675 min
Delta R.T.: 0.016 min
Response: 236035
Conc: 1.90 ug/ml

Instrument :
FID_F
ClientSampleId :
93-94