

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031619\
 Data File : FF003861.D
 Signal(s) : FID2B.ch
 Acq On : 15 Mar 2019 19:03
 Operator : AJ\SJ
 Sample : K1908-03 10X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 101-102

Integration File: autoint1.e
 Quant Time: Mar 15 23:01:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.585	177352	1.274 ug/ml
Target Compounds			
7) N-EICOSANE	12.537	703842	4.302 ug/ml
10) N-TETRACOSANE	14.765	390629	2.469 ug/ml
12) N-OCTACOSANE	16.776	158030	1.046 ug/ml
13) N-TRIACONTANE	17.654	172959	1.176 ug/ml
14) N-DOTRIACONTANE	18.494	172687	1.214 ug/ml
15) N-TETRATRIACONTANE	19.301	100680	0.752 ug/ml
16) N-HEXATRIACONTANE	20.074	196227	1.504 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031619\
Data File : FF003861.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2019 19:03
Operator : AJ\SJ
Sample : K1908-03 10X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
101-102

Integration File: autoint1.e
Quant Time: Mar 15 23:01:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

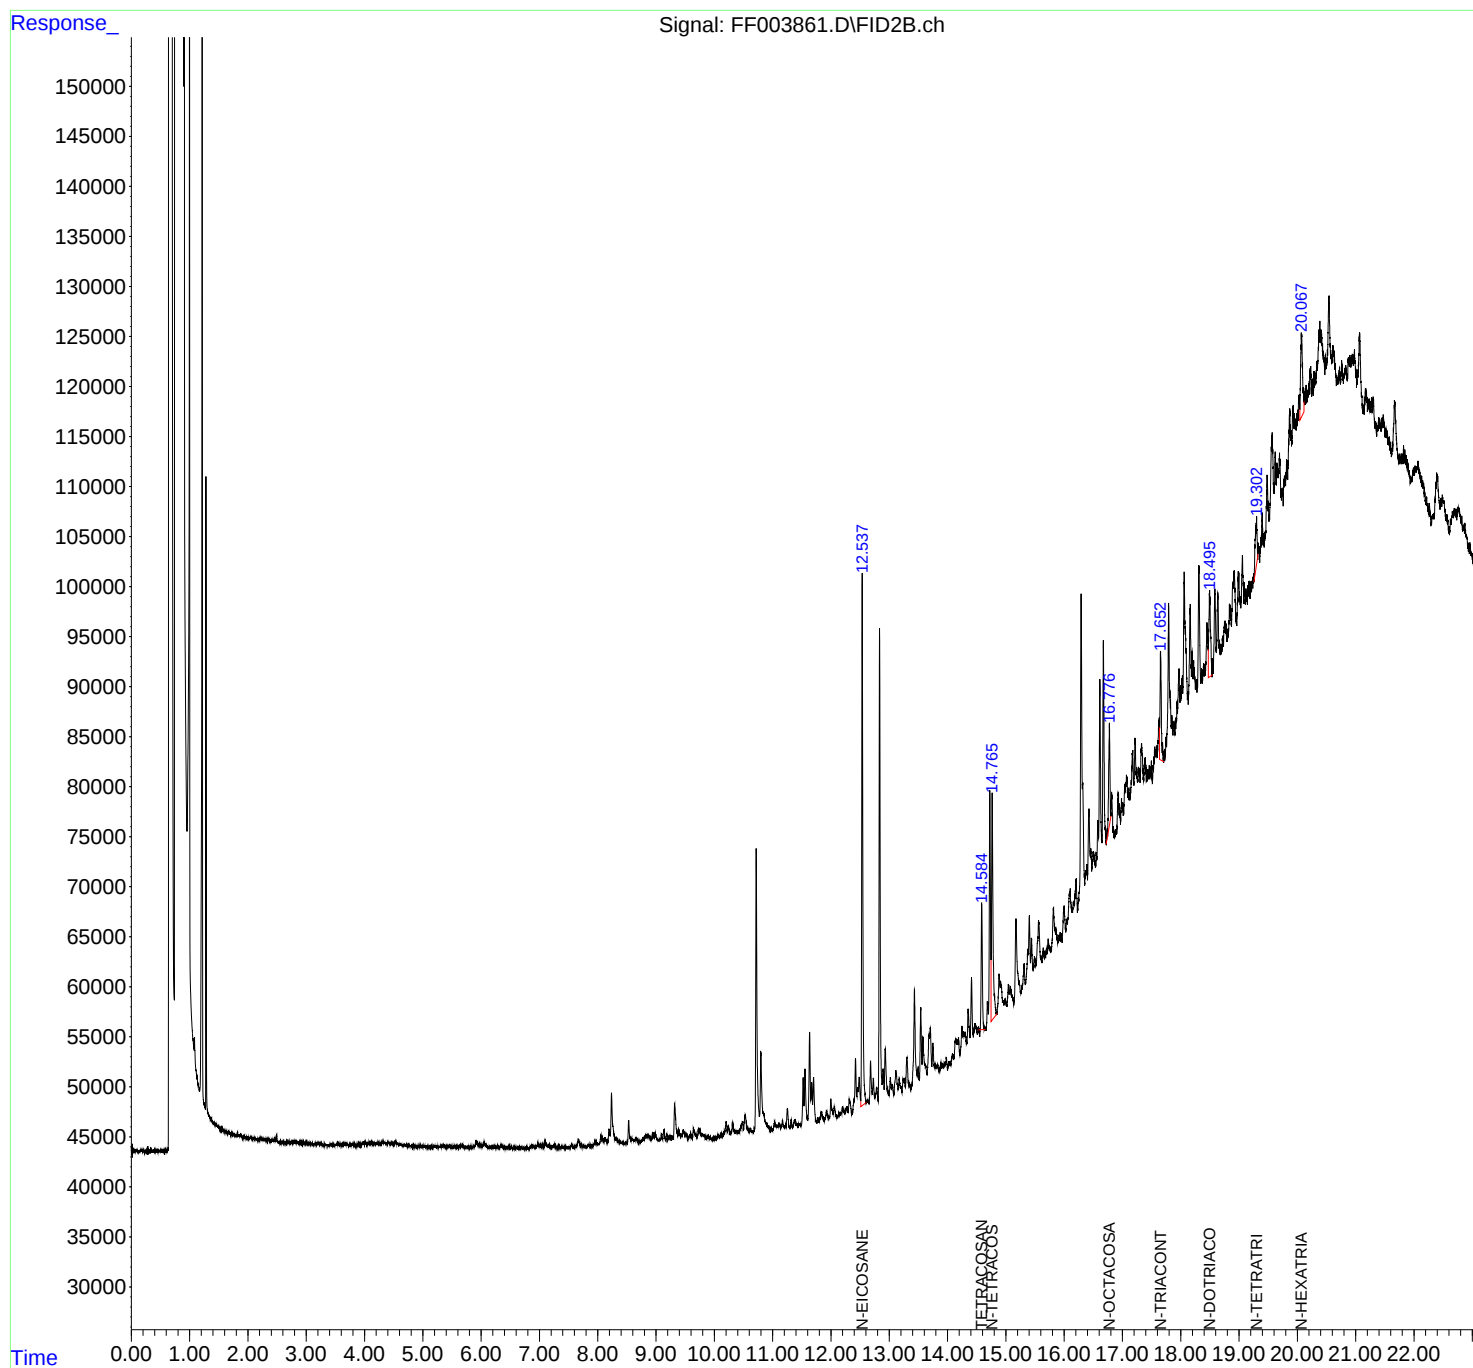


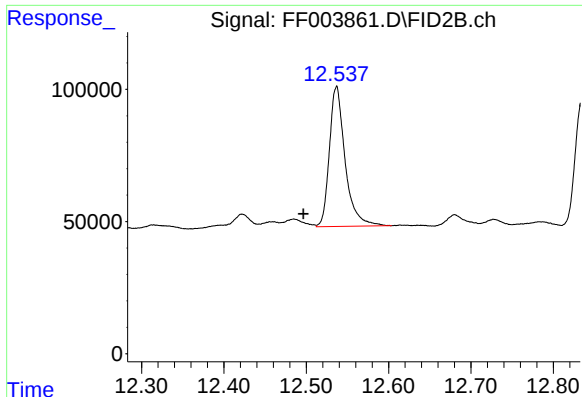

#7 N-EICOSANE


R.T.: 12.537 min
Delta R.T.: 0.040 min
Response: 703842
Conc: 4.30 ug/ml

Instrument :
FID_F
ClientSampleId :
101-102

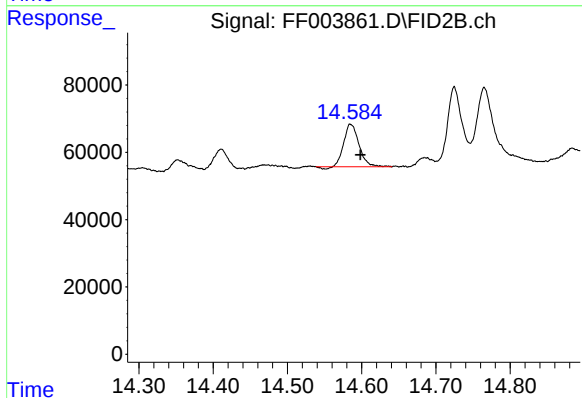


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.585 min
Delta R.T.: -0.013 min
Response: 177352
Conc: 1.27 ug/ml

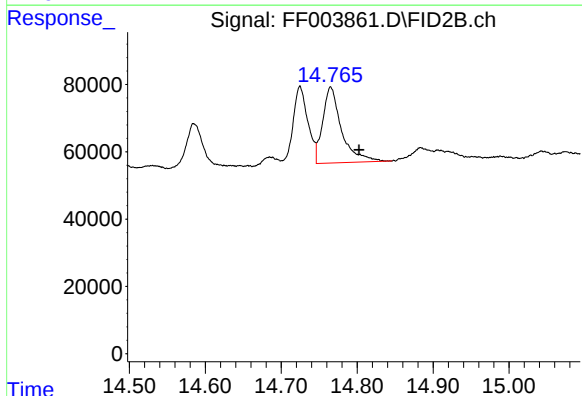


#10 N-TETRACOSANE

R.T.: 14.765 min
Delta R.T.: -0.037 min
Response: 390629
Conc: 2.47 ug/ml

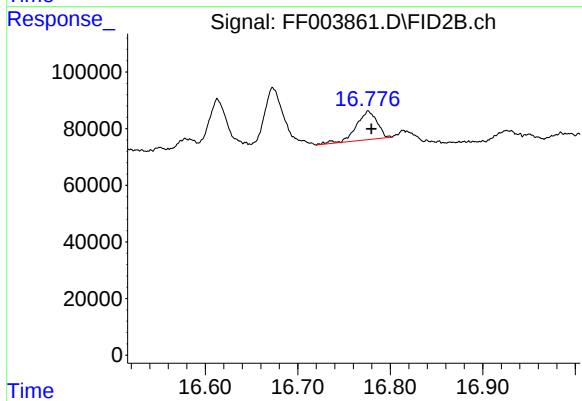

#12 N-OCTACOSANE


R.T.: 16.776 min
Delta R.T.: -0.003 min
Response: 158030
Conc: 1.05 ug/ml

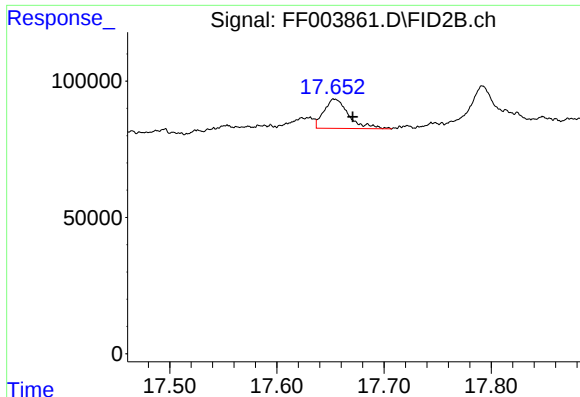

#13 N-TRIACONTANE


R.T.: 17.654 min
Delta R.T.: -0.017 min
Response: 172959
Conc: 1.18 ug/ml

Instrument :
FID_F
ClientSampleId :
101-102

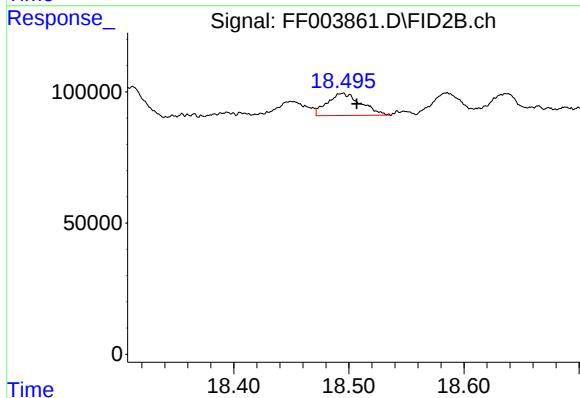


#14 N-DOTRIACONTANE

R.T.: 18.494 min
Delta R.T.: -0.012 min
Response: 172687
Conc: 1.21 ug/ml

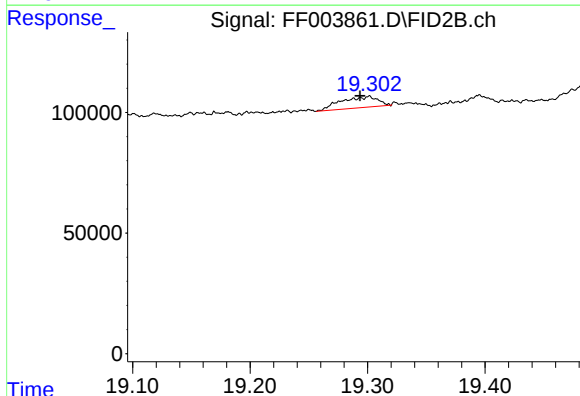

#15 N-TETRATRIACONTANE

R.T.: 19.301 min
Delta R.T.: 0.008 min
Response: 100680
Conc: 0.75 ug/ml

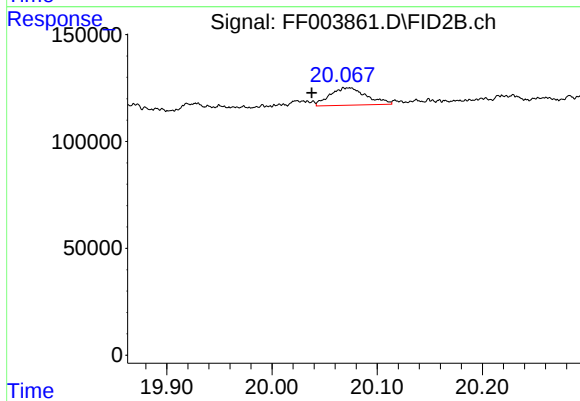

#16 N-HEXATRIACONTANE

R.T.: 20.074 min
Delta R.T.: 0.036 min
Response: 196227
Conc: 1.50 ug/ml