

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031619\
Data File : FF003852.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2019 14:19
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 15 22:55:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.335	3642371	23.339 ug/ml
12)	N-OCTACOSANE	16.766	3403211	22.521 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031619\
Data File : FF003852.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2019 14:19
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 15 22:55:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

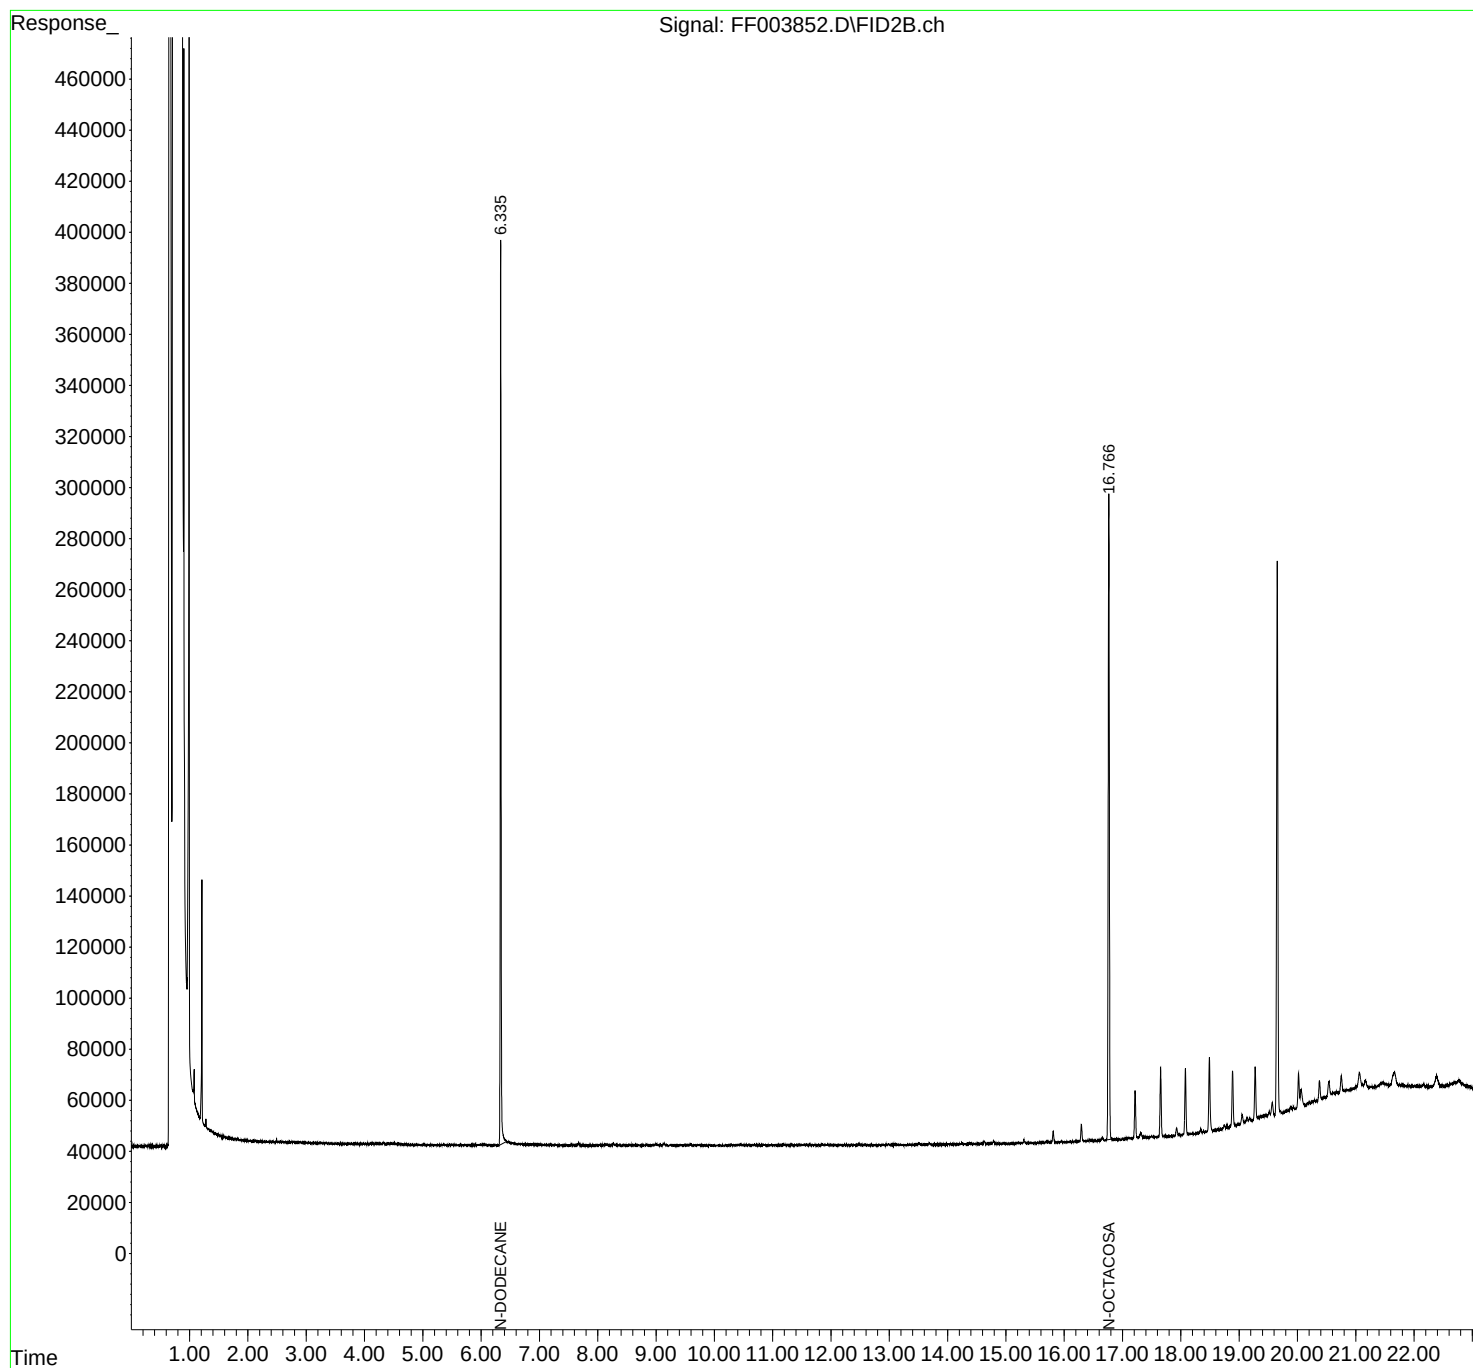


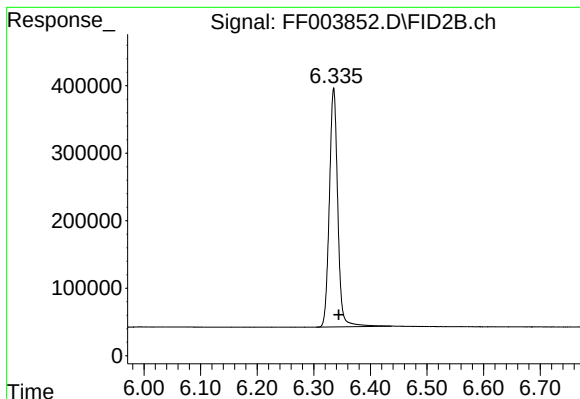

#3 N-DODECANE


R.T.: 6.335 min
Delta R.T.: -0.009 min
Response: 3642371
Conc: 23.34 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

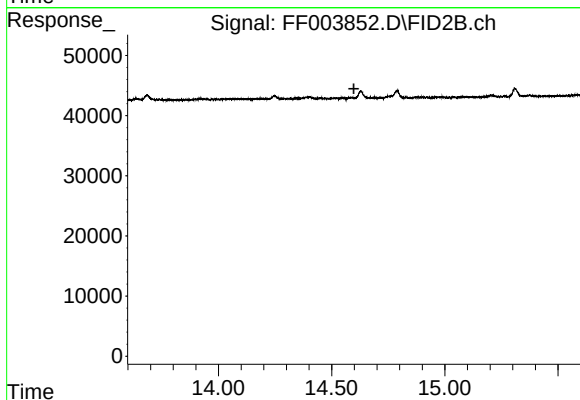

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.598 min
Response: 0
Conc: N.D.

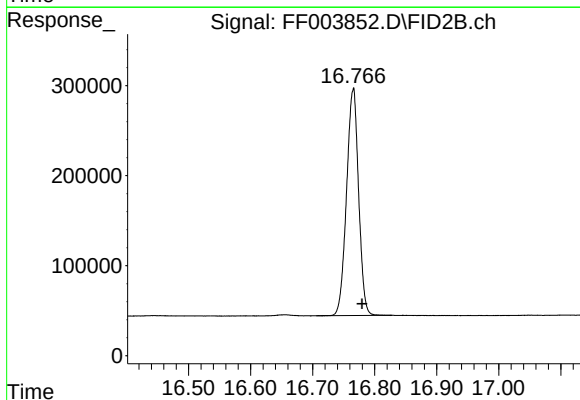

#12 N-OCTACOSANE

R.T.: 16.766 min
Delta R.T.: -0.014 min
Response: 3403211
Conc: 22.52 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

rteres

Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031619\
Data File : FF003852.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2019 14:19
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e

Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Title :

Signal : FID2B.ch

peak #	R.T. min	Start min	End min	PK TY	peak height	peak area	peak % max.	% of total
1	6.335	6.304	6.437	BB	354629	3642371	100.00%	51.697%
2	16.766	16.706	16.827	BB	252235	3403211	93.43%	48.303%
Sum of corrected areas:							7045582	

FF030119.M Mon Mar 18 09:03:26 2019