

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF031619\  
Data File : FF003863.D  
Signal(s) : FID2B.ch  
Acq On : 15 Mar 2019 20:05  
Operator : AJ\SJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Mar 15 23:01:20 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Quant Title :  
QLast Update : Mon Mar 04 08:35:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.587 | 2091616  | 15.023 ug/ml |

Target Compounds  
-----

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF031619\  
Data File : FF003863.D  
Signal(s) : FID2B.ch  
Acq On : 15 Mar 2019 20:05  
Operator : AJ\SJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Mar 15 23:01:20 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Quant Title :  
QLast Update : Mon Mar 04 08:35:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

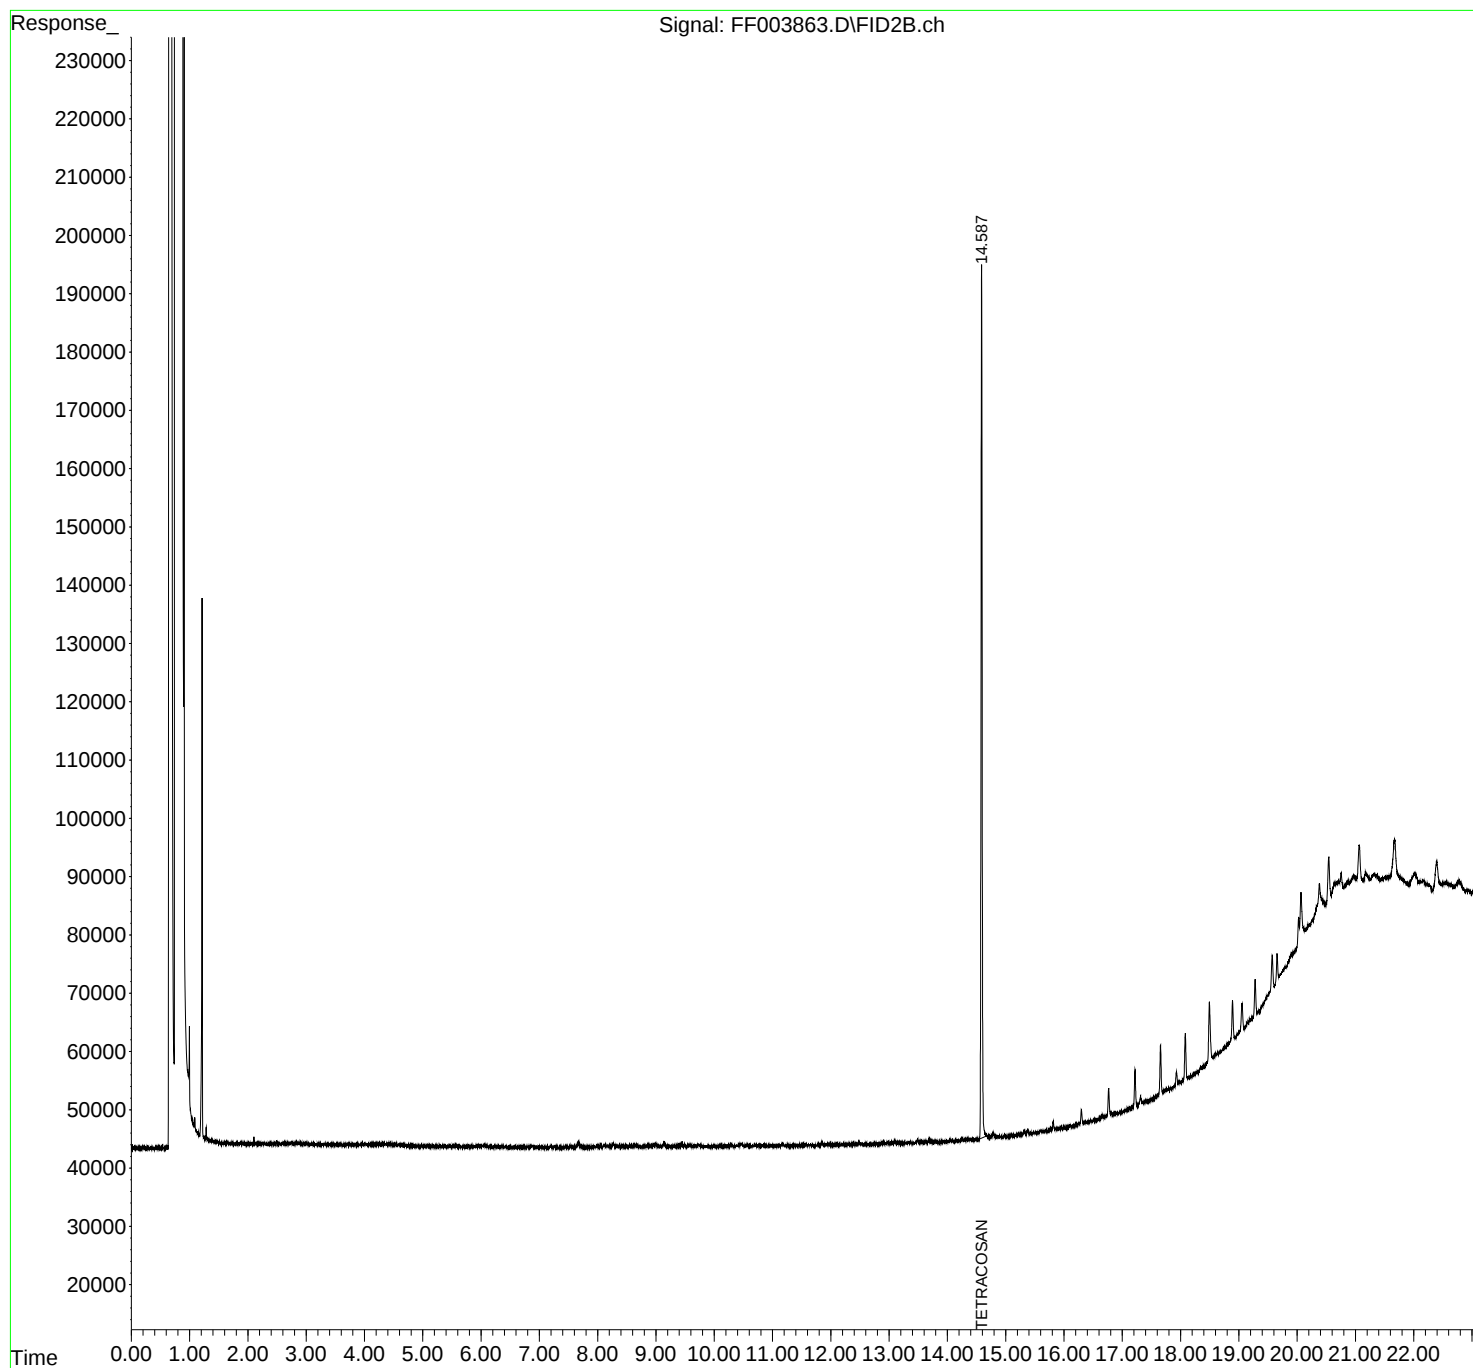

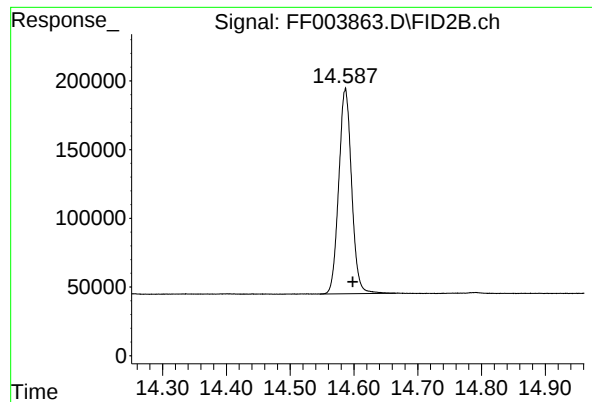

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.587 min  
Delta R.T.: -0.012 min  
Response: 2091616  
Conc: 15.02 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

rteres

# Area Percent Report

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF031619\  
Data File : FF003863.D  
Signal(s) : FID2B.ch  
Acq On : 15 Mar 2019 20:05  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e

Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Title :

Signal : FID2B.ch

| peak<br>#               | R.T.<br>min | Start<br>min | End<br>min | PK<br>TY | peak<br>height | peak<br>area | peak<br>% max. | % of<br>total |
|-------------------------|-------------|--------------|------------|----------|----------------|--------------|----------------|---------------|
| 1                       | 14.587      | 14.547       | 14.665     | BB       | 149753         | 2091616      | 100.00%        | 100.000%      |
| Sum of corrected areas: |             |              |            |          |                | 2091616      |                |               |

FF030119.M Mon Mar 18 09:22:13 2019