

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031622\
Data File : FF010028.D
Signal(s) : FID2B.ch
Acq On : 16 Mar 2022 15:37
Operator : AJ\MA
Sample : PB143390BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 17 00:34:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.694	3126533	20.848 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031622\
Data File : FF010028.D
Signal(s) : FID2B.ch
Acq On : 16 Mar 2022 15:37
Operator : AJ\MA
Sample : PB143390BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 17 00:34:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

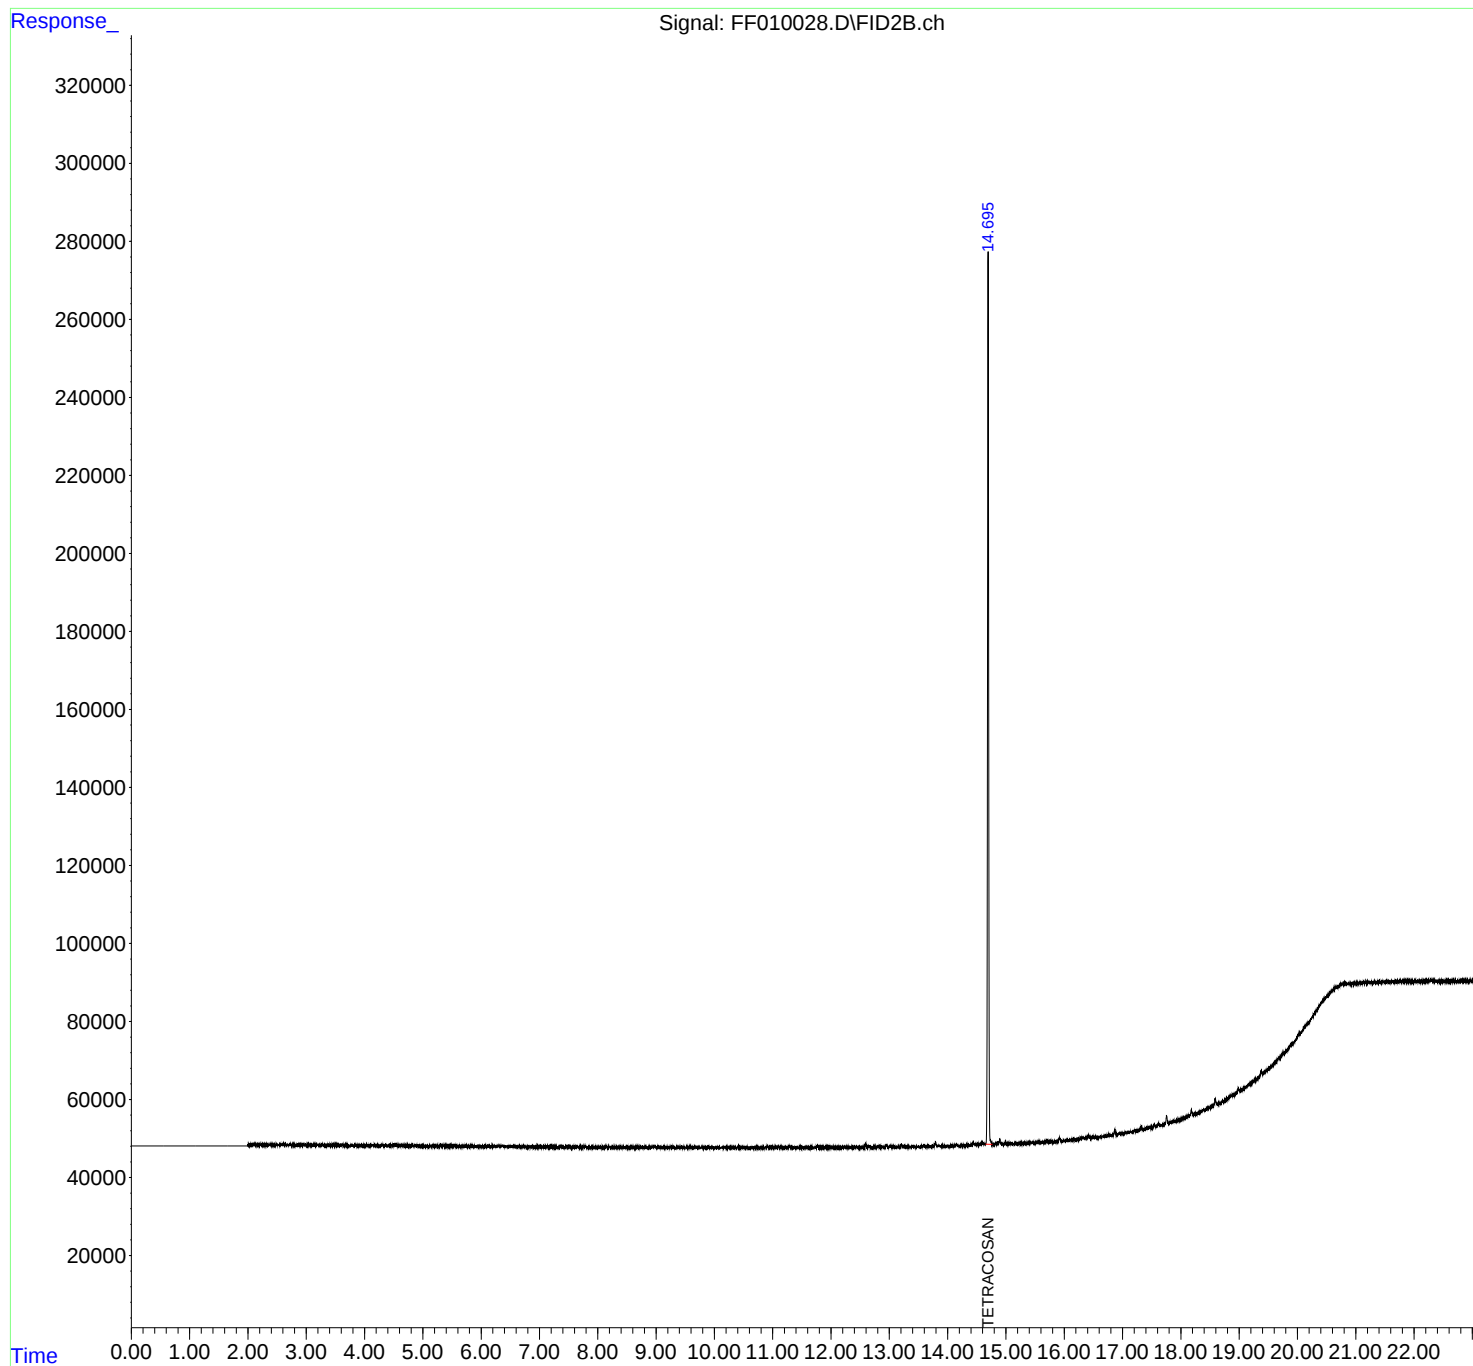

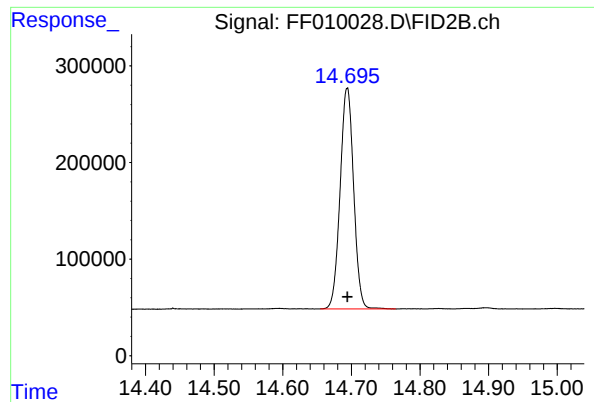

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.694 min
Delta R.T.: 0.000 min
Response: 3126533
Conc: 20.85 ug/ml

Instrument :
FID_F
ClientSampleId :