

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031622\
 Data File : FF010035.D
 Signal(s) : FID2B.ch
 Acq On : 16 Mar 2022 19:10
 Operator : AJ\MA
 Sample : N1951-04
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 17 00:35:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
 Quant Title :
 QLast Update : Thu Mar 10 12:46:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.699	2062551	13.753 ug/ml
Target Compounds			
4) N-TETRADECANE	8.184f	133538	0.769 ug/ml
7) N-EICOSANE	12.663f	91833	0.529 ug/ml
10) N-TETRACOSANE	14.900	51214	0.303 ug/ml
12) N-OCTACOSANE	16.867	309528	1.934 ug/ml
13) N-TRIACONTANE	17.739	56263	0.366 ug/ml
15) N-TETRATRIACONTANE	19.353	371382	2.712 ug/ml
16) N-HEXATRIACONTANE	20.153	1320252	10.618 ug/ml
17) N-OCTATRIACONTANE	20.796f	1395178	12.529 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031622\
Data File : FF010035.D
Signal(s) : FID2B.ch
Acq On : 16 Mar 2022 19:10
Operator : AJ\MA
Sample : N1951-04
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 17 00:35:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

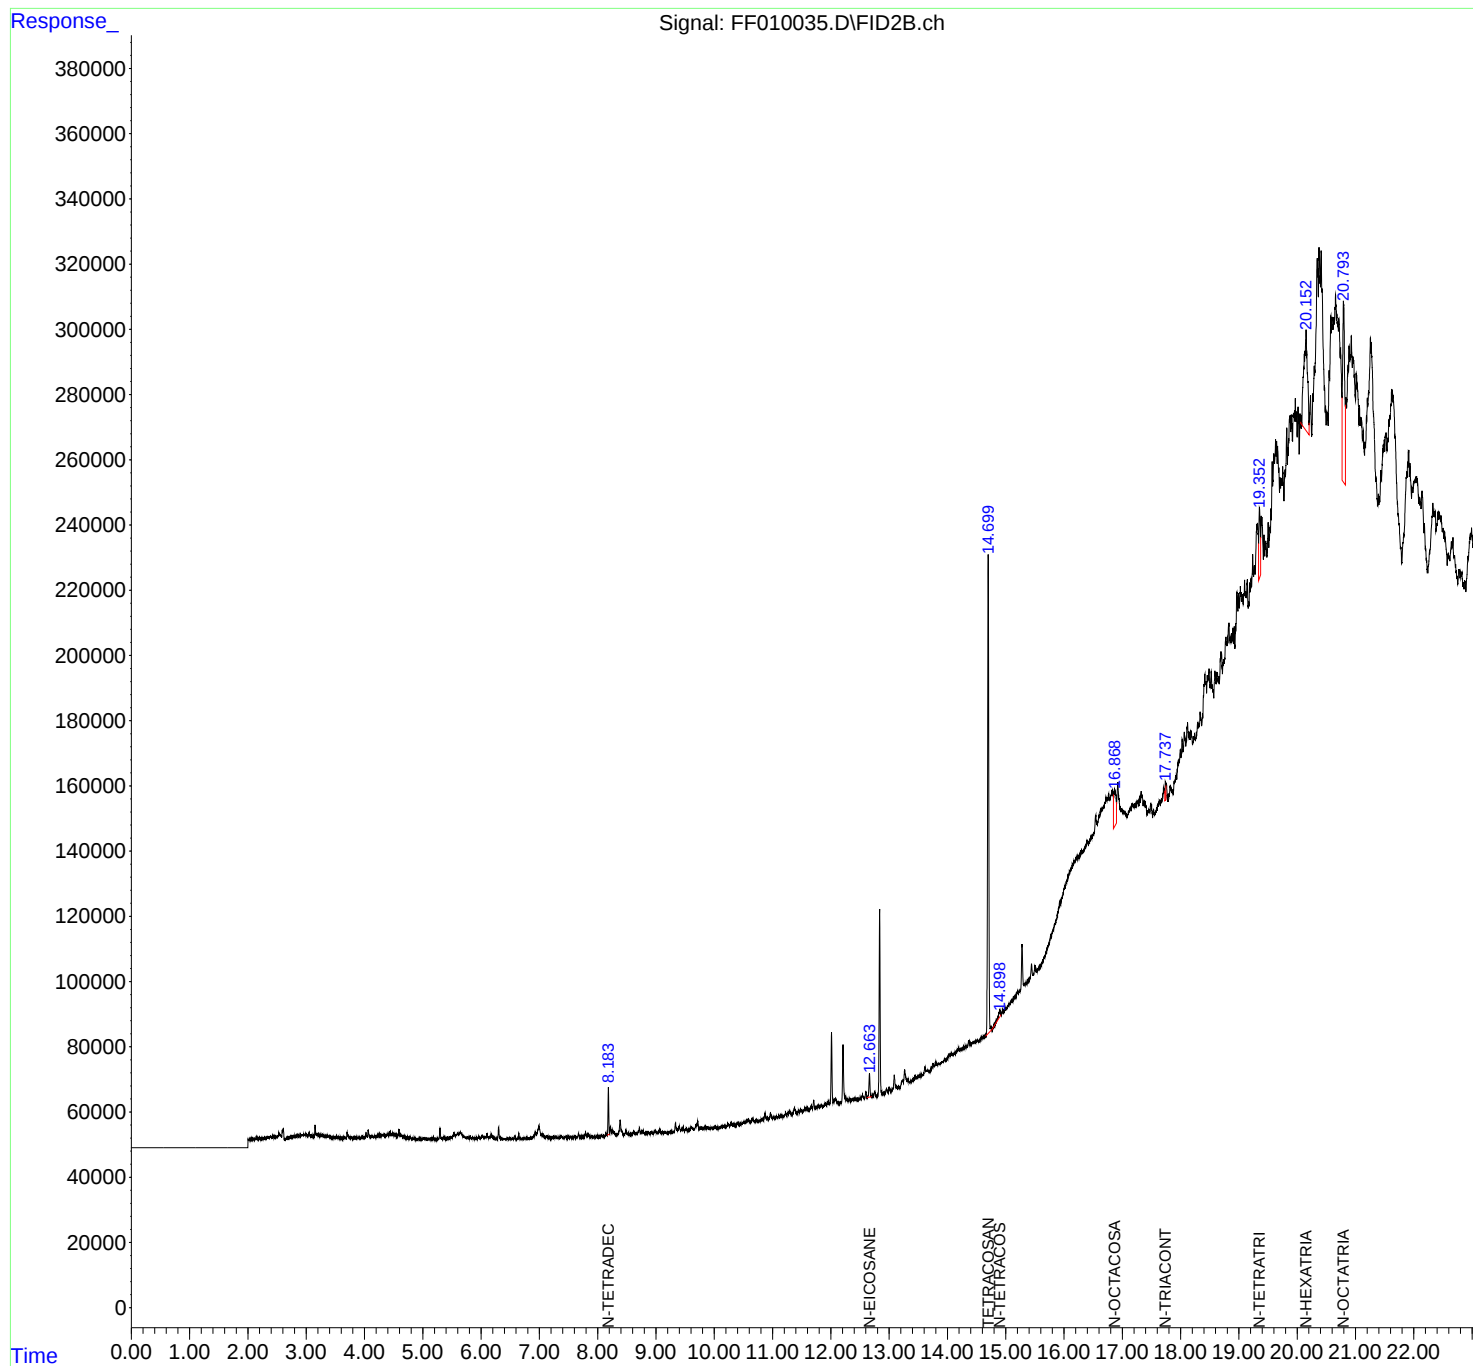


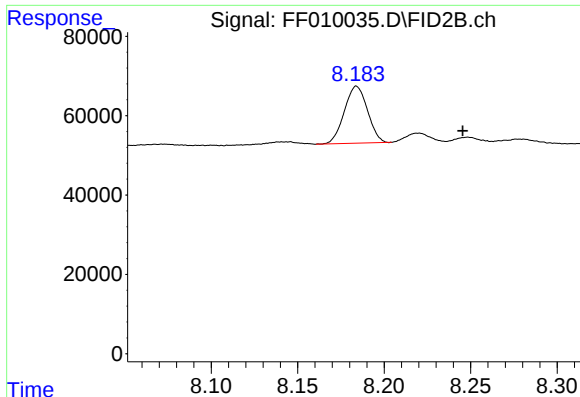

#4 N-TETRADECANE


R.T.: 8.184 min
Delta R.T.: -0.061 min
Response: 133538
Conc: 0.77 ug/ml

Instrument :
FID_F
ClientSampleId :

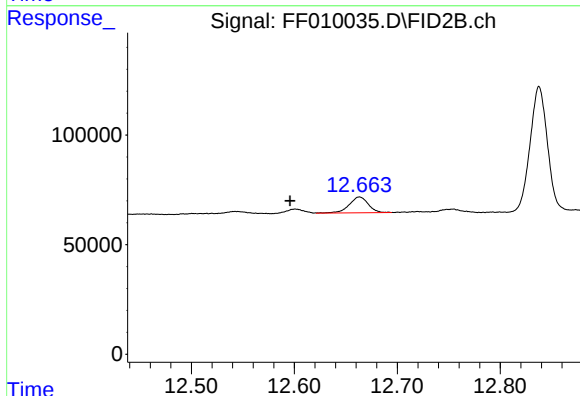


#7 N-EICOSANE

R.T.: 12.663 min
Delta R.T.: 0.067 min
Response: 91833
Conc: 0.53 ug/ml

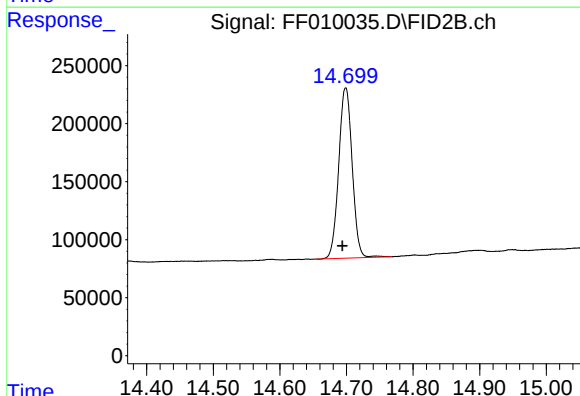


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.699 min
Delta R.T.: 0.005 min
Response: 2062551
Conc: 13.75 ug/ml

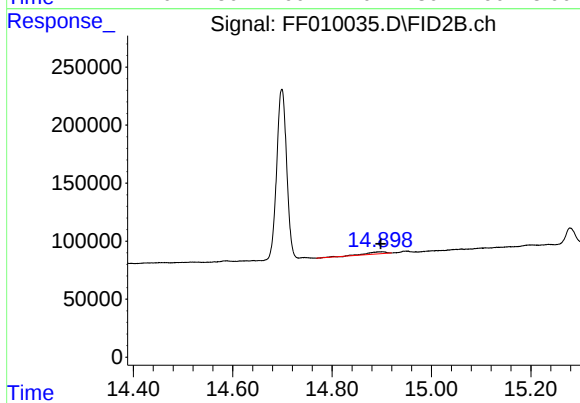

#10 N-TETRACOSANE


R.T.: 14.900 min
Delta R.T.: 0.002 min
Response: 51214
Conc: 0.30 ug/ml

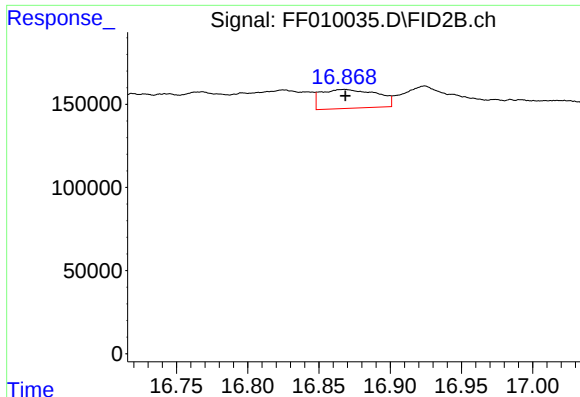

#12 N-OCTACOSANE


R.T.: 16.867 min
Delta R.T.: -0.001 min
Response: 309528
Conc: 1.93 ug/ml

Instrument :
FID_F
ClientSampleId :

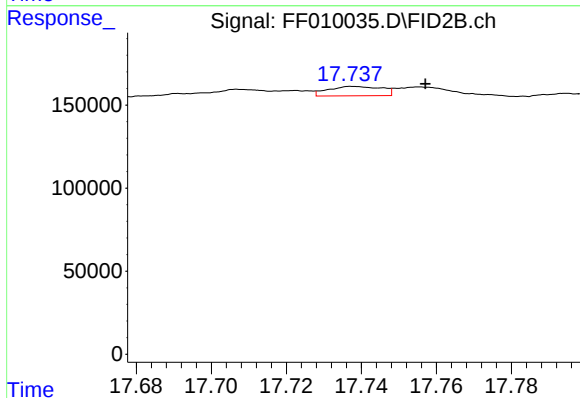


#13 N-TRIACONTANE

R.T.: 17.739 min
Delta R.T.: -0.018 min
Response: 56263
Conc: 0.37 ug/ml

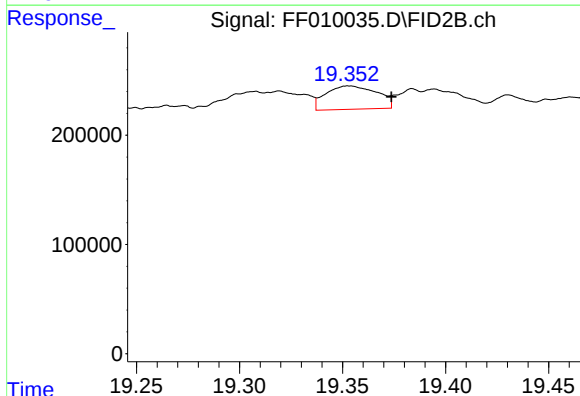


#15 N-TETRATRIACONTANE

R.T.: 19.353 min
Delta R.T.: -0.020 min
Response: 371382
Conc: 2.71 ug/ml

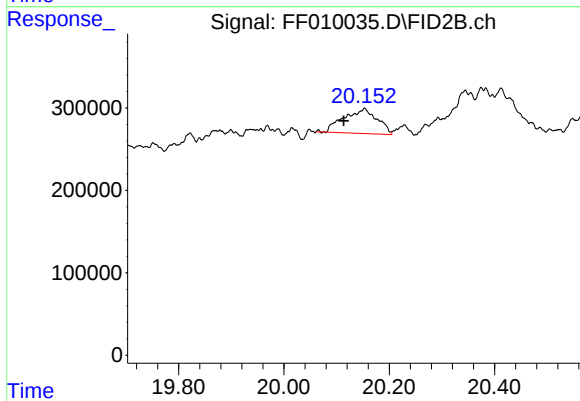

#16 N-HEXATRIACONTANE

R.T.: 20.153 min
Delta R.T.: 0.039 min
Response: 1320252
Conc: 10.62 ug/ml

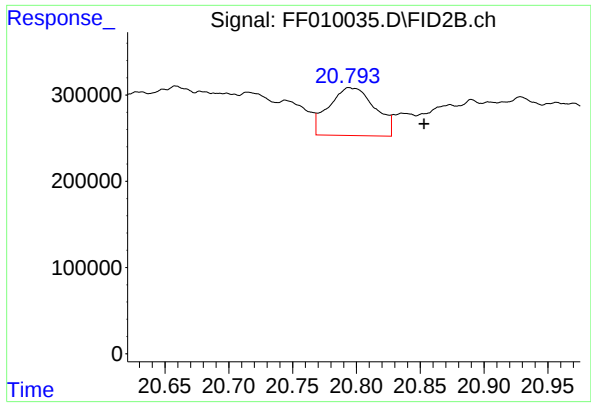

#17 N-OCTATRIACONTANE

R.T.: 20.796 min
Delta R.T.: -0.057 min
Response: 1395178
Conc: 12.53 ug/ml

Instrument :
FID_F
ClientSampleId :