

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031622\
Data File : FF010027.D
Signal(s) : FID2B.ch
Acq On : 16 Mar 2022 14:09
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 17 00:34:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.455	4180719	24.313 ug/ml
12)	N-OCTACOSANE	16.871	3812840	23.823 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031622\
Data File : FF010027.D
Signal(s) : FID2B.ch
Acq On : 16 Mar 2022 14:09
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 17 00:34:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

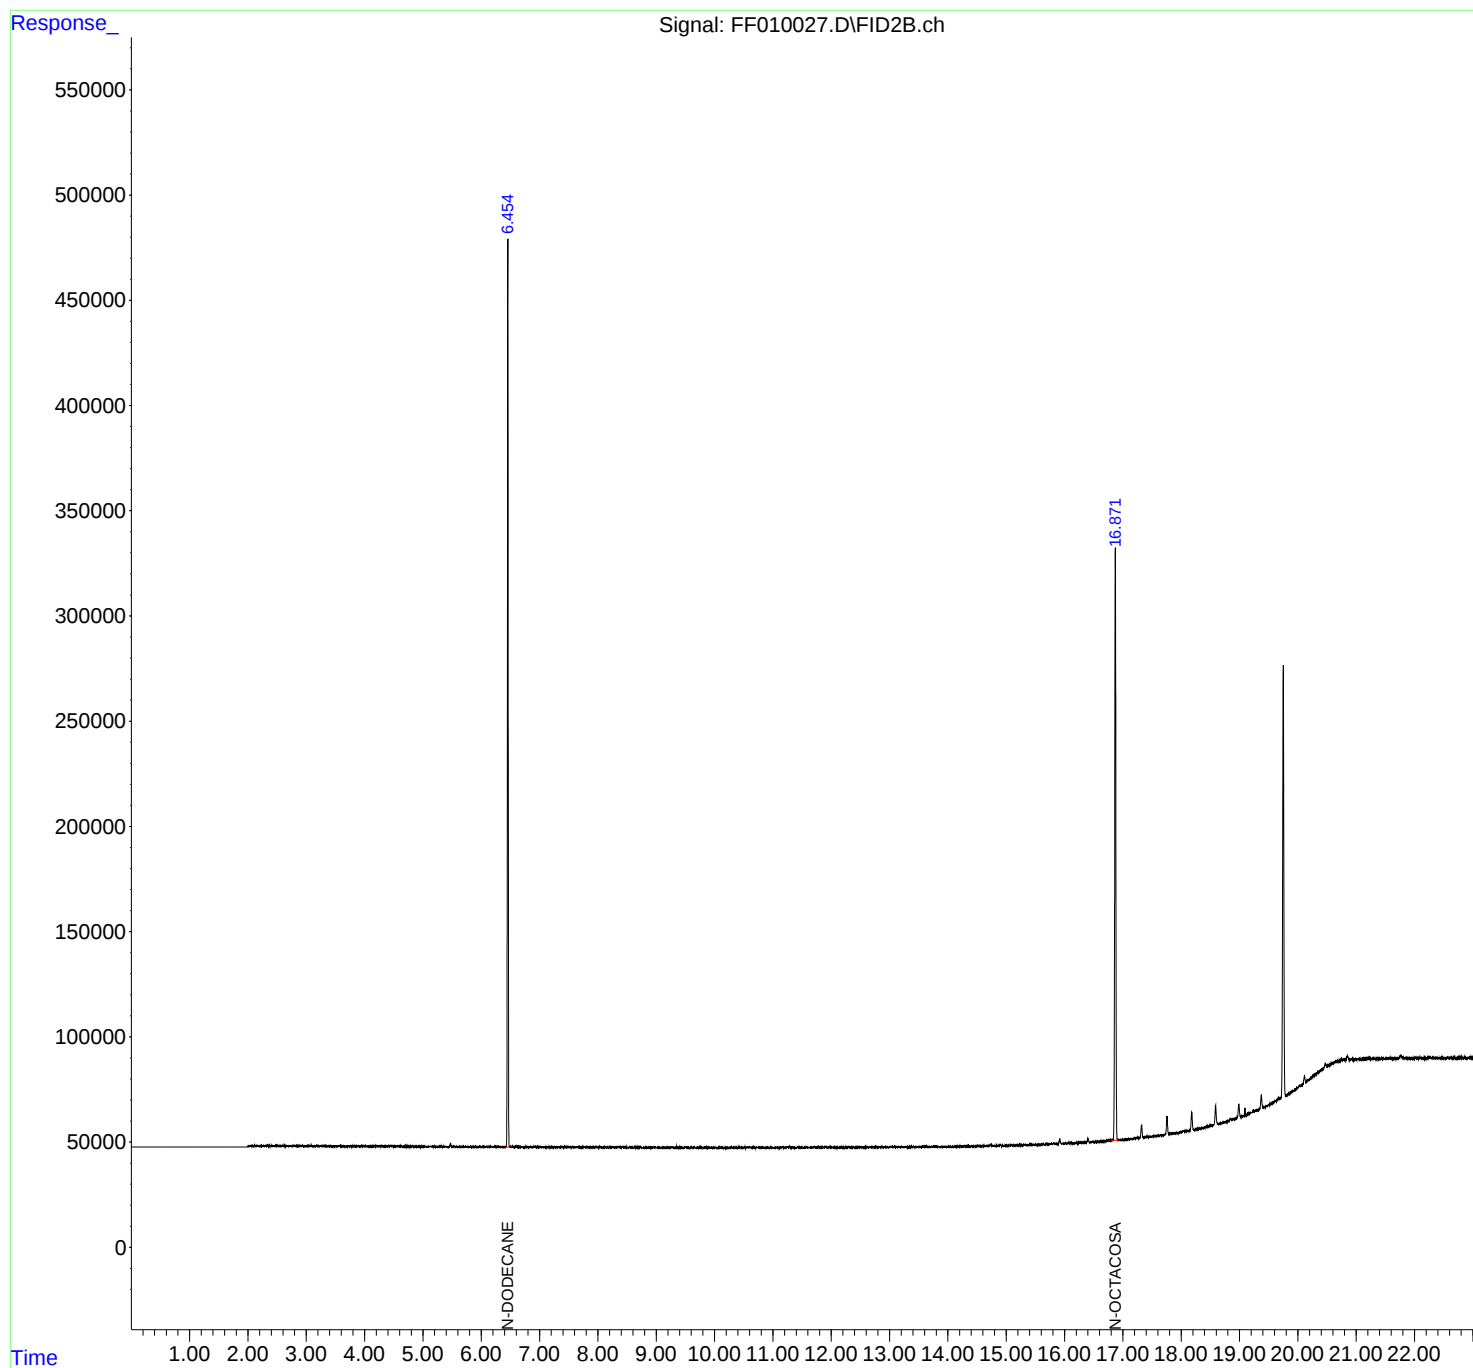


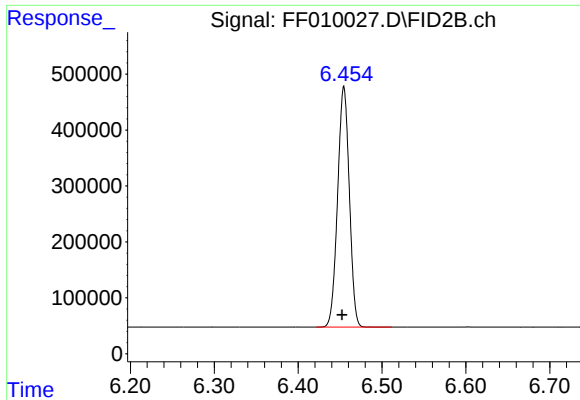

#3 N-DODECANE


R.T.: 6.455 min
Delta R.T.: 0.002 min
Response: 4180719
Conc: 24.31 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

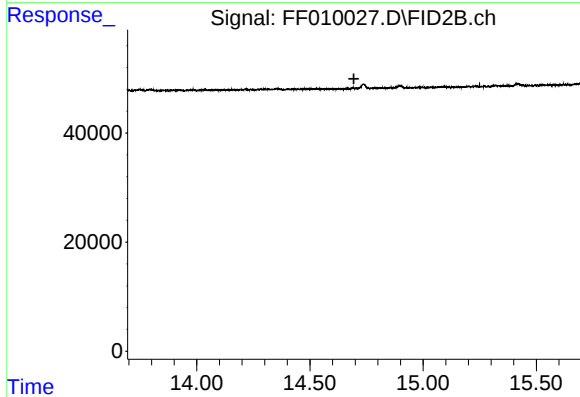

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.694 min
Response: 0
Conc: N.D.

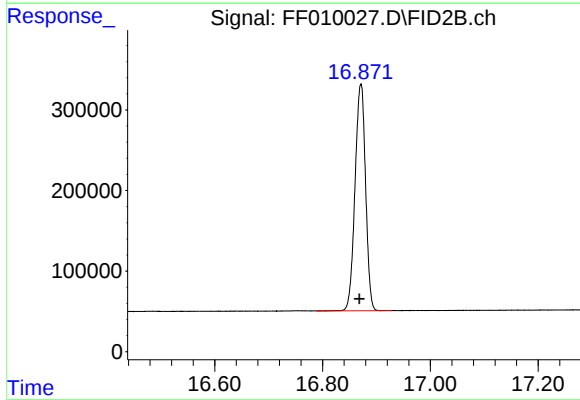

#12 N-OCTACOSANE

R.T.: 16.871 min
Delta R.T.: 0.002 min
Response: 3812840
Conc: 23.82 ug/ml