

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031622\
 Data File : FF010030.D
 Signal(s) : FID2B.ch
 Acq On : 16 Mar 2022 16:38
 Operator : AJ\MA
 Sample : N1951-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 DB-27-(22-25)-3-12-22

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/17/2022
 Supervised By :Ankita Jodhani 03/17/2022

Integration File: autoint1.e
 Quant Time: Mar 17 00:34:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
 Quant Title :
 QLast Update : Thu Mar 10 12:46:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.695	2851777	19.016 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031622\
Data File : FF010030.D
Signal(s) : FID2B.ch
Acq On : 16 Mar 2022 16:38
Operator : AJ\MA
Sample : N1951-01
Misc :
ALS Vial : 58 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
DB-27-(22-25)-3-12-22


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022

Integration File: autoint1.e
Quant Time: Mar 17 00:34:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

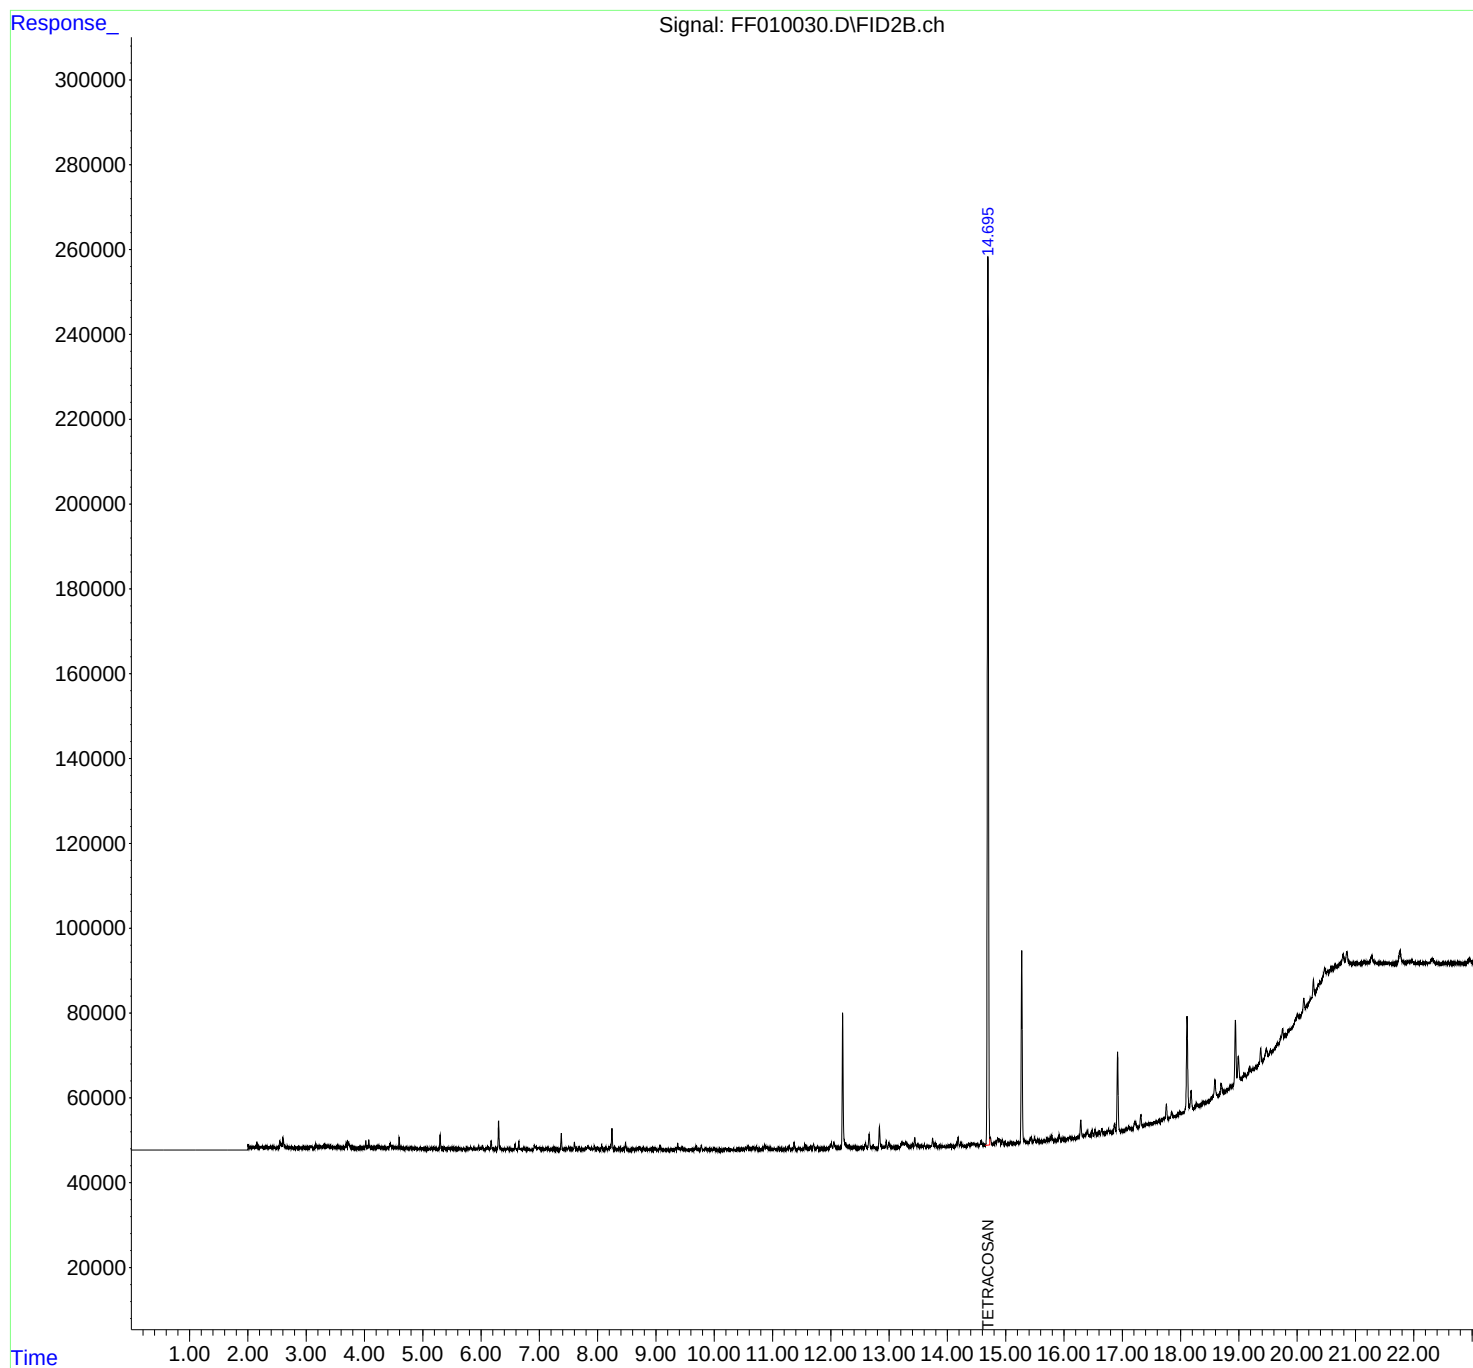

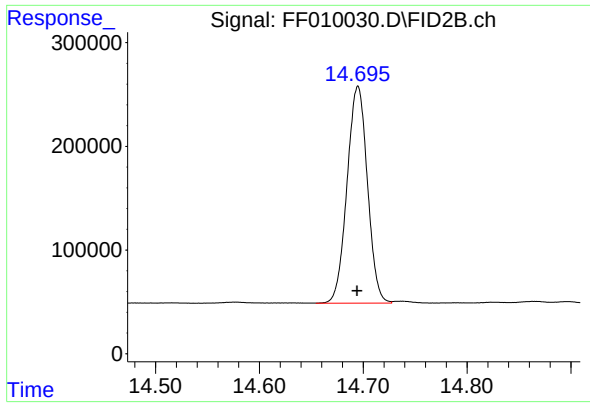

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.695 min
Delta R.T.: 0.000 min
Response: 2851777
Conc: 19.02 ug/ml

Instrument :
FID_F
ClientSampleId :
DB-27-(22-25)-3-12-22

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/17/2022
Supervised By :Ankita Jodhani 03/17/2022