

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031722\
 Data File : FF010049.D
 Signal(s) : FID2B.ch
 Acq On : 17 Mar 2022 11:19
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 17 22:13:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
 Quant Title :
 QLast Update : Thu Mar 10 12:46:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.454	4599701	26.750 ug/ml
12) N-OCTACOSANE	16.871	4048100	25.293 ug/ml
13) N-TRIACONTANE	17.757	237440	1.546 ug/ml
14) N-DOTRIACONTANE	18.590	277173	1.898 ug/ml
15) N-TETRATRIACONTANE	19.374	208741	1.524 ug/ml
16) N-HEXATRIACONTANE	20.114	150888	1.213 ug/ml
17) N-OCTATRIACONTANE	20.851	94981	0.853 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031722\
Data File : FF010049.D
Signal(s) : FID2B.ch
Acq On : 17 Mar 2022 11:19
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 17 22:13:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

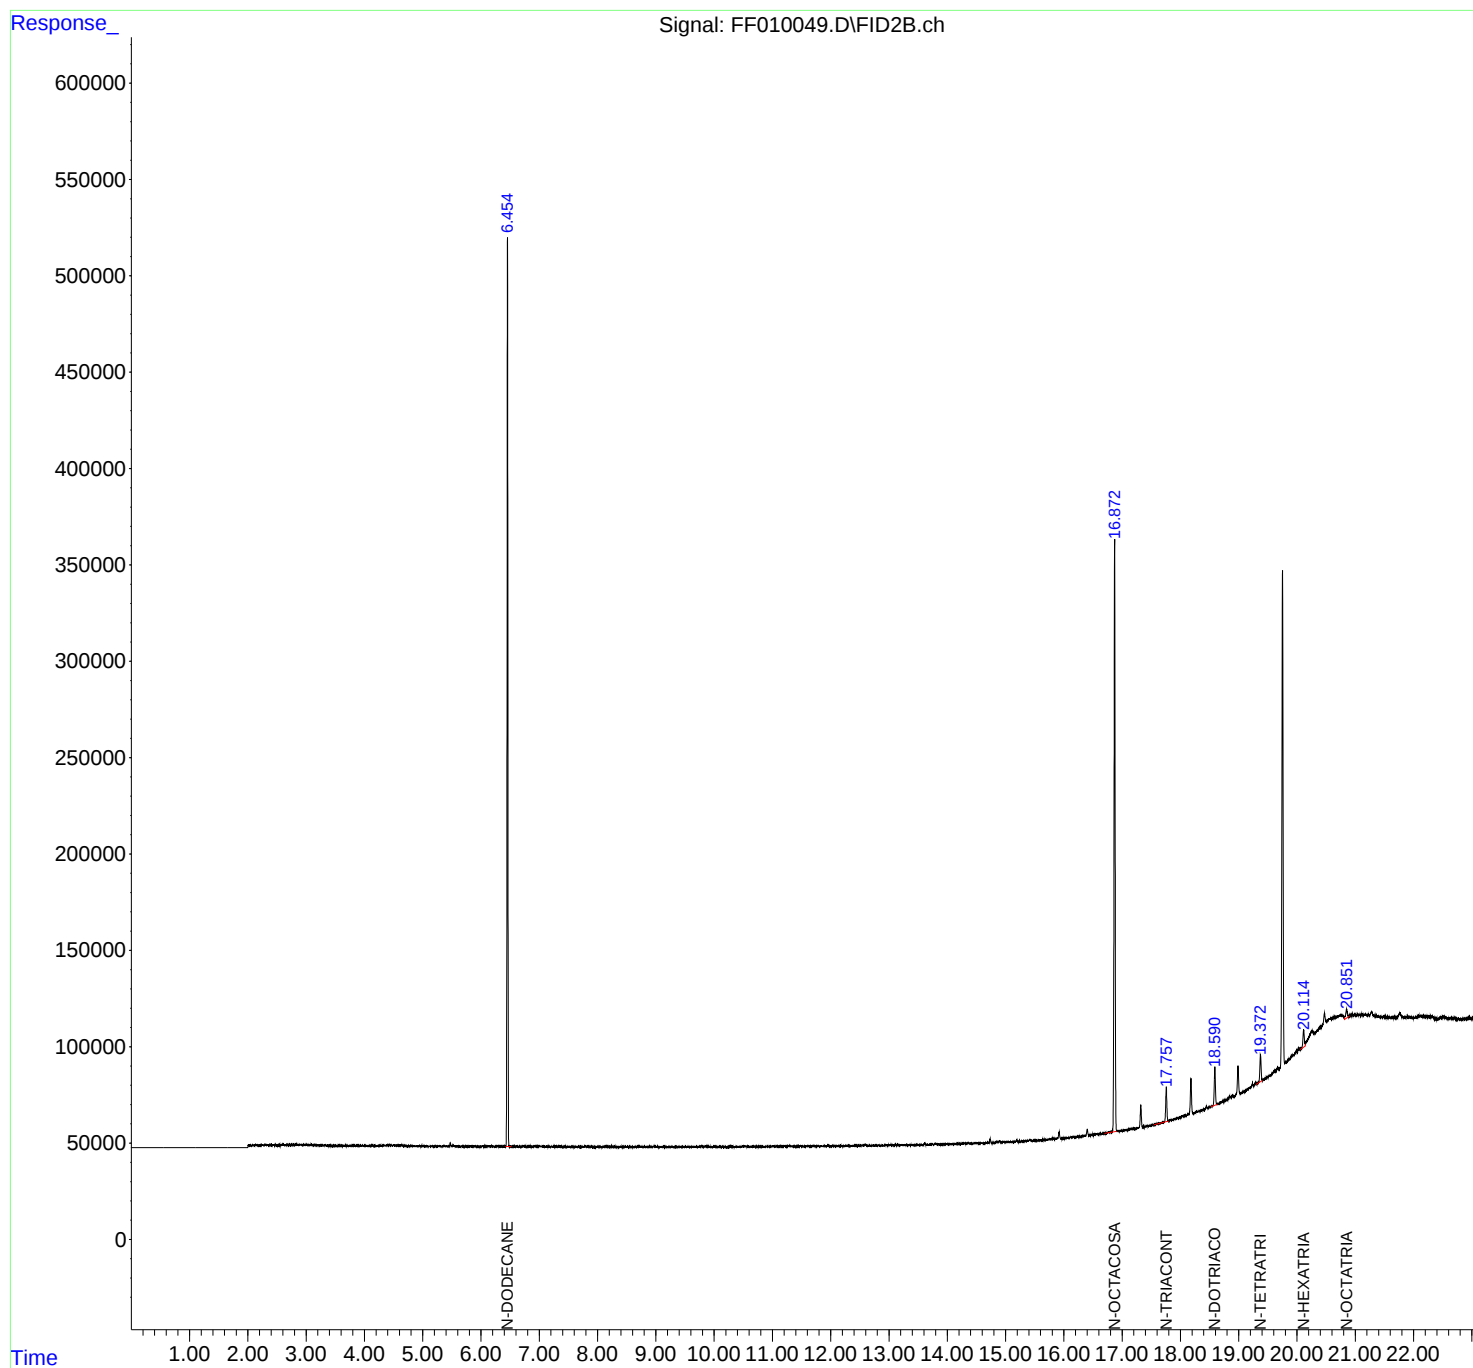


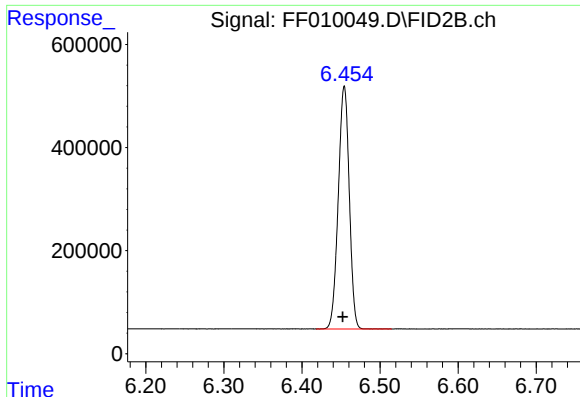

#3 N-DODECANE


R.T.: 6.454 min
Delta R.T.: 0.002 min
Response: 4599701
Conc: 26.75 ug/ml

Instrument :
FID_F
ClientSampleId :

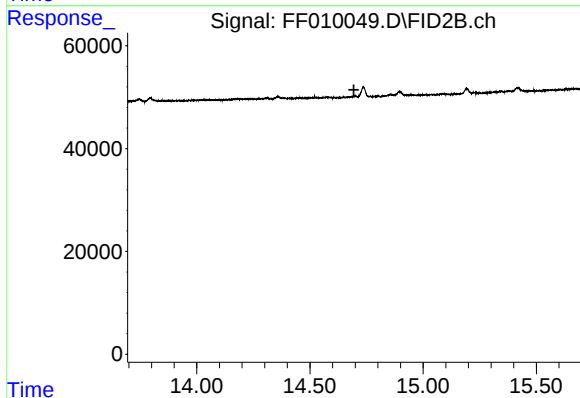


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.694 min
Response: 0
Conc: N.D.

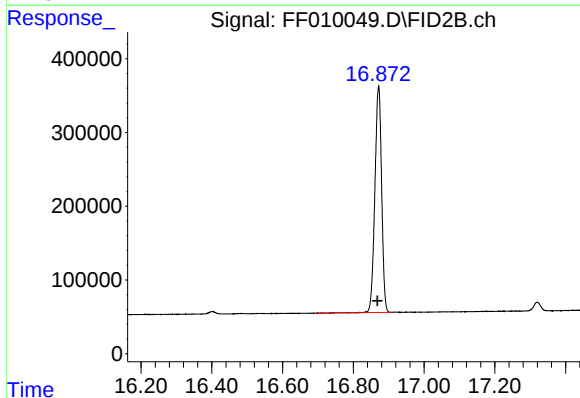


#12 N-OCTACOSANE

R.T.: 16.871 min
Delta R.T.: 0.003 min
Response: 4048100
Conc: 25.29 ug/ml

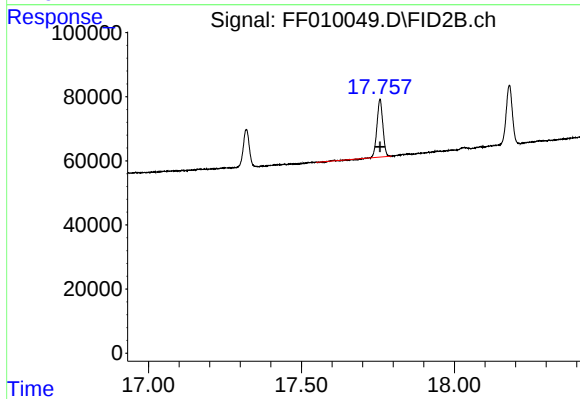

#13 N-TRIACONTANE


R.T.: 17.757 min
Delta R.T.: 0.000 min
Response: 237440
Conc: 1.55 ug/ml

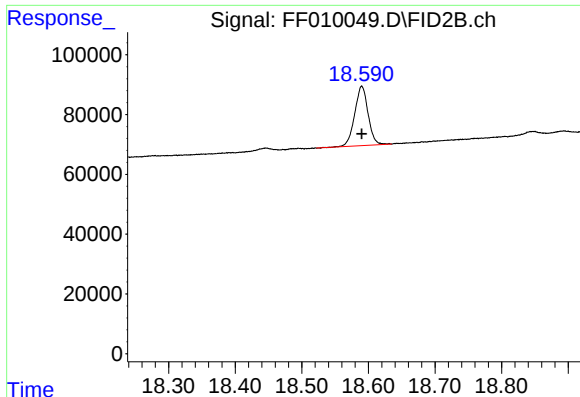

#14 N-DOTRIACONTANE


R.T.: 18.590 min
Delta R.T.: 0.000 min
Response: 277173
Conc: 1.90 ug/ml

Instrument :
FID_F
ClientSampleId :

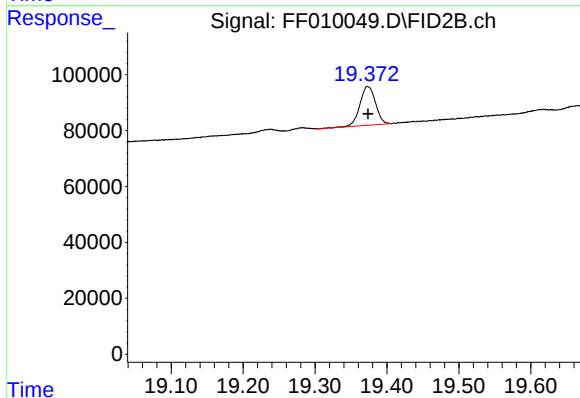


#15 N-TETRATRIACONTANE

R.T.: 19.374 min
Delta R.T.: 0.000 min
Response: 208741
Conc: 1.52 ug/ml

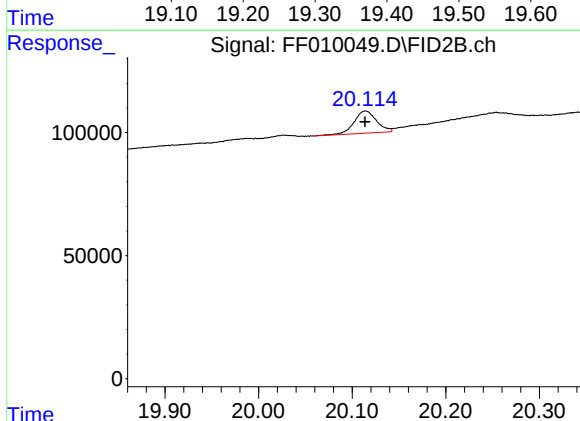

#16 N-HEXATRIACONTANE

R.T.: 20.114 min
Delta R.T.: 0.000 min
Response: 150888
Conc: 1.21 ug/ml

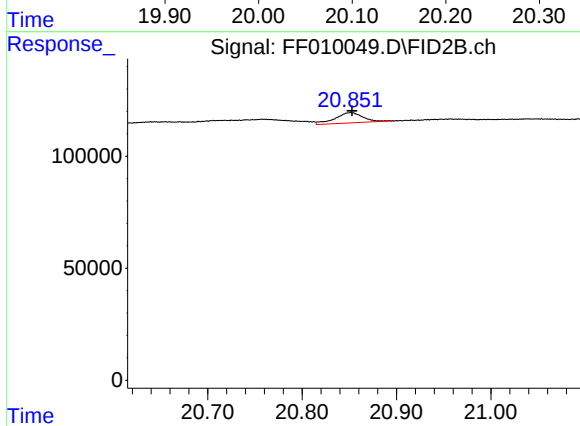

#17 N-OCTATRIACONTANE

R.T.: 20.851 min
Delta R.T.: -0.002 min
Response: 94981
Conc: 0.85 ug/ml