

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031722\
Data File : FF010051.D
Signal(s) : FID2B.ch
Acq On : 17 Mar 2022 12:21
Operator : AJ\MA
Sample : N1951-05 50X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 17 22:13:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
15) N-TETRATRIACONTANE	19.410	89360	0.652 ug/ml
17) N-OCTATRIACONTANE	20.791f	1341584	12.048 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031722\
Data File : FF010051.D
Signal(s) : FID2B.ch
Acq On : 17 Mar 2022 12:21
Operator : AJ\MA
Sample : N1951-05 50X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 17 22:13:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

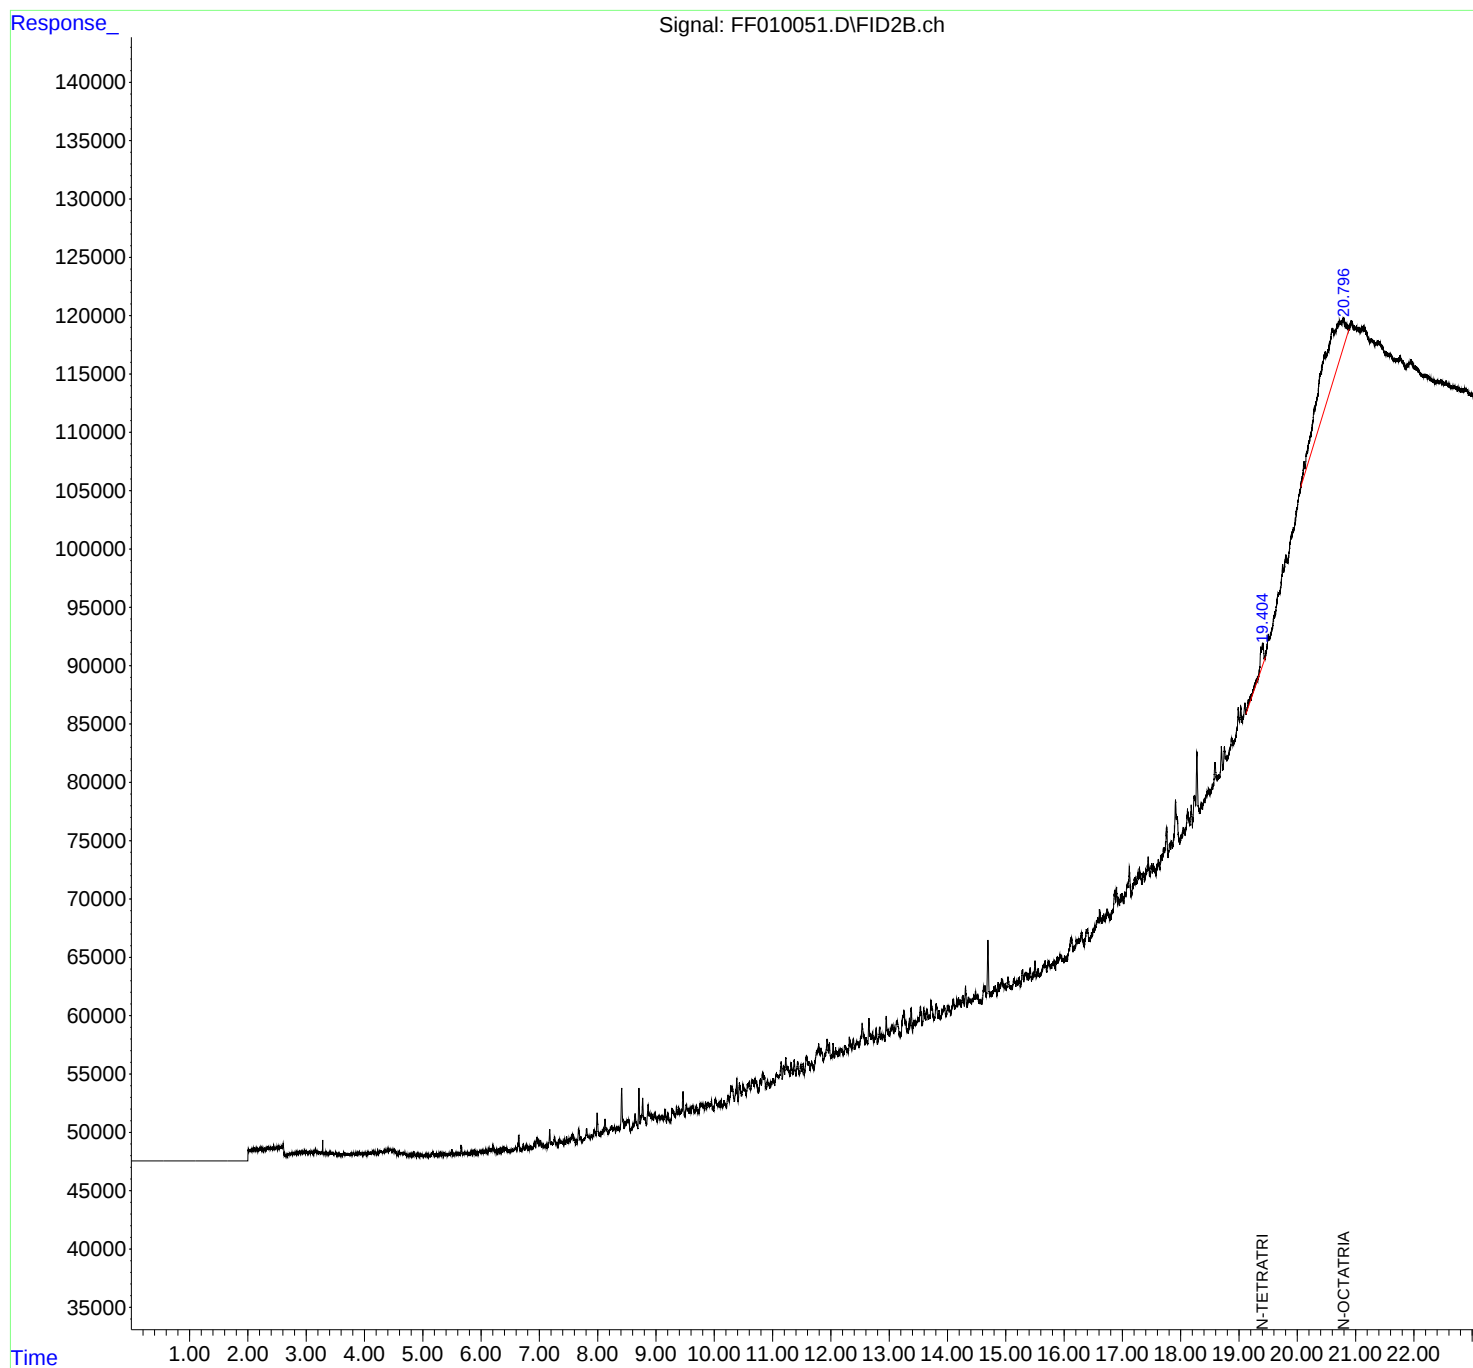


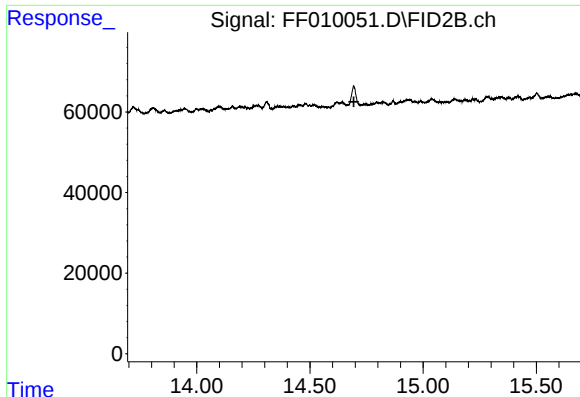

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.694 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

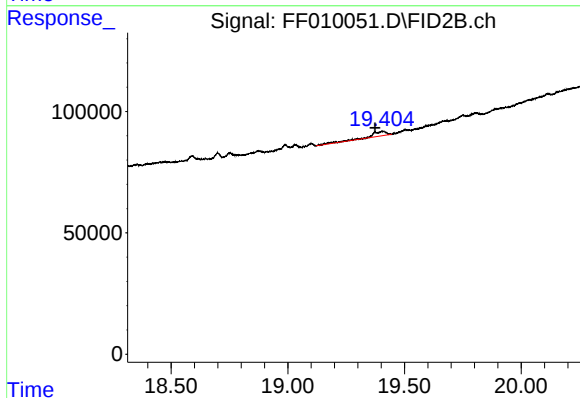

#15 N-TETRATRIACONTANE

R.T.: 19.410 min
Delta R.T.: 0.036 min
Response: 89360
Conc: 0.65 ug/ml

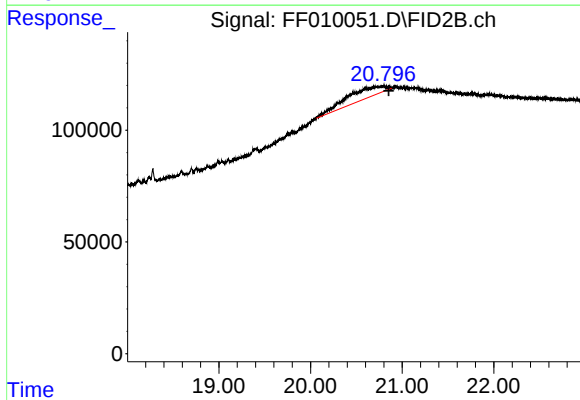

#17 N-OCTATRIACONTANE

R.T.: 20.791 min
Delta R.T.: -0.061 min
Response: 1341584
Conc: 12.05 ug/ml