

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031722\
 Data File : FF010058.D
 Signal(s) : FID2B.ch
 Acq On : 17 Mar 2022 17:56
 Operator : AJ\MA
 Sample : N1962-02
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 17 22:14:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
 Quant Title :
 QLast Update : Thu Mar 10 12:46:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.694	2480161	16.538 ug/ml
Target Compounds			
4) N-TETRADECANE	8.243	97737	0.563 ug/ml
5) N-HEXADECANE	9.854	284864	1.635 ug/ml
7) N-EICOSANE	12.600	241449	1.391 ug/ml
8) N-DOCOSANE	13.817	602308	3.523 ug/ml
10) N-TETRACOSANE	14.870	1675770	9.922 ug/ml
12) N-OCTACOSANE	16.866	394785	2.467 ug/ml
13) N-TRIACONTANE	17.754	233892	1.523 ug/ml
15) N-TETRATRIACONTANE	19.436f	202891	1.481 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031722\
Data File : FF010058.D
Signal(s) : FID2B.ch
Acq On : 17 Mar 2022 17:56
Operator : AJ\MA
Sample : N1962-02
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 17 22:14:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

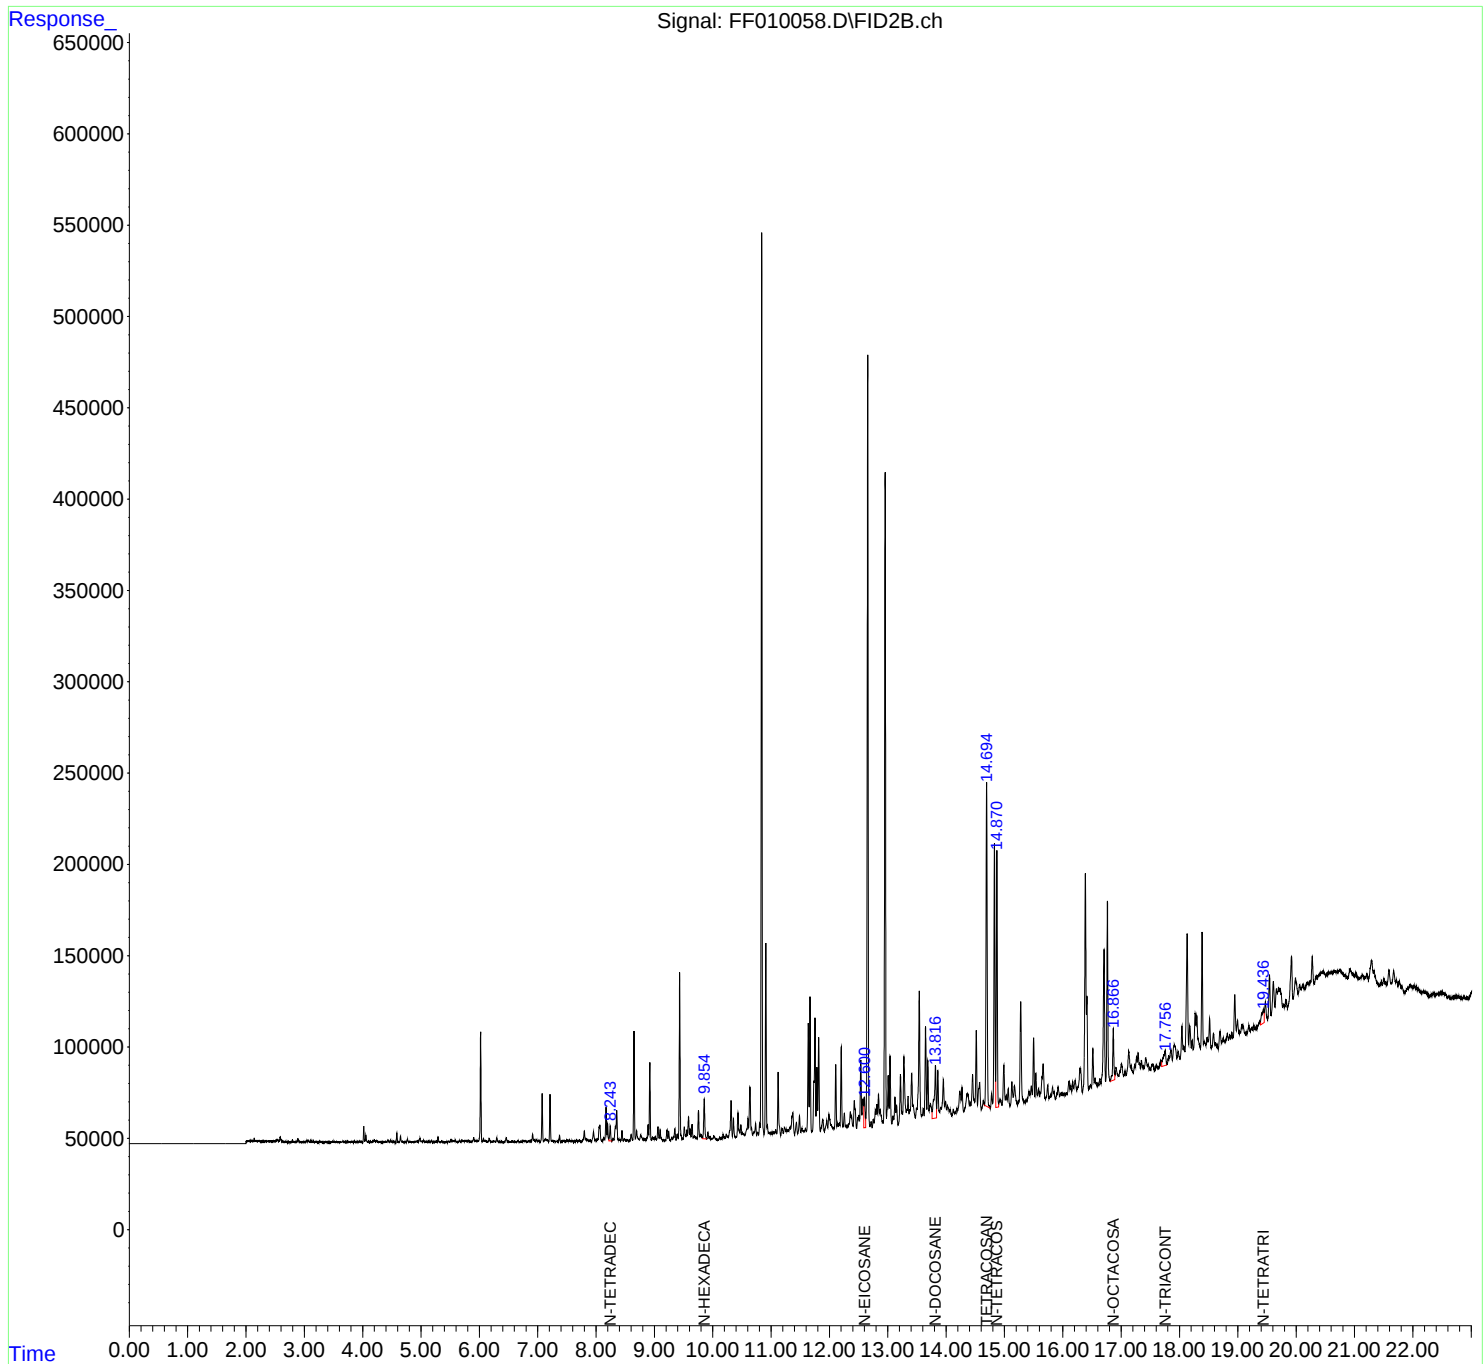


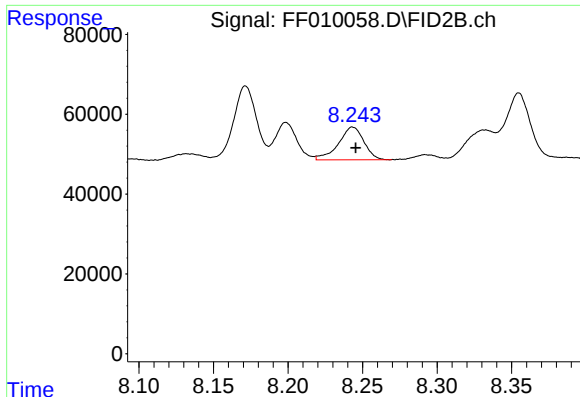

#4 N-TETRADECANE


R.T.: 8.243 min
Delta R.T.: -0.002 min
Response: 97737
Conc: 0.56 ug/ml

Instrument :
FID_F
ClientSampleId :

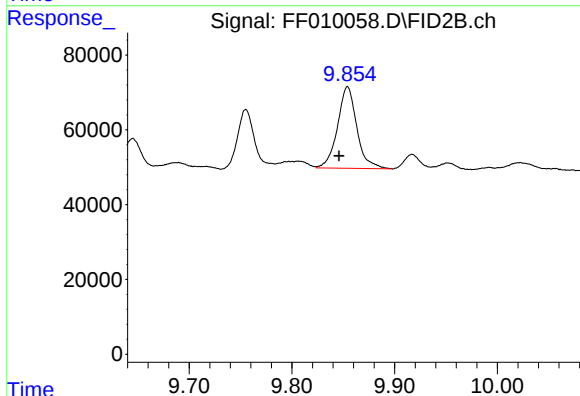


#5 N-HEXADECANE

R.T.: 9.854 min
Delta R.T.: 0.008 min
Response: 284864
Conc: 1.64 ug/ml

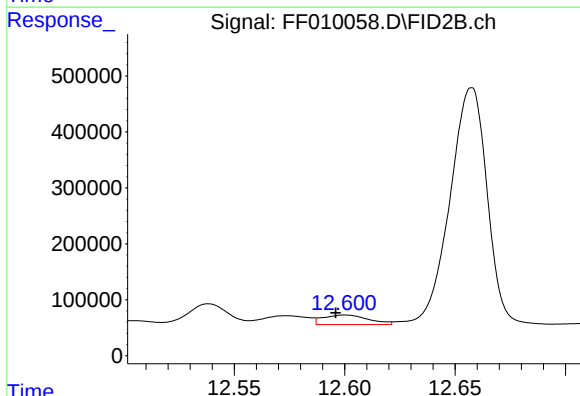


#7 N-EICOSANE

R.T.: 12.600 min
Delta R.T.: 0.004 min
Response: 241449
Conc: 1.39 ug/ml

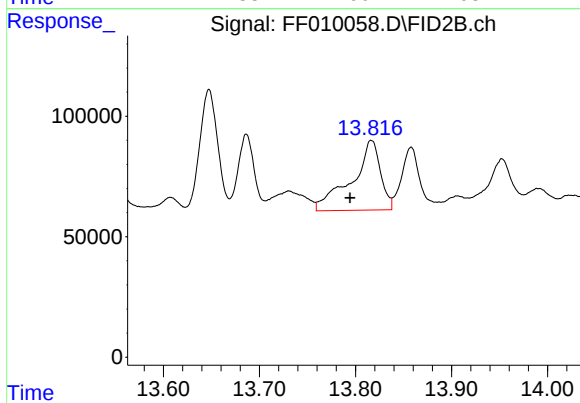

#8 N-DOCOSANE


R.T.: 13.817 min
Delta R.T.: 0.022 min
Response: 602308
Conc: 3.52 ug/ml

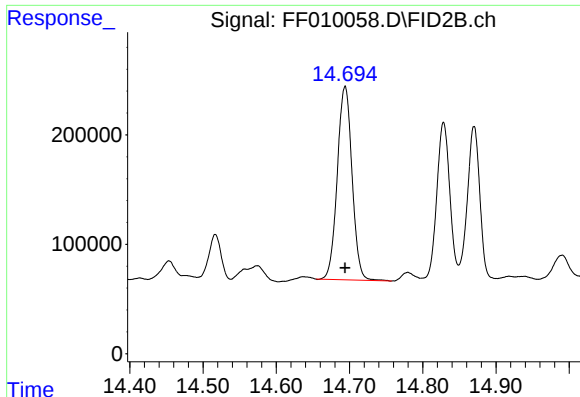

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.694 min
Delta R.T.: 0.000 min
Response: 2480161
Conc: 16.54 ug/ml

Instrument :
FID_F
ClientSampleId :

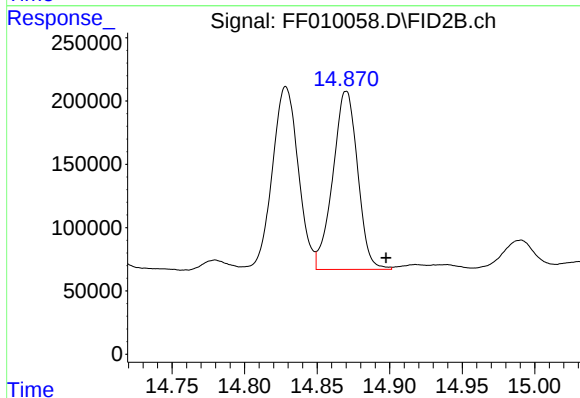


#10 N-TETRACOSANE

R.T.: 14.870 min
Delta R.T.: -0.028 min
Response: 1675770
Conc: 9.92 ug/ml

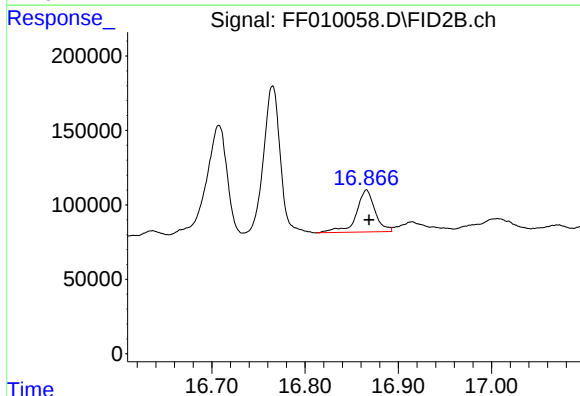


#12 N-OCTACOSANE

R.T.: 16.866 min
Delta R.T.: -0.003 min
Response: 394785
Conc: 2.47 ug/ml

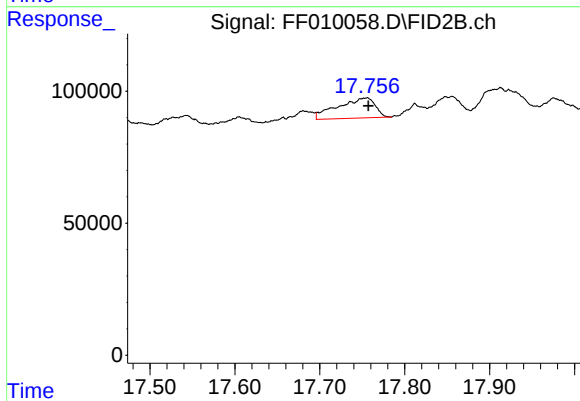

#13 N-TRIACONTANE

R.T.: 17.754 min
Delta R.T.: -0.003 min
Response: 233892
Conc: 1.52 ug/ml

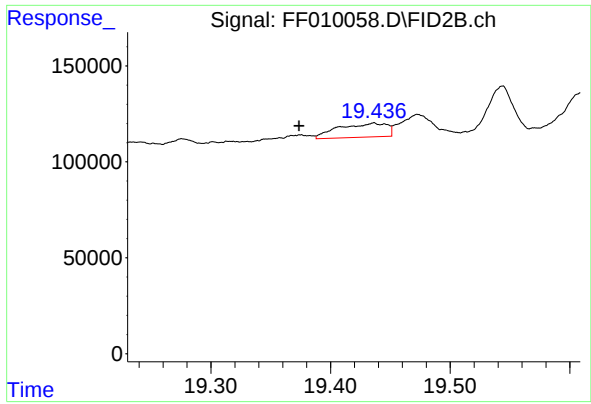

#15 N-TETRATRIACONTANE

R.T.: 19.436 min
Delta R.T.: 0.062 min
Response: 202891
Conc: 1.48 ug/ml

Instrument :

FID_F

ClientSampleId :