

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031722\
Data File : FF010058.D
Signal(s) : FID2B.ch
Acq On : 17 Mar 2022 17:56
Operator : AJ\MA
Sample : N1962-02
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
C-17-16-17

Integration File: autoint1.e
Quant Time: Mar 17 22:14:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.694	2480161	16.538 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031722\
Data File : FF010058.D
Signal(s) : FID2B.ch
Acq On : 17 Mar 2022 17:56
Operator : AJ\MA
Sample : N1962-02
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
C-17-16-17

Integration File: autoint1.e
Quant Time: Mar 17 22:14:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

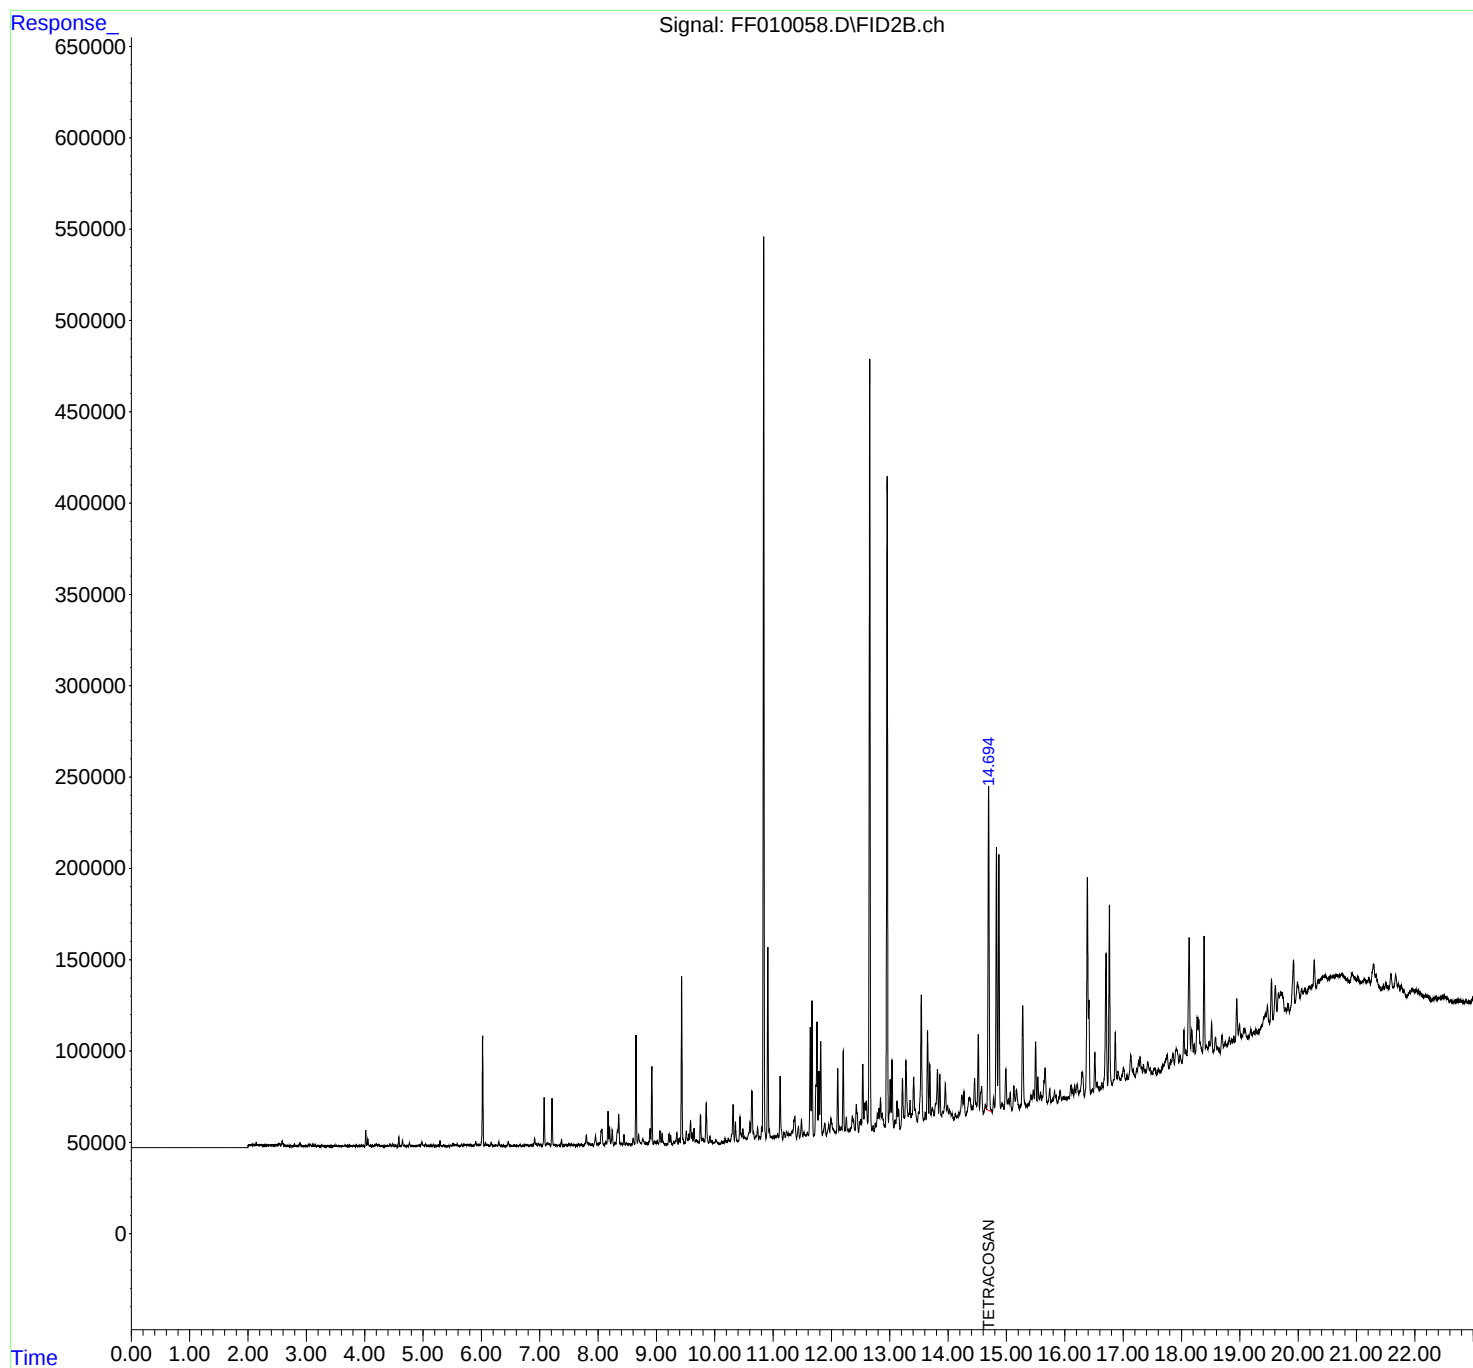

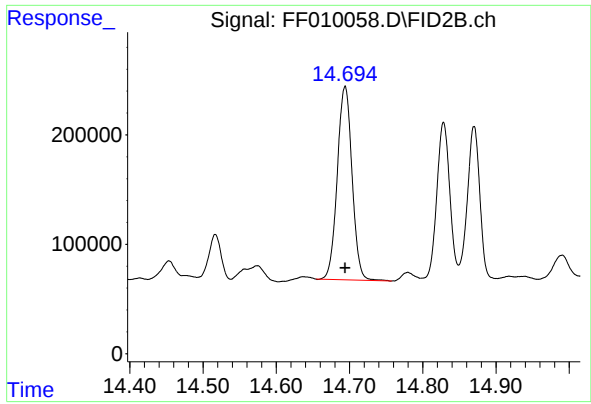

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.694 min
Delta R.T.: 0.000 min
Response: 2480161
Conc: 16.54 ug/ml

Instrument :
FID_F
ClientSampleId :
C-17-16-17