

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031722\
Data File : FF010065.D
Signal(s) : FID2B.ch
Acq On : 17 Mar 2022 21:26
Operator : AJ\MA
Sample : N1962-09
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
C-22-23-25

Integration File: autoint1.e
Quant Time: Mar 17 22:16:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.692	3232416	21.554 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031722\
Data File : FF010065.D
Signal(s) : FID2B.ch
Acq On : 17 Mar 2022 21:26
Operator : AJ\MA
Sample : N1962-09
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
C-22-23-25

Integration File: autoint1.e
Quant Time: Mar 17 22:16:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

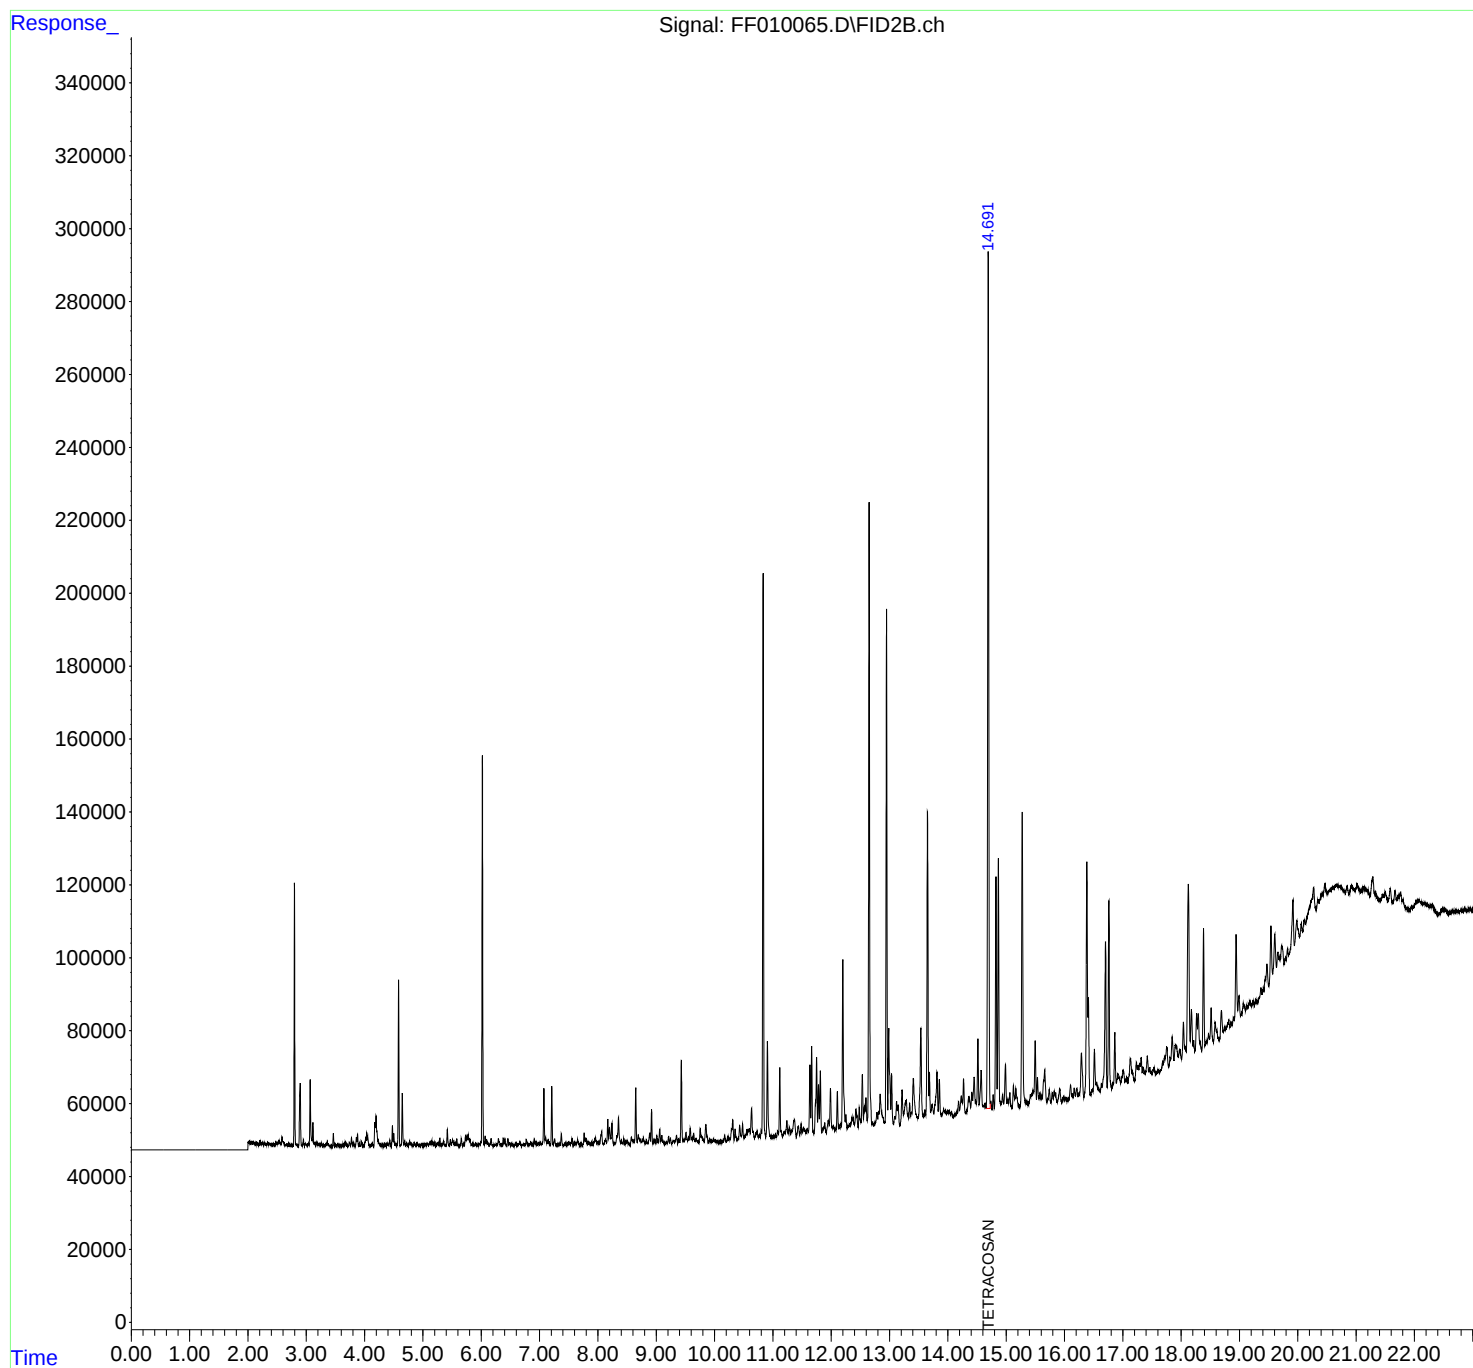

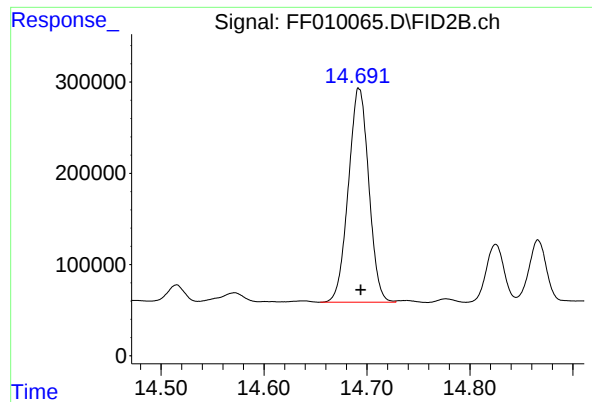

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.692 min
Delta R.T.: -0.002 min
Response: 3232416
Conc: 21.55 ug/ml

Instrument :
FID_F
ClientSampleId :
C-22-23-25