

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031723\
 Data File : FF012290.D
 Signal(s) : FID2B.ch
 Acq On : 17 Mar 2023 09:53
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 18 00:11:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) N-TETRACOSANE	15.209	82289	0.660 ug/ml
14) N-DOTRIACONTANE	18.924	162737	1.568 ug/ml
16) N-HEXATRIACONTANE	20.473	255282	2.914 ug/ml
18) N-TETRACONTANE	22.118	148632	1.820 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031723\
Data File : FF012290.D
Signal(s) : FID2B.ch
Acq On : 17 Mar 2023 09:53
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 18 00:11:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

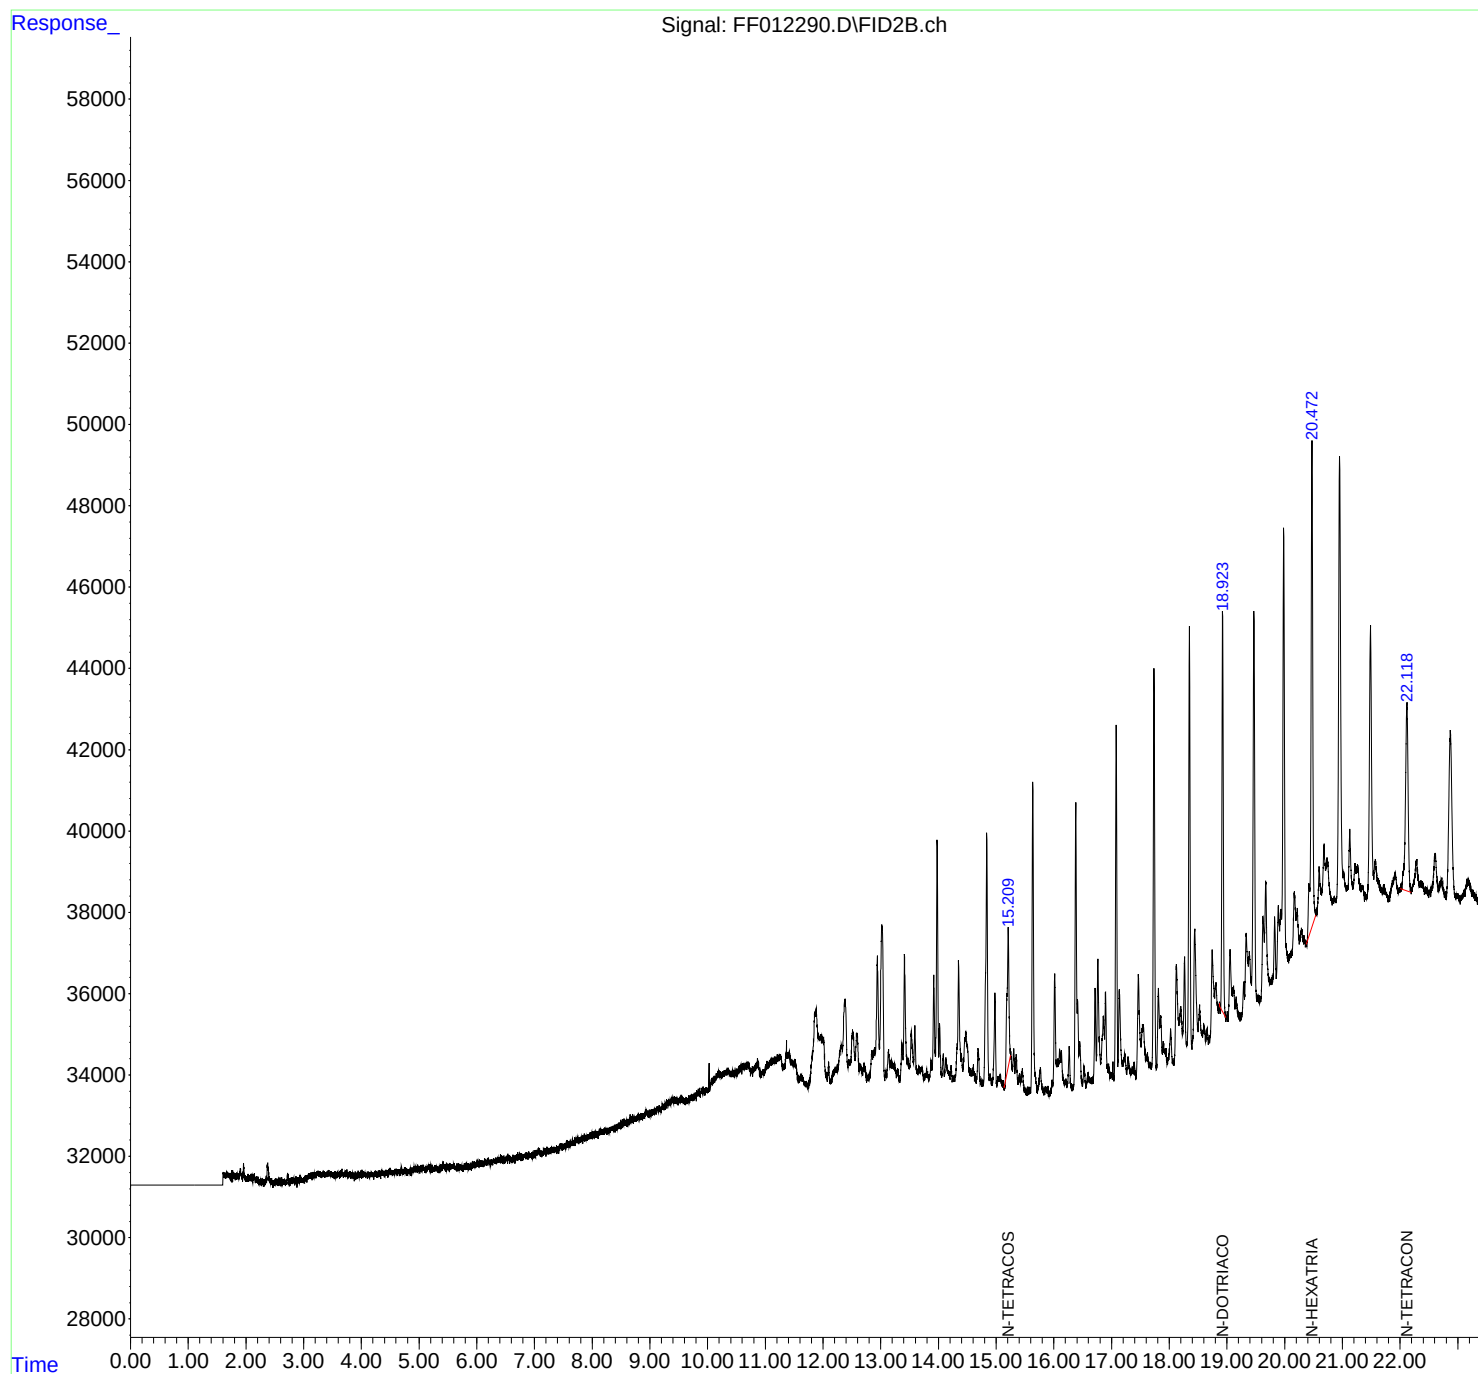


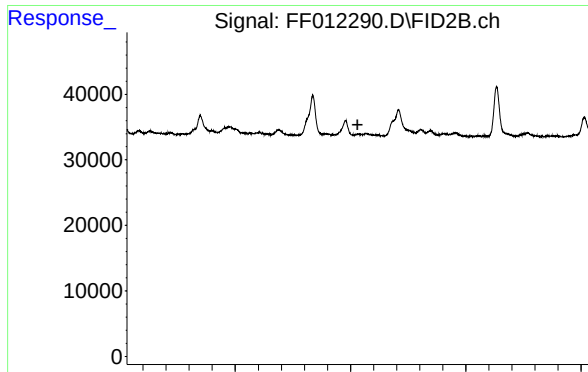

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.030 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

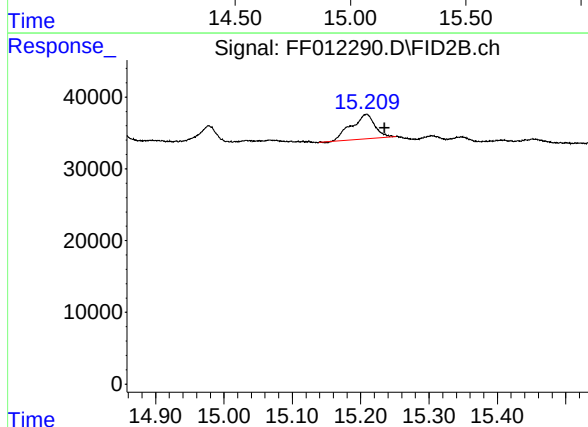


#10 N-TETRACOSANE

R.T.: 15.209 min
Delta R.T.: -0.027 min
Response: 82289
Conc: 0.66 ug/ml

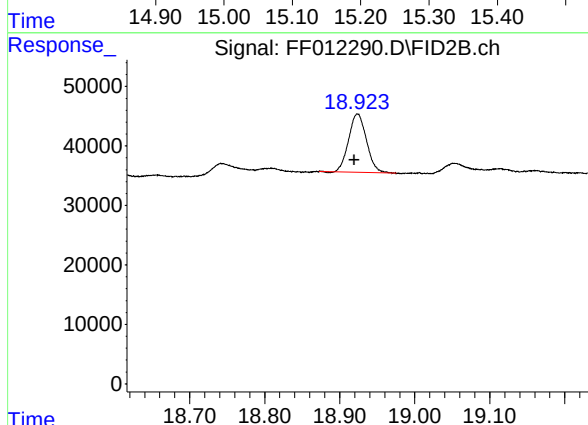


#14 N-DOTRIACONTANE

R.T.: 18.924 min
Delta R.T.: 0.004 min
Response: 162737
Conc: 1.57 ug/ml

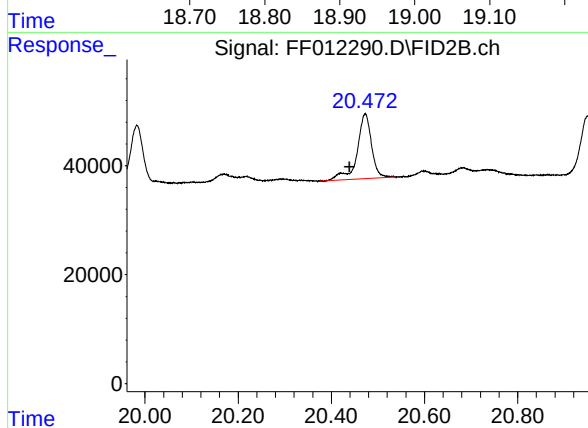

#16 N-HEXATRIACONTANE

R.T.: 20.473 min
Delta R.T.: 0.033 min
Response: 255282
Conc: 2.91 ug/ml

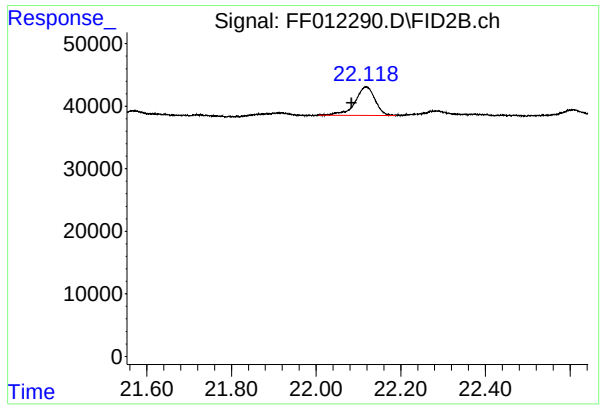

#18 N-TETRACONTANE

R.T.: 22.118 min
Delta R.T.: 0.034 min
Response: 148632
Conc: 1.82 ug/ml

Instrument :
FID_F
ClientSampleId :