

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031819\
 Data File : FF003875.D
 Signal(s) : FID2B.ch
 Acq On : 18 Mar 2019 16:14
 Operator : AJ\SJ
 Sample : K1697-11 10X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 19 01:36:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.581	374800	2.692 ug/ml
Target Compounds			
7) N-EICOSANE	12.534	1295425	7.919 ug/ml
8) N-DOCOSANE	13.703	93297	0.578 ug/ml
10) N-TETRACOSANE	14.760	714168	4.514 ug/ml
11) N-HEXACOSANE	15.809	125418	0.813 ug/ml
12) N-OCTACOSANE	16.770	273191	1.808 ug/ml
13) N-TRIACONTANE	17.649	203096	1.381 ug/ml
14) N-DOTRIACONTANE	18.491	302803	2.129 ug/ml
15) N-TETRATRIACONTANE	19.281	120091	0.897 ug/ml
16) N-HEXATRIACONTANE	20.062	625501	4.794 ug/ml
18) N-TETRACONTANE	21.664	943043	7.580 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031819\
Data File : FF003875.D
Signal(s) : FID2B.ch
Acq On : 18 Mar 2019 16:14
Operator : AJ\SJ
Sample : K1697-11 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 19 01:36:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

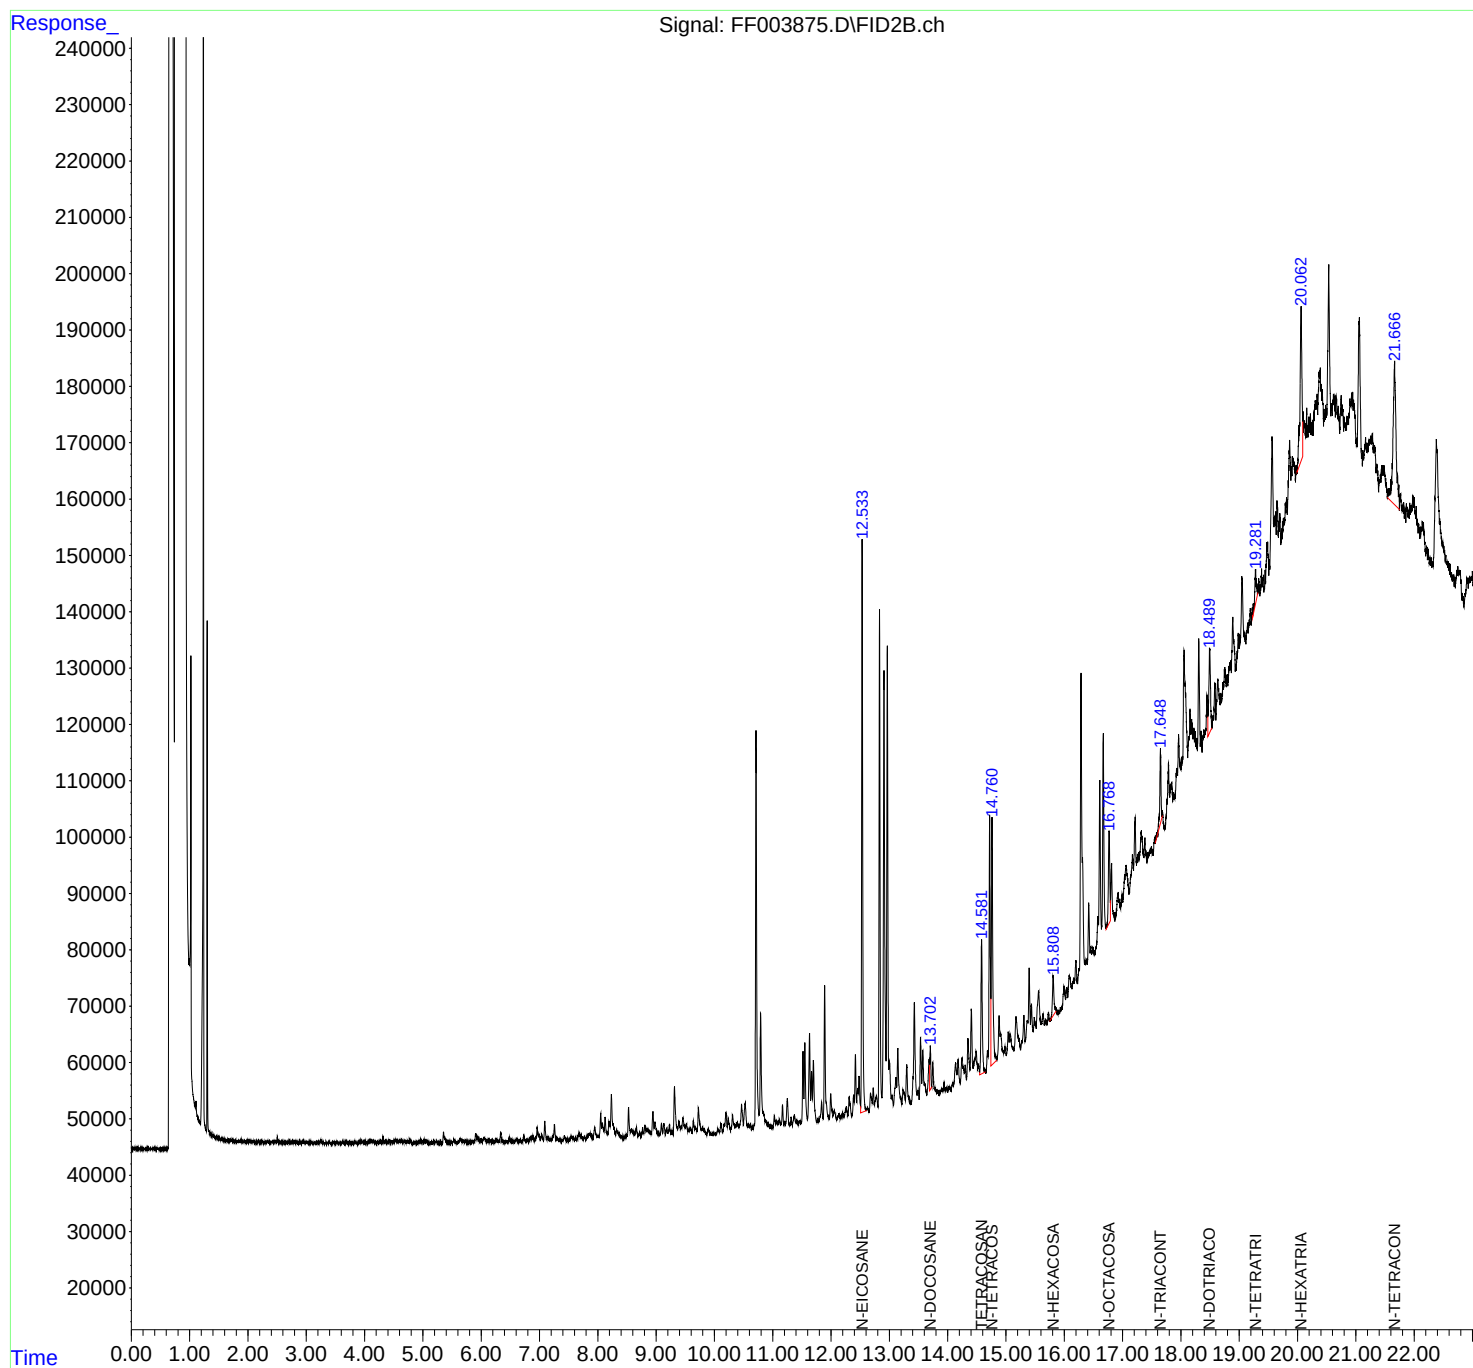

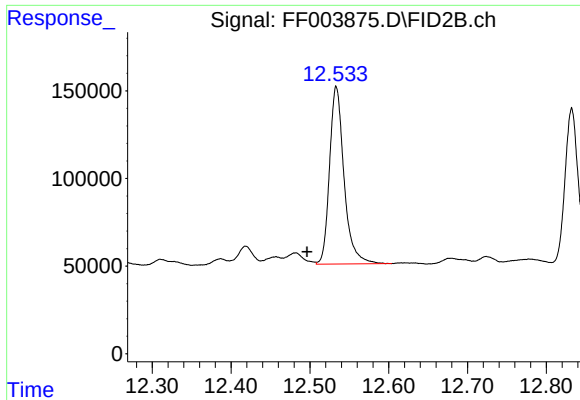


#7 N-EICOSANE

R.T.: 12.534 min
Delta R.T.: 0.037 min
Response: 1295425
Conc: 7.92 ug/ml

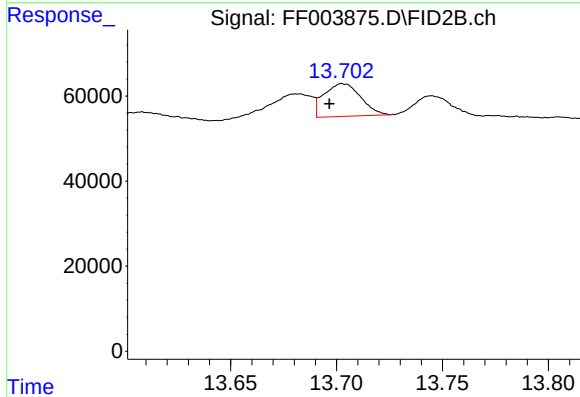


#8 N-DOCOSANE

R.T.: 13.703 min
Delta R.T.: 0.006 min
Response: 93297
Conc: 0.58 ug/ml

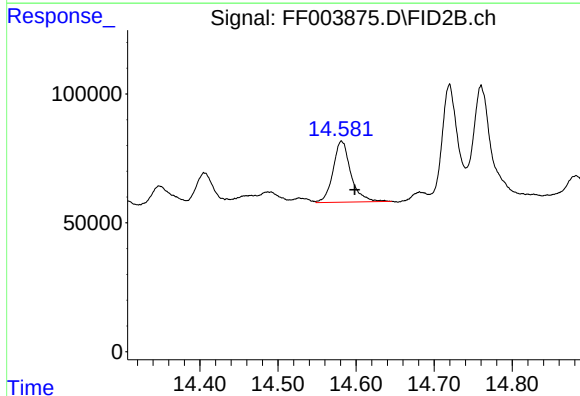


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.581 min
Delta R.T.: -0.017 min
Response: 374800
Conc: 2.69 ug/ml

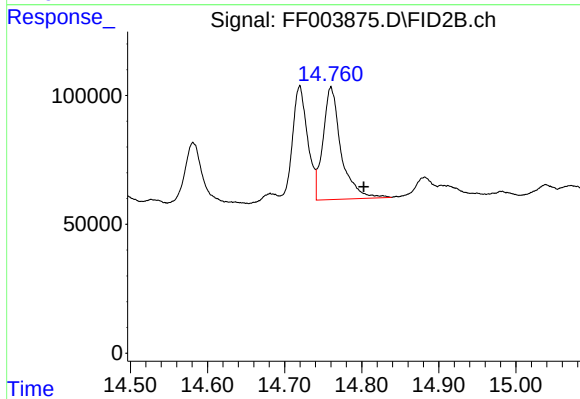


#10 N-TETRACOSANE

R.T.: 14.760 min
Delta R.T.: -0.042 min
Response: 714168
Conc: 4.51 ug/ml

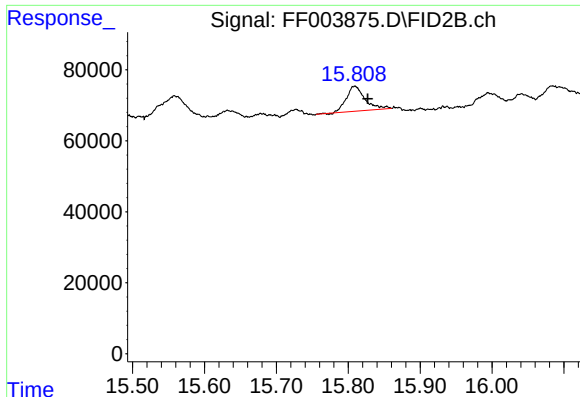


#11 N-HEXACOSANE

R.T.: 15.809 min
Delta R.T.: -0.018 min
Response: 125418
Conc: 0.81 ug/ml

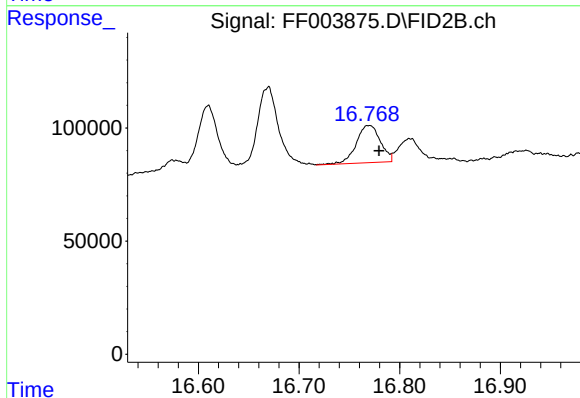


#12 N-OCTACOSANE

R.T.: 16.770 min
Delta R.T.: -0.010 min
Response: 273191
Conc: 1.81 ug/ml

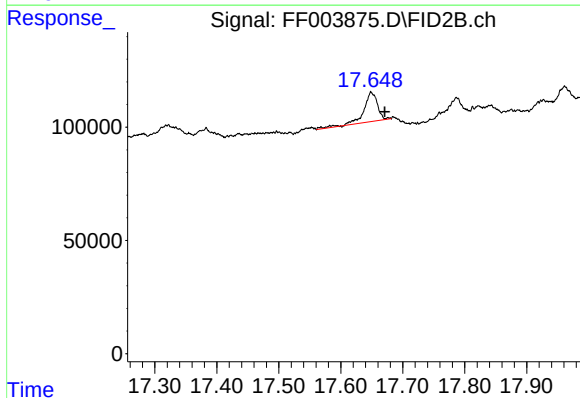


#13 N-TRIACONTANE

R.T.: 17.649 min
Delta R.T.: -0.022 min
Response: 203096
Conc: 1.38 ug/ml

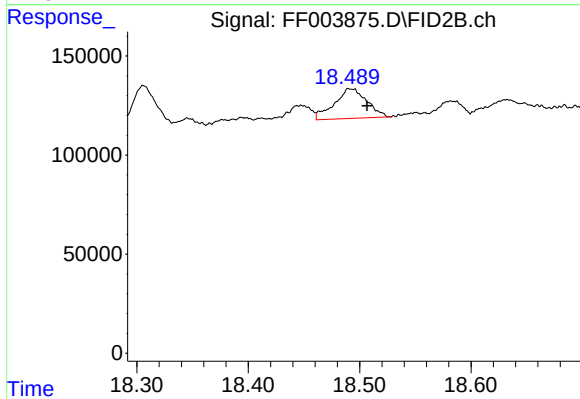

#14 N-DOTRIACONTANE

R.T.: 18.491 min
Delta R.T.: -0.016 min
Response: 302803
Conc: 2.13 ug/ml

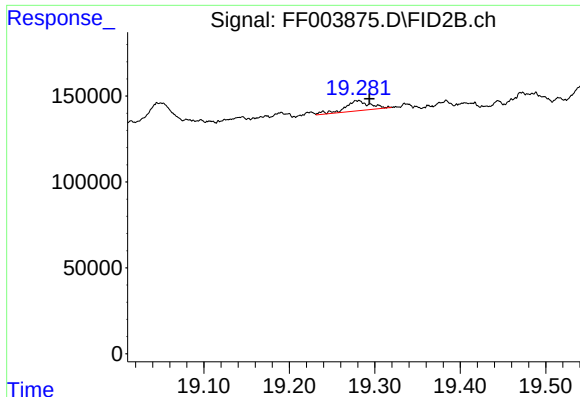


#15 N-TETRATRIACONTANE

R.T.: 19.281 min

Delta R.T.: -0.012 min

Response: 120091

Conc: 0.90 ug/ml

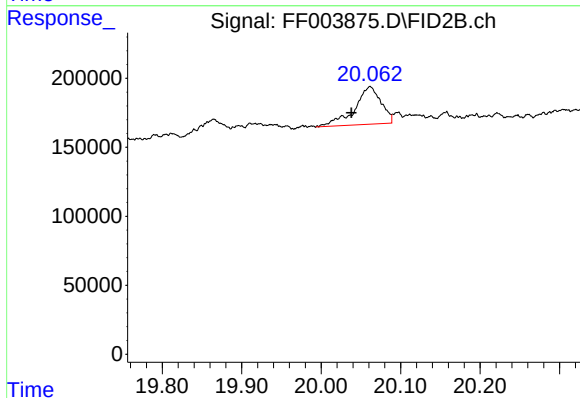


#16 N-HEXATRIACONTANE

R.T.: 20.062 min

Delta R.T.: 0.024 min

Response: 625501

Conc: 4.79 ug/ml

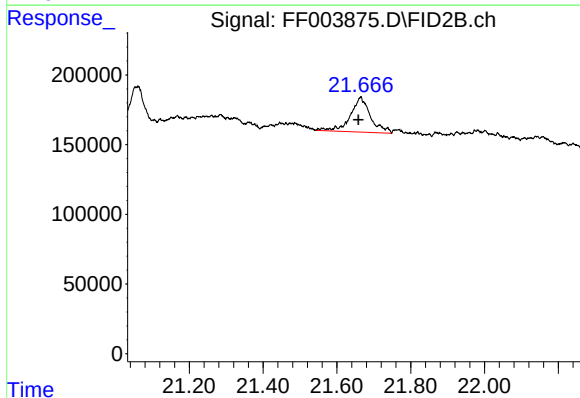

#18 N-TETRACONTANE

R.T.: 21.664 min

Delta R.T.: 0.005 min

Response: 943043

Conc: 7.58 ug/ml