

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031819\
 Data File : FF003878.D
 Signal(s) : FID2B.ch
 Acq On : 18 Mar 2019 17:44
 Operator : AJ\SJ
 Sample : K1930-11MS
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 19 01:37:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.582	1659981	11.923 ug/ml
Target Compounds			
2) N-DECANE	4.313	2115535	13.753 ug/ml
3) N-DODECANE	6.334	2111967	13.533 ug/ml
4) N-TETRADECANE	8.126	2074957	12.941 ug/ml
5) N-HEXADECANE	9.727	2053216	12.606 ug/ml
6) N-OCTADECANE	11.169	2005296	12.171 ug/ml
7) N-EICOSANE	12.480	1951500	11.929 ug/ml
8) N-DOCOSANE	13.681	1943418	12.042 ug/ml
10) N-TETRACOSANE	14.786	1893860	11.970 ug/ml
11) N-HEXACOSANE	15.811	1889489	12.242 ug/ml
12) N-OCTACOSANE	16.763	1927934	12.758 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031819\
Data File : FF003878.D
Signal(s) : FID2B.ch
Acq On : 18 Mar 2019 17:44
Operator : AJ\SJ
Sample : K1930-11MS
Misc :
ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 19 01:37:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

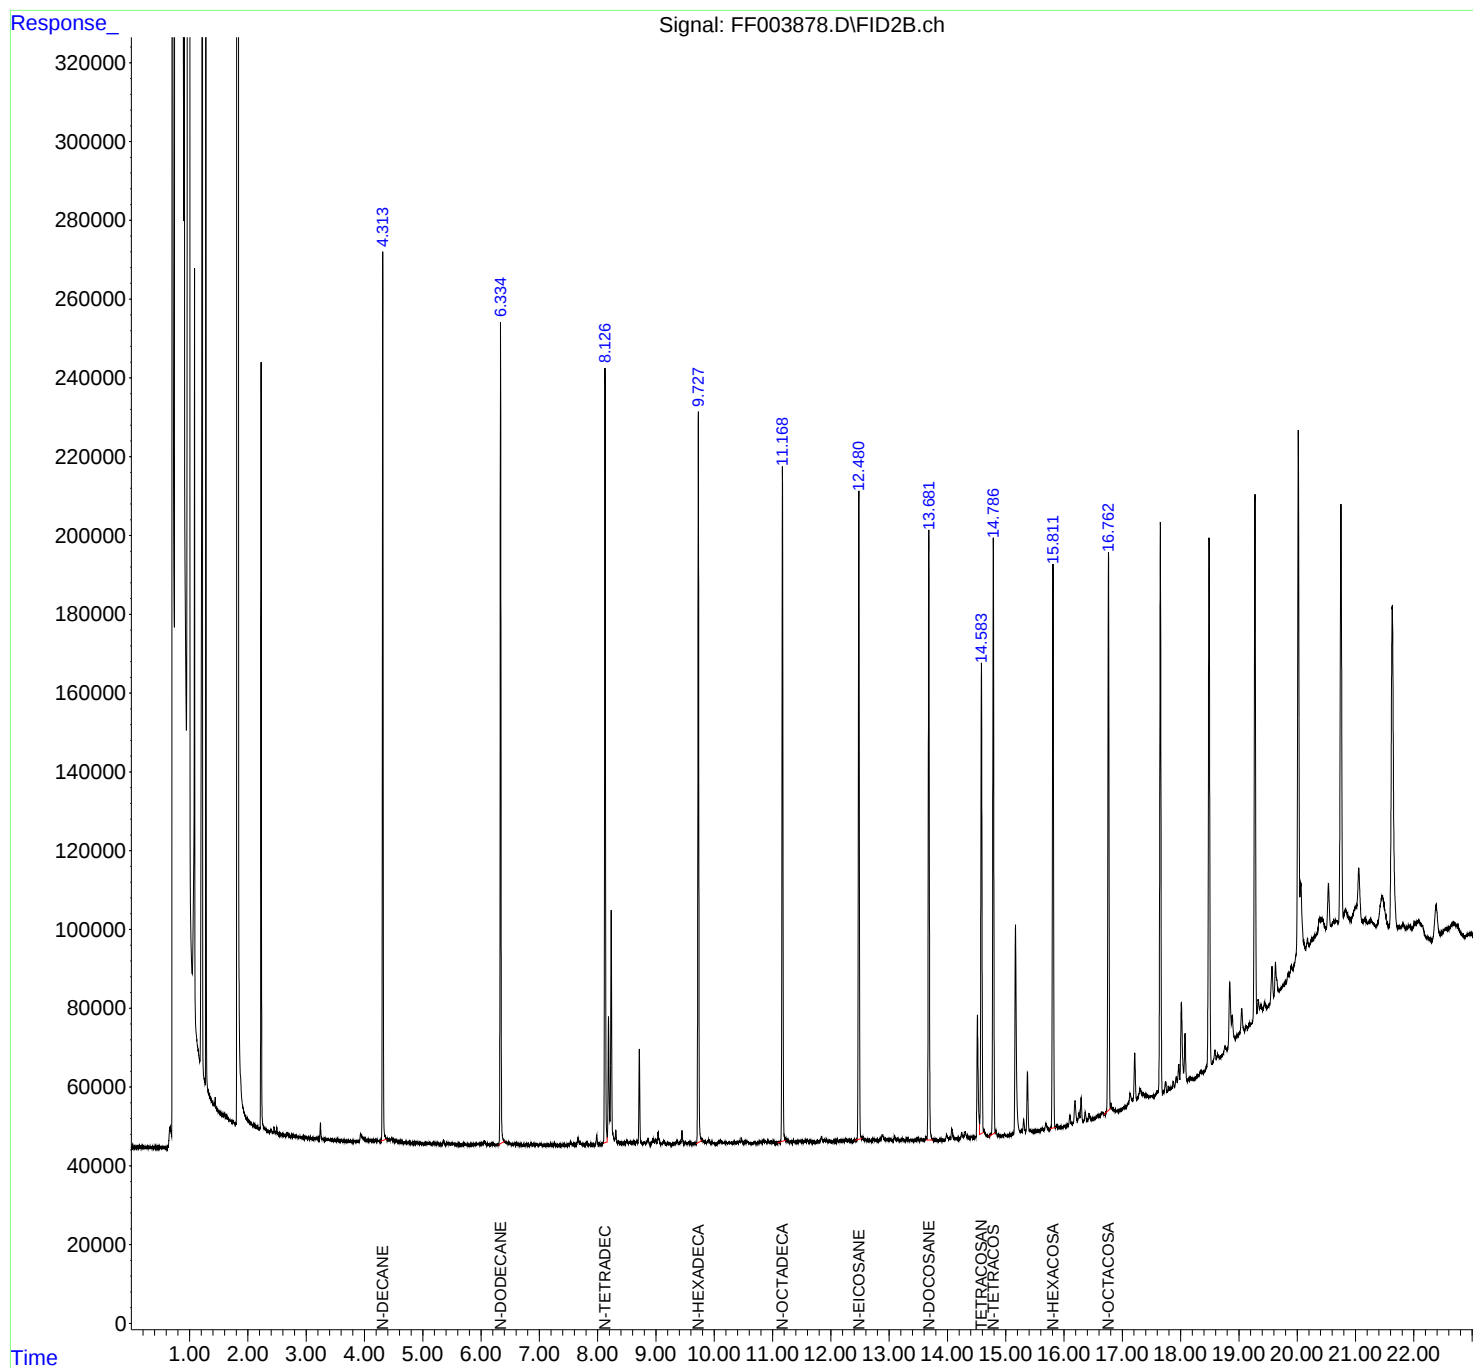

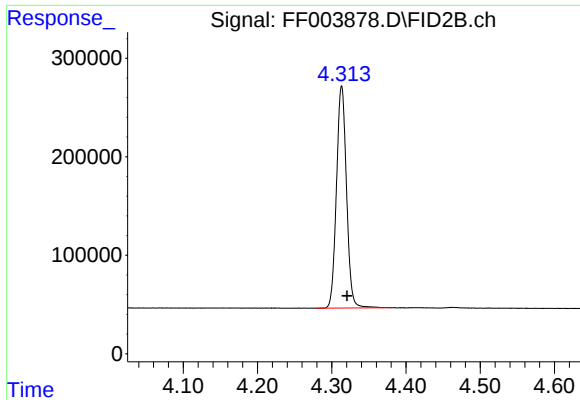


#2 N-DECANE

R.T.: 4.313 min
Delta R.T.: -0.007 min
Response: 2115535
Conc: 13.75 ug/ml

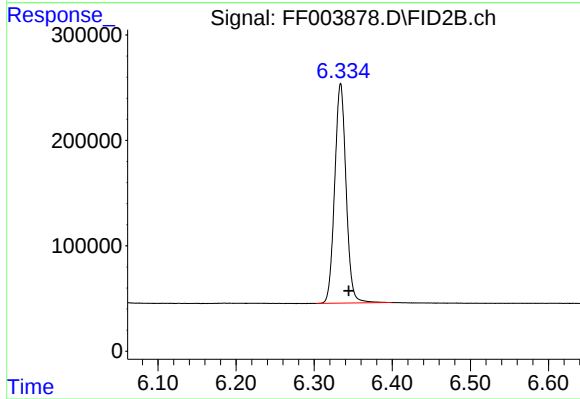


#3 N-DODECANE

R.T.: 6.334 min
Delta R.T.: -0.010 min
Response: 2111967
Conc: 13.53 ug/ml

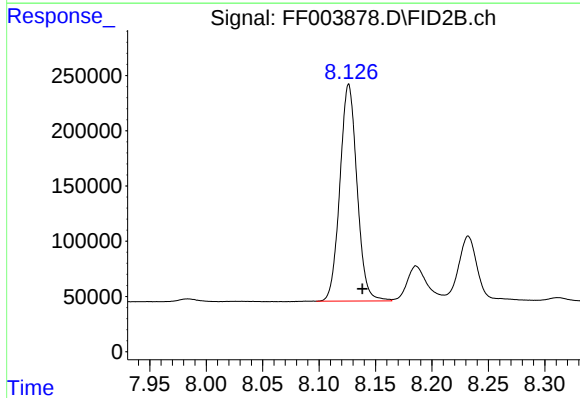


#4 N-TETRADECANE

R.T.: 8.126 min
Delta R.T.: -0.012 min
Response: 2074957
Conc: 12.94 ug/ml

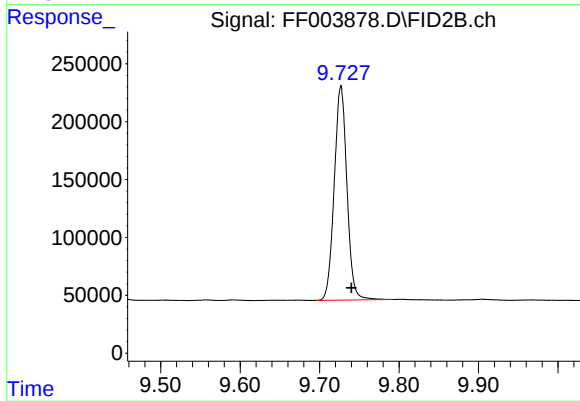


#5 N-HEXADECANE

R.T.: 9.727 min
Delta R.T.: -0.013 min
Response: 2053216
Conc: 12.61 ug/ml

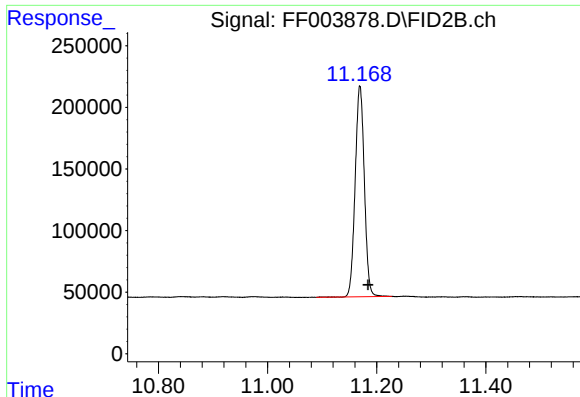


#6 N-OCTADECANE

R.T.: 11.169 min
Delta R.T.: -0.015 min
Response: 2005296
Conc: 12.17 ug/ml

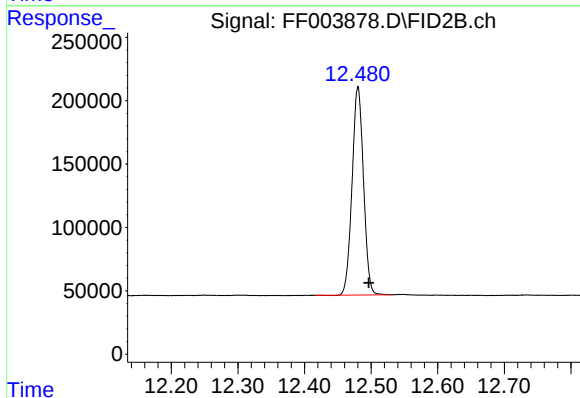


#7 N-EICOSANE

R.T.: 12.480 min
Delta R.T.: -0.016 min
Response: 1951500
Conc: 11.93 ug/ml

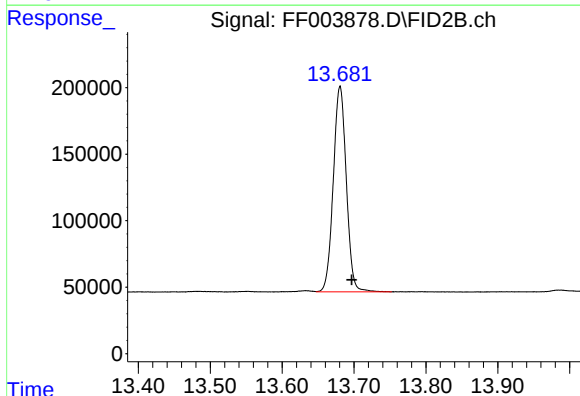


#8 N-DOCOSANE

R.T.: 13.681 min
Delta R.T.: -0.016 min
Response: 1943418
Conc: 12.04 ug/ml

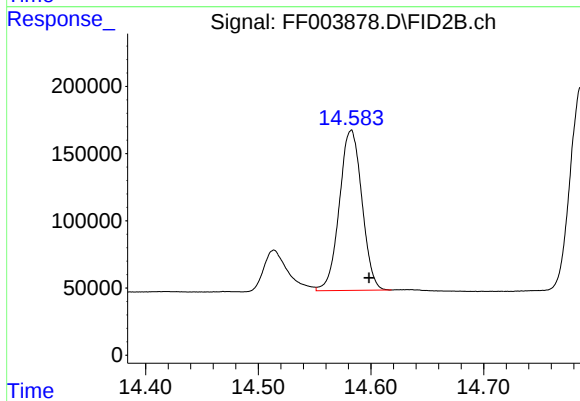


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.582 min
Delta R.T.: -0.016 min
Response: 1659981
Conc: 11.92 ug/ml

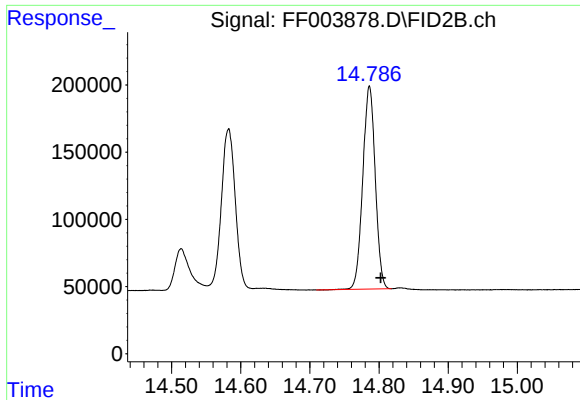


#10 N-TETRACOSANE

R.T.: 14.786 min
Delta R.T.: -0.016 min
Response: 1893860
Conc: 11.97 ug/ml

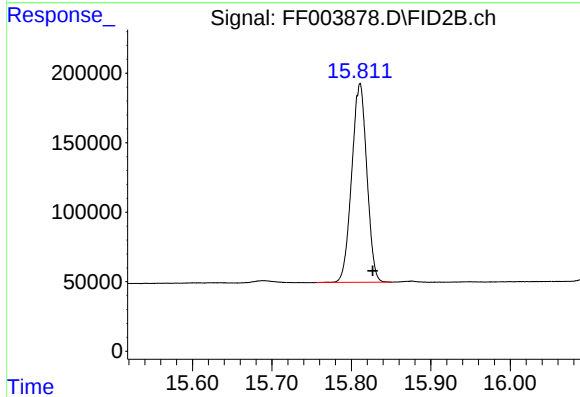

#11 N-HEXACOSANE

R.T.: 15.811 min
Delta R.T.: -0.016 min
Response: 1889489
Conc: 12.24 ug/ml

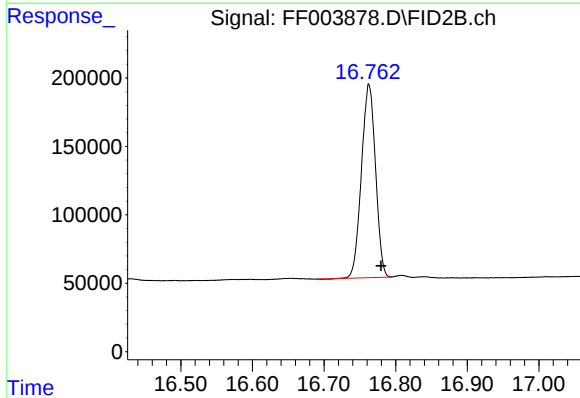

#12 N-OCTACOSANE

R.T.: 16.763 min
Delta R.T.: -0.017 min
Response: 1927934
Conc: 12.76 ug/ml