

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031819\
 Data File : FF003884.D
 Signal(s) : FID2B.ch
 Acq On : 18 Mar 2019 20:46
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 19 01:38:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.583	6228822	44.738 ug/ml
Target Compounds			
2) N-DECANE	4.314	8415447	54.710 ug/ml
3) N-DODECANE	6.336	8307300	53.230 ug/ml
4) N-TETRADECANE	8.128	8135193	50.739 ug/ml
5) N-HEXADECANE	9.729	7905709	48.540 ug/ml
6) N-OCTADECANE	11.171	7676409	46.593 ug/ml
7) N-EICOSANE	12.482	7400698	45.239 ug/ml
8) N-DOCOSANE	13.682	7192802	44.568 ug/ml
10) N-TETRACOSANE	14.788	7079155	44.742 ug/ml
11) N-HEXACOSANE	15.811	7048143	45.665 ug/ml
12) N-OCTACOSANE	16.764	7135626	47.220 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031819\
Data File : FF003884.D
Signal(s) : FID2B.ch
Acq On : 18 Mar 2019 20:46
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 19 01:38:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

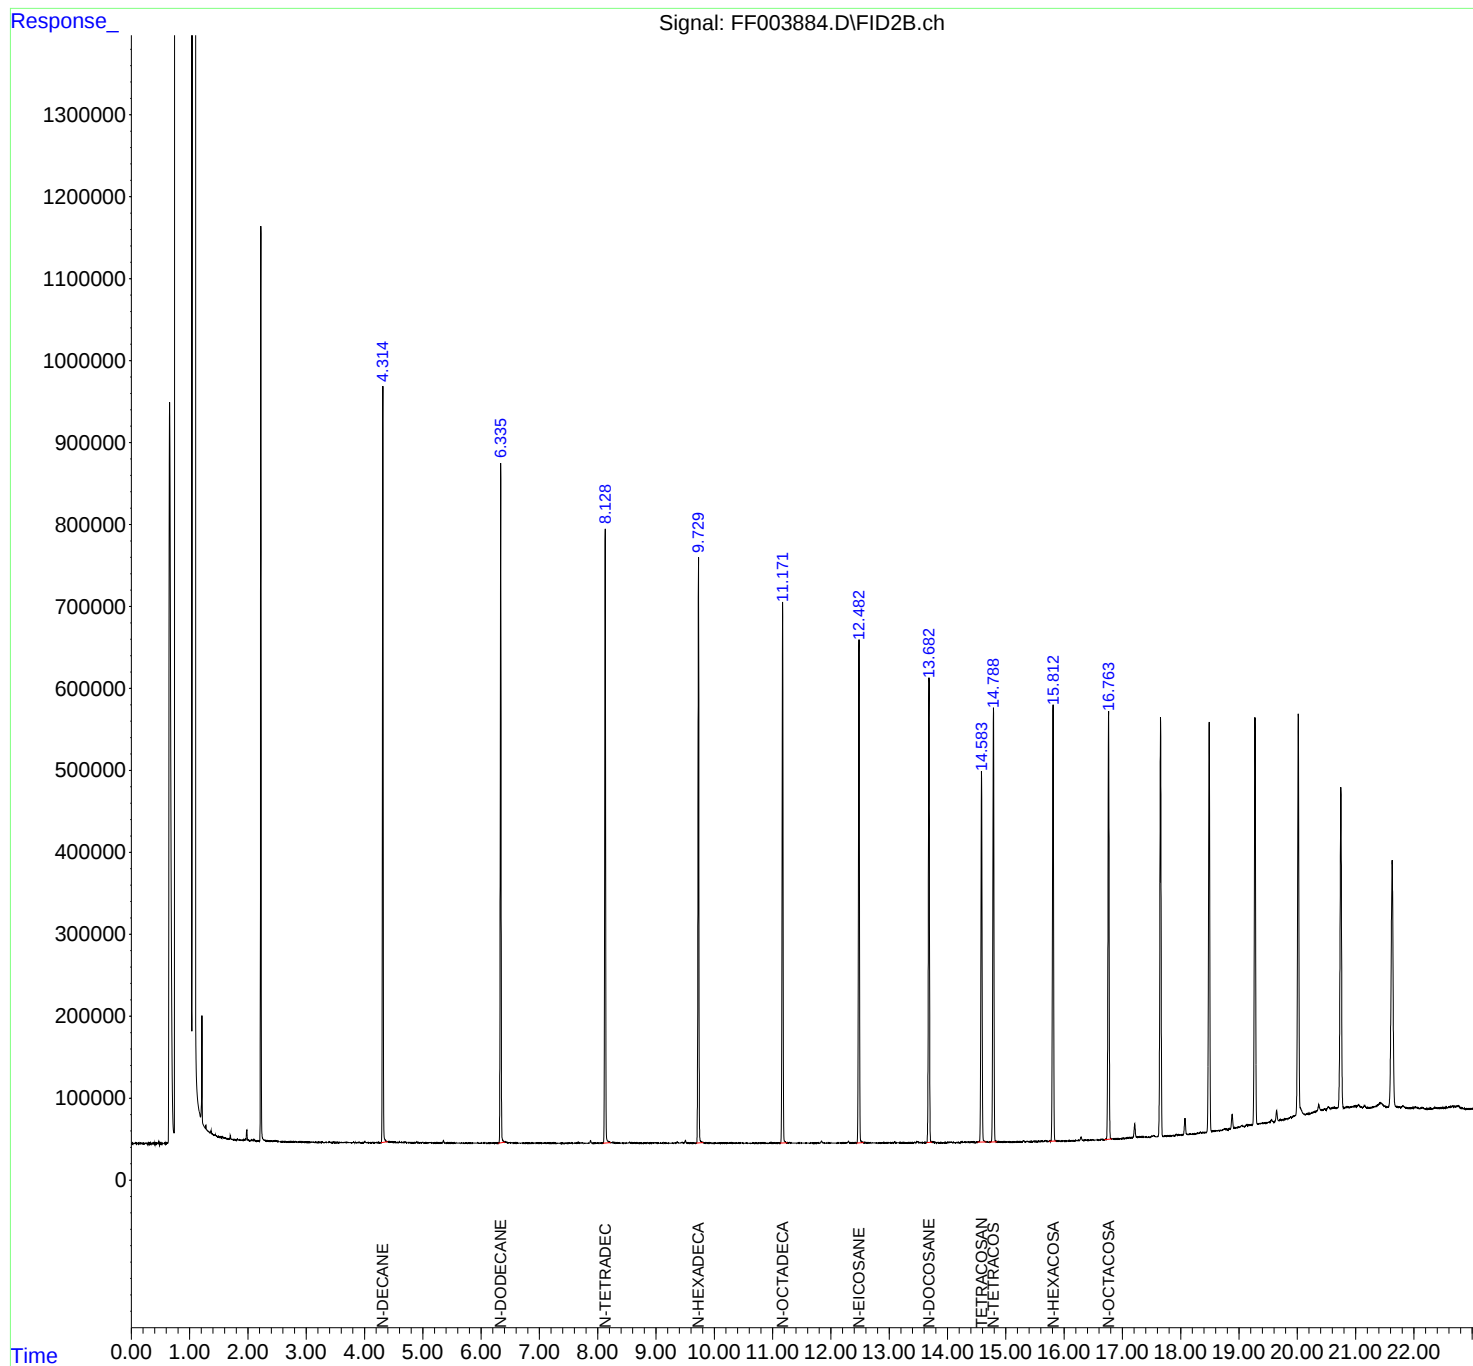

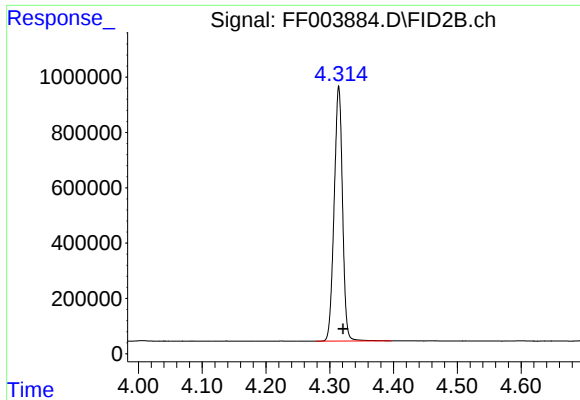


#2 N-DECANE

R.T.: 4.314 min
Delta R.T.: -0.007 min
Response: 8415447
Conc: 54.71 ug/ml

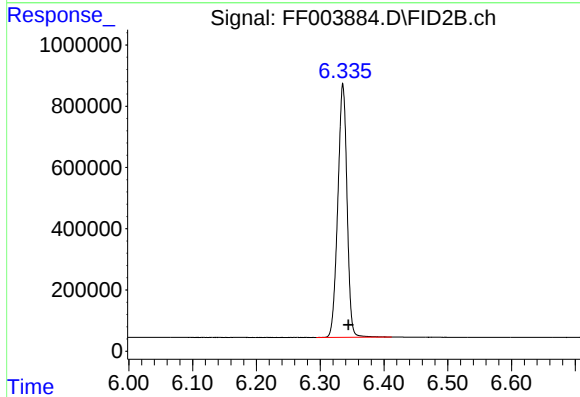


#3 N-DODECANE

R.T.: 6.336 min
Delta R.T.: -0.008 min
Response: 8307300
Conc: 53.23 ug/ml

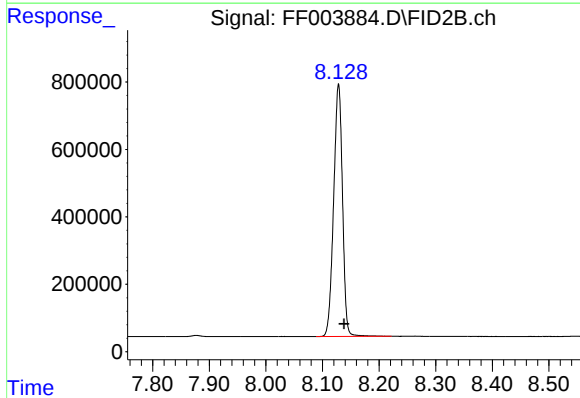


#4 N-TETRADECANE

R.T.: 8.128 min
Delta R.T.: -0.010 min
Response: 8135193
Conc: 50.74 ug/ml

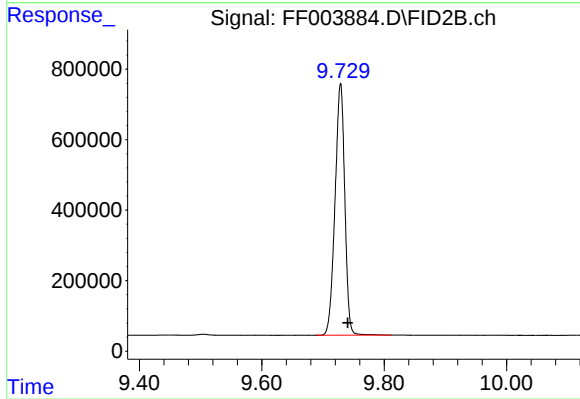


#5 N-HEXADECANE

R.T.: 9.729 min
Delta R.T.: -0.011 min
Response: 7905709
Conc: 48.54 ug/ml

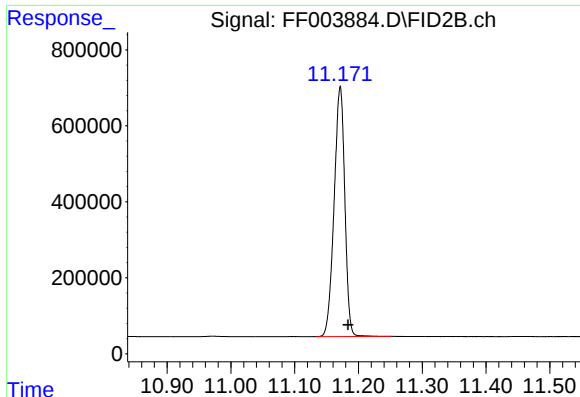


#6 N-OCTADECANE

R.T.: 11.171 min
Delta R.T.: -0.012 min
Response: 7676409
Conc: 46.59 ug/ml

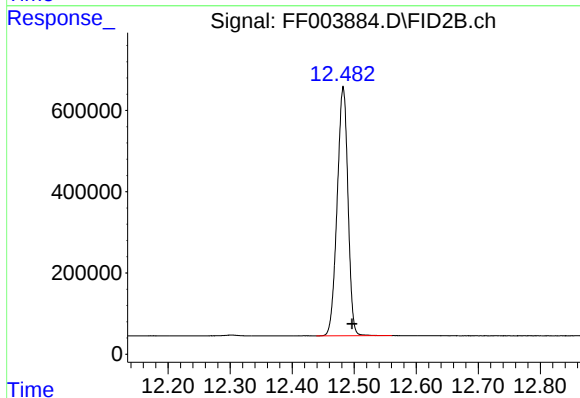


#7 N-EICOSANE

R.T.: 12.482 min
Delta R.T.: -0.014 min
Response: 7400698
Conc: 45.24 ug/ml

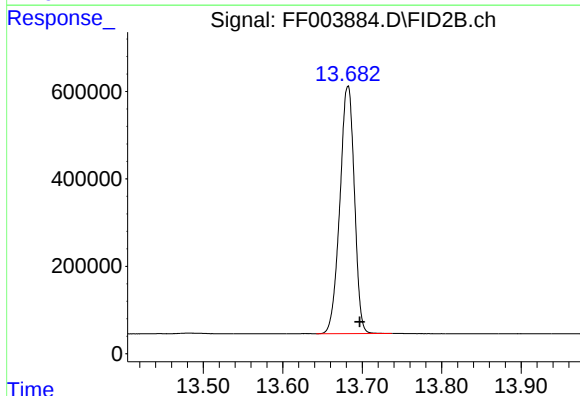


#8 N-DOCOSANE

R.T.: 13.682 min
Delta R.T.: -0.015 min
Response: 7192802
Conc: 44.57 ug/ml

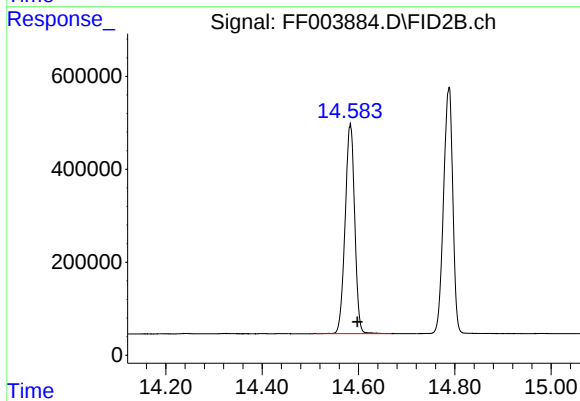


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.583 min
Delta R.T.: -0.015 min
Response: 6228822
Conc: 44.74 ug/ml

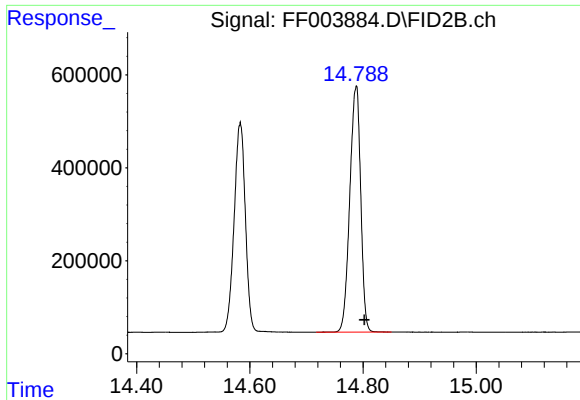


#10 N-TETRACOSANE

R.T.: 14.788 min
Delta R.T.: -0.014 min
Response: 7079155
Conc: 44.74 ug/ml

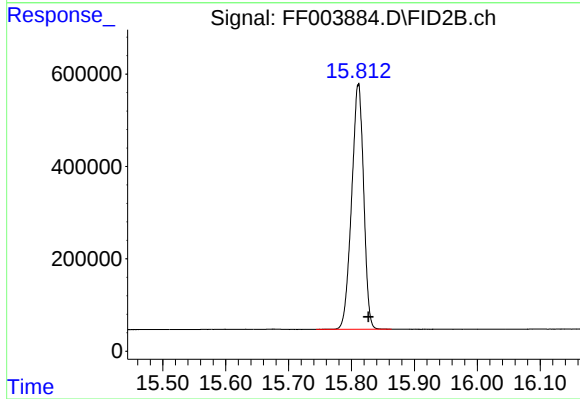

#11 N-HEXACOSANE

R.T.: 15.811 min
Delta R.T.: -0.016 min
Response: 7048143
Conc: 45.67 ug/ml

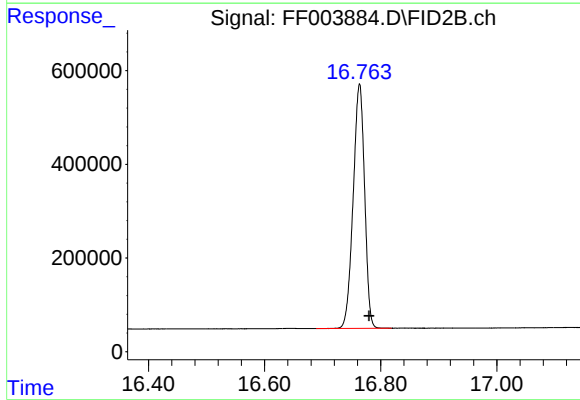

#12 N-OCTACOSANE

R.T.: 16.764 min
Delta R.T.: -0.016 min
Response: 7135626
Conc: 47.22 ug/ml