

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
Data File : FF010072.D
Signal(s) : FID2B.ch
Acq On : 18 Mar 2022 13:57
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 18 23:29:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
15) N-TETRATRIACONTANE	19.374	174757	1.276 ug/ml
16) N-HEXATRIACONTANE	20.159	451324	3.630 ug/ml
17) N-OCTATRIACONTANE	20.836	817943	7.345 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
Data File : FF010072.D
Signal(s) : FID2B.ch
Acq On : 18 Mar 2022 13:57
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 18 23:29:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

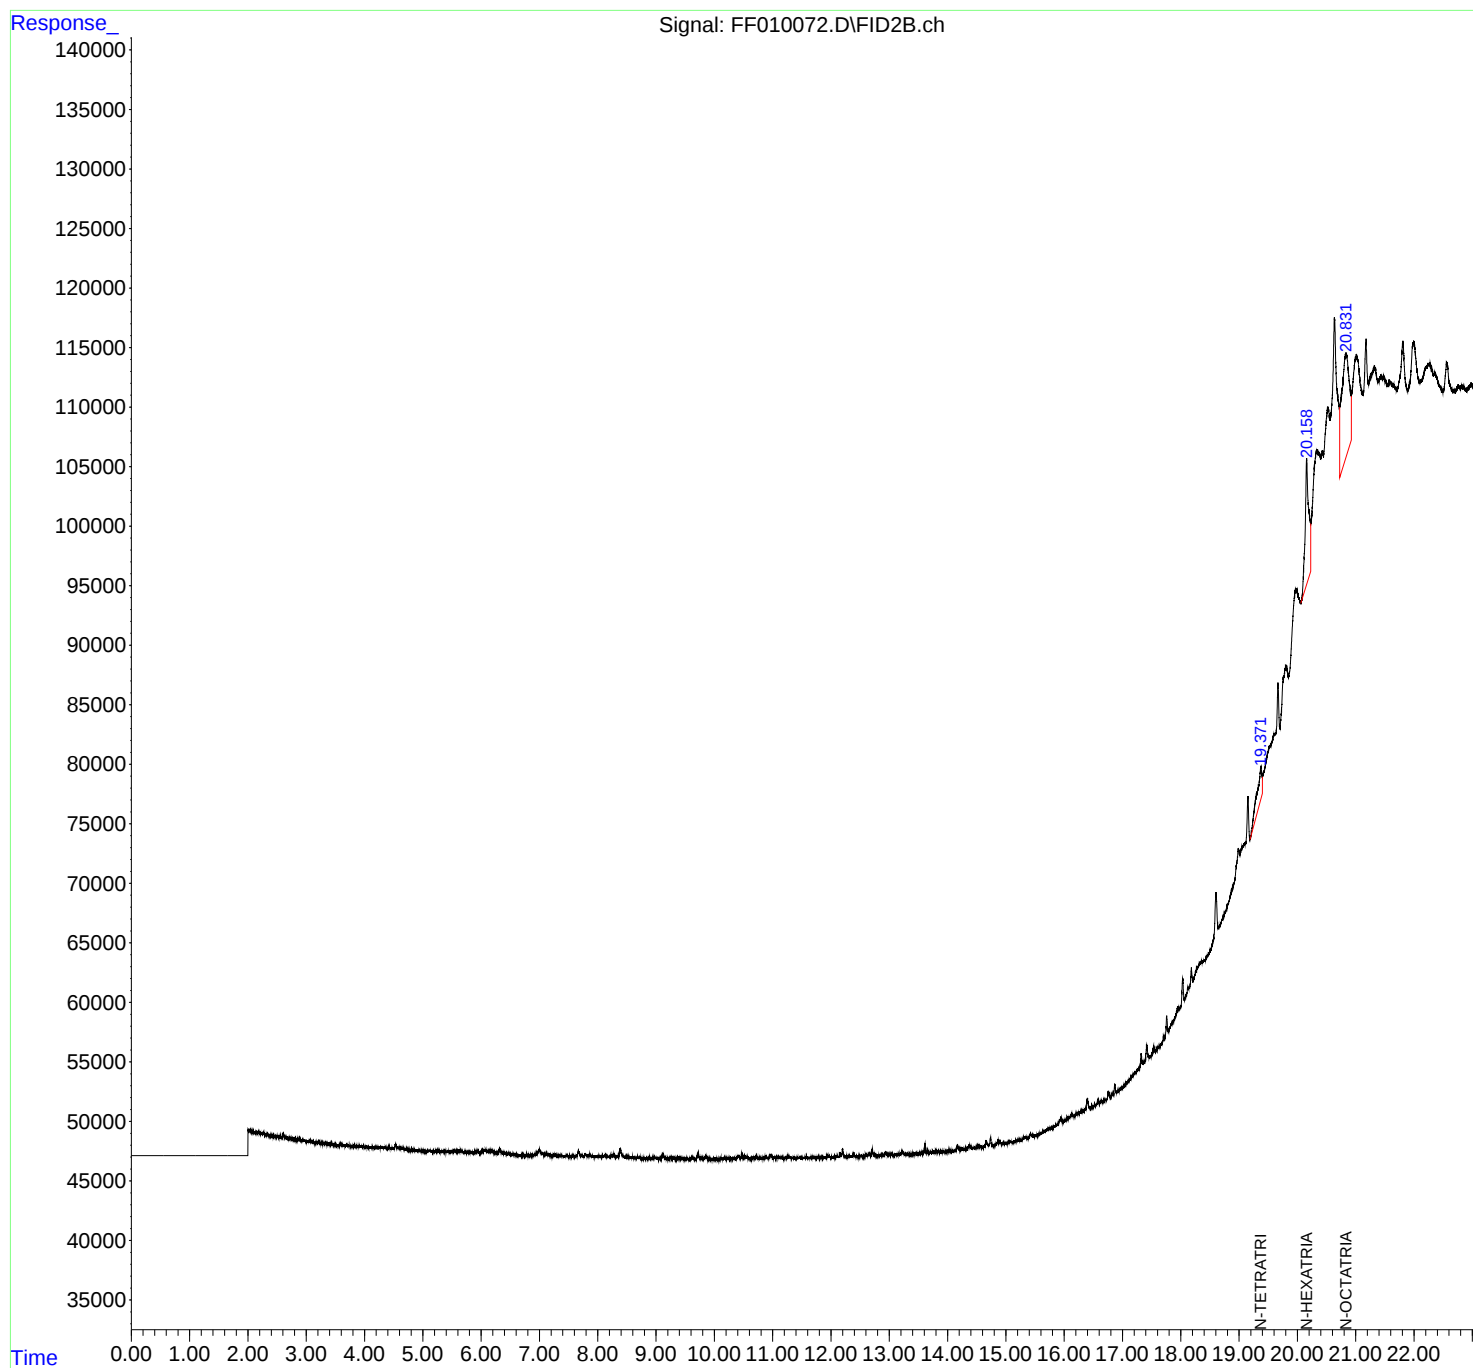


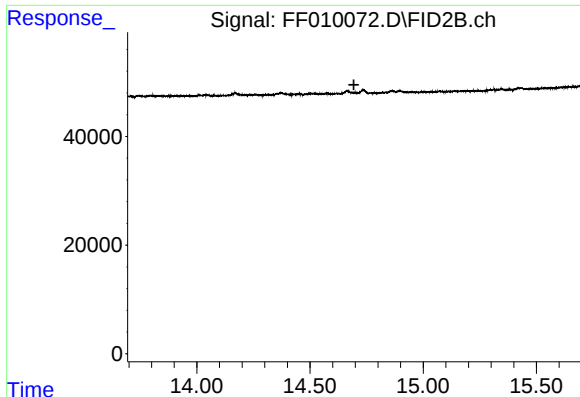

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.694 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

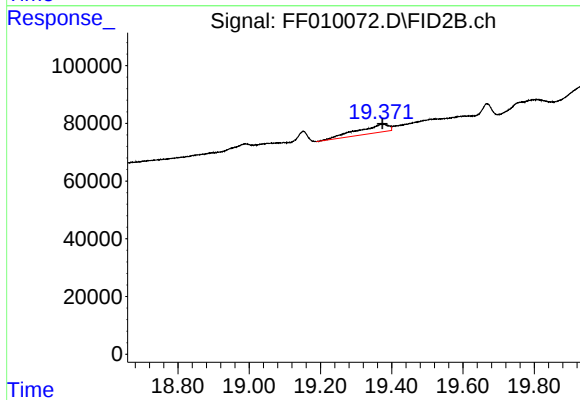


#15 N-TETRATRIACONTANE

R.T.: 19.374 min
Delta R.T.: 0.000 min
Response: 174757
Conc: 1.28 ug/ml

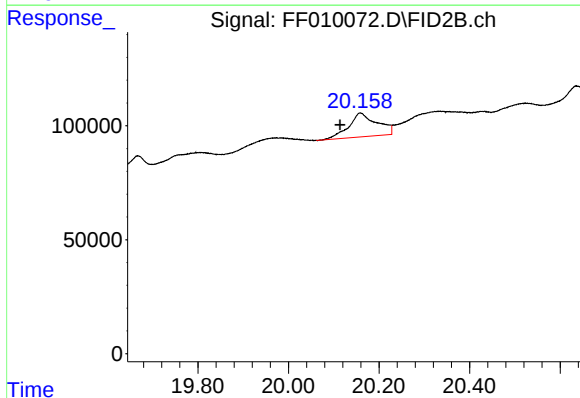

#16 N-HEXATRIACONTANE

R.T.: 20.159 min
Delta R.T.: 0.045 min
Response: 451324
Conc: 3.63 ug/ml

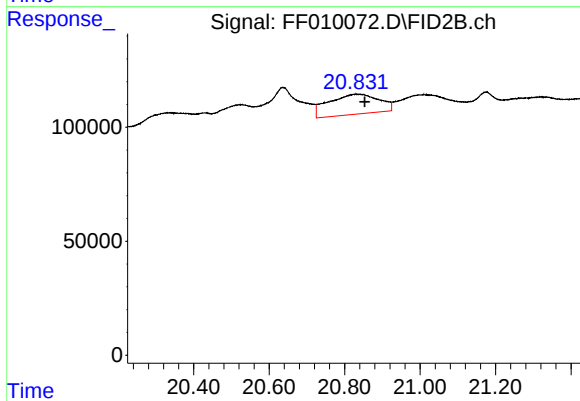

#17 N-OCTATRIACONTANE

R.T.: 20.836 min
Delta R.T.: -0.017 min
Response: 817943
Conc: 7.35 ug/ml