

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
Data File : FF010076.D
Signal(s) : FID2B.ch
Acq On : 18 Mar 2022 16:30
Operator : AJ\MA
Sample : PB143446BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 18 23:30:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.694	2756814	18.383 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.607	129352	0.886 ug/ml
16) N-HEXATRIACONTANE	20.159	221960	1.785 ug/ml
17) N-OCTATRIACONTANE	20.811	272324	2.446 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
Data File : FF010076.D
Signal(s) : FID2B.ch
Acq On : 18 Mar 2022 16:30
Operator : AJ\MA
Sample : PB143446BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 18 23:30:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

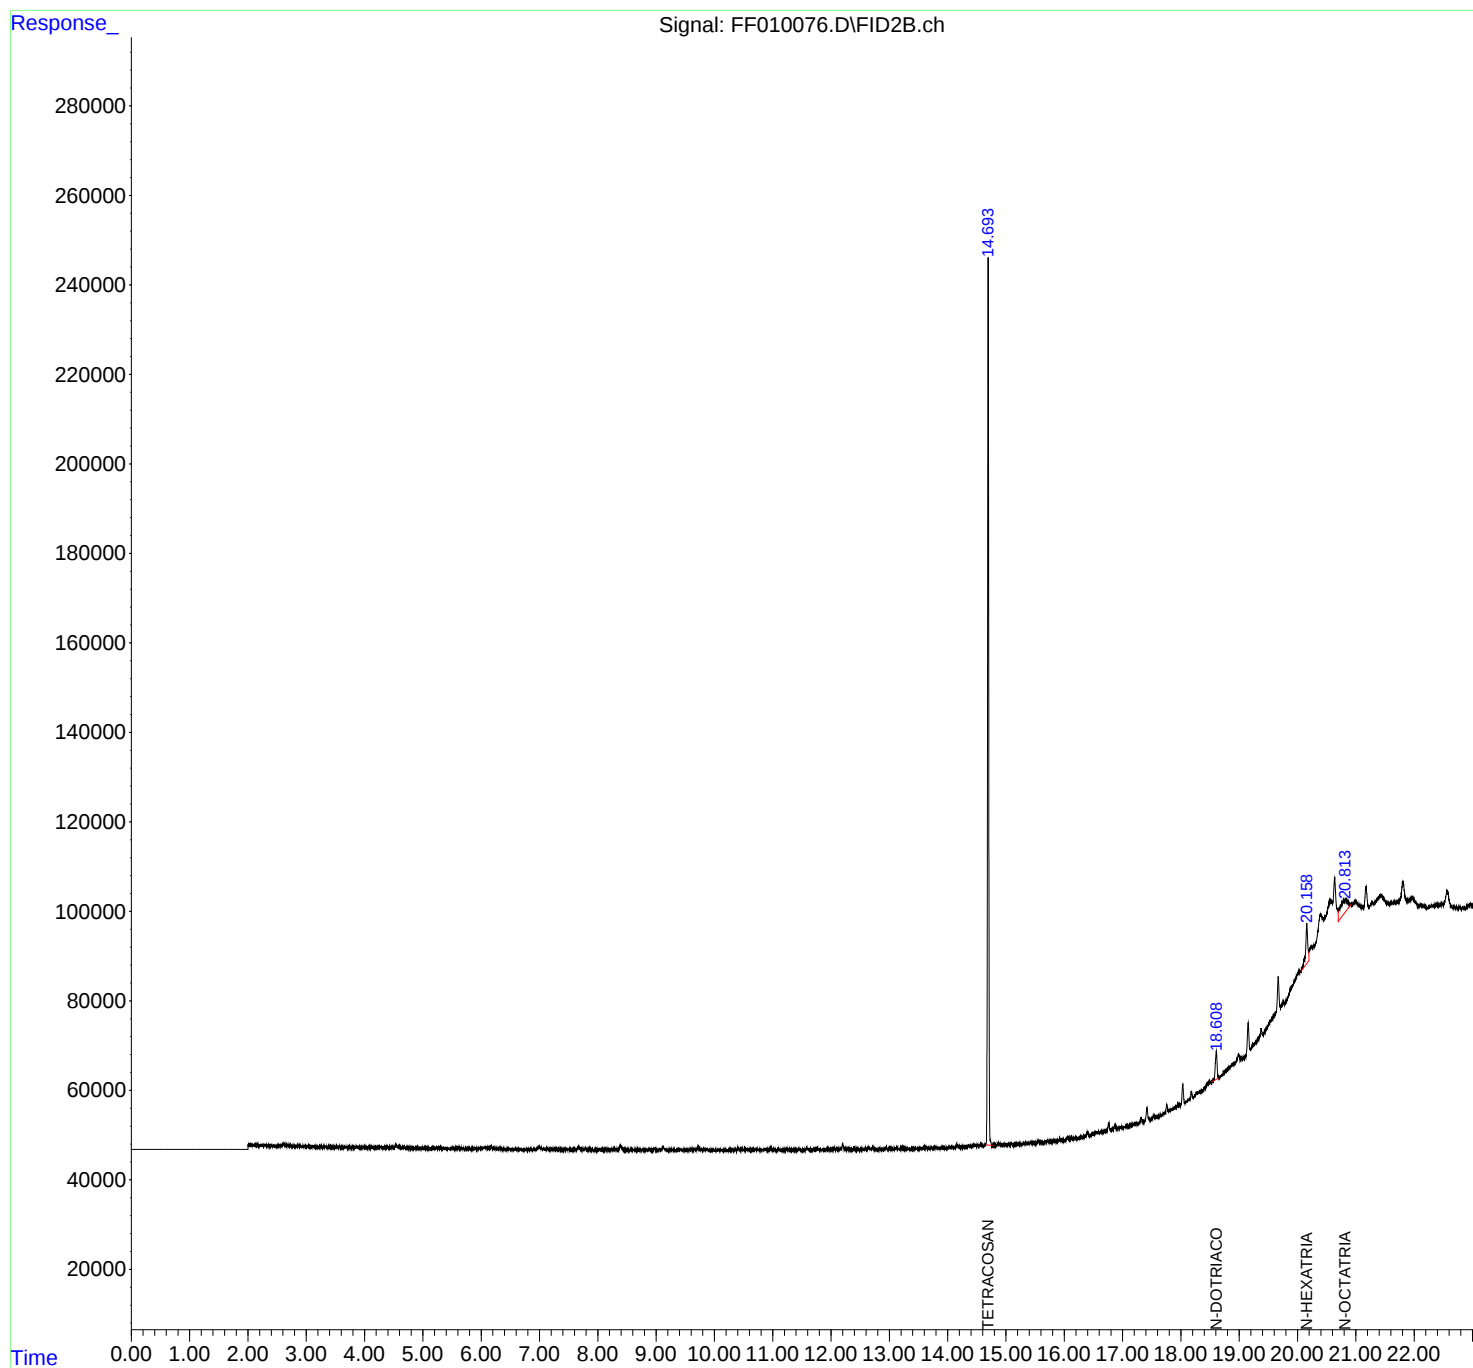


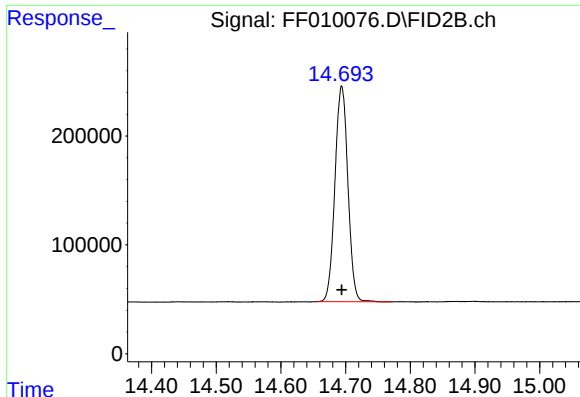

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.694 min
Delta R.T.: 0.000 min
Response: 2756814
Conc: 18.38 ug/ml

Instrument :
FID_F
ClientSampleId :

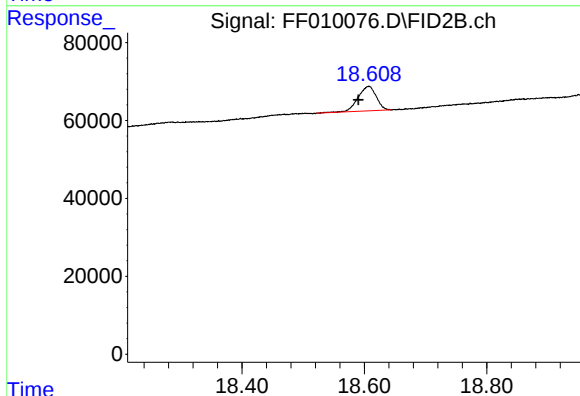


#14 N-DOTRIACONTANE

R.T.: 18.607 min
Delta R.T.: 0.017 min
Response: 129352
Conc: 0.89 ug/ml

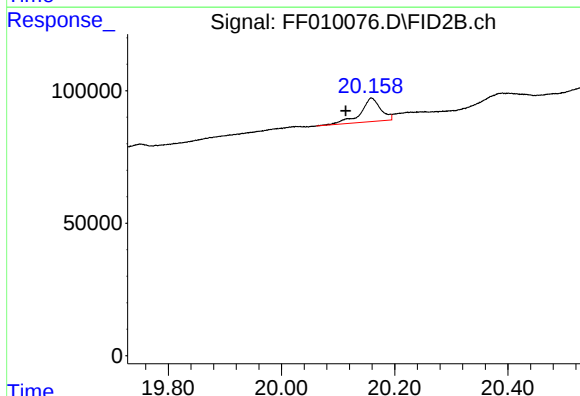

#16 N-HEXATRIACONTANE

R.T.: 20.159 min
Delta R.T.: 0.045 min
Response: 221960
Conc: 1.79 ug/ml

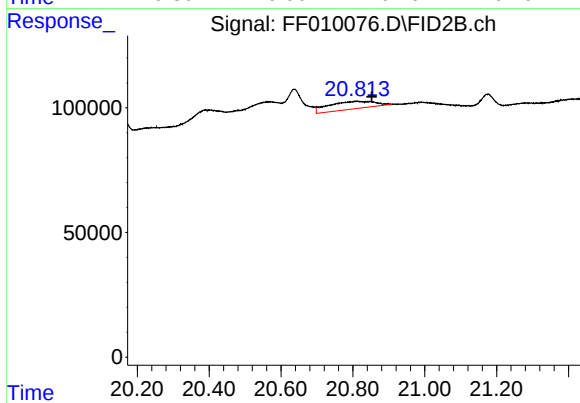

#17 N-OCTATRIACONTANE

R.T.: 20.811 min
Delta R.T.: -0.042 min
Response: 272324
Conc: 2.45 ug/ml