

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
 Data File : FF010078.D
 Signal(s) : FID2B.ch
 Acq On : 18 Mar 2022 17:31
 Operator : AJ\MA
 Sample : N1994-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 18 23:30:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
 Quant Title :
 QLast Update : Thu Mar 10 12:46:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.693	1961164	13.077 ug/ml
Target Compounds			
7) N-EICOSANE	12.652f	535896	3.086 ug/ml
10) N-TETRACOSANE	14.868	272055	1.611 ug/ml
12) N-OCTACOSANE	16.866	82733	0.517 ug/ml
14) N-DOTRIACONTANE	18.605	253319	1.735 ug/ml
15) N-TETRATRIACONTANE	19.374	64097	0.468 ug/ml
16) N-HEXATRIACONTANE	20.158	277433	2.231 ug/ml
17) N-OCTATRIACONTANE	20.851	107402	0.964 ug/ml
18) N-TETRACONTANE	21.810	565971	5.515 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
Data File : FF010078.D
Signal(s) : FID2B.ch
Acq On : 18 Mar 2022 17:31
Operator : AJ\MA
Sample : N1994-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 18 23:30:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

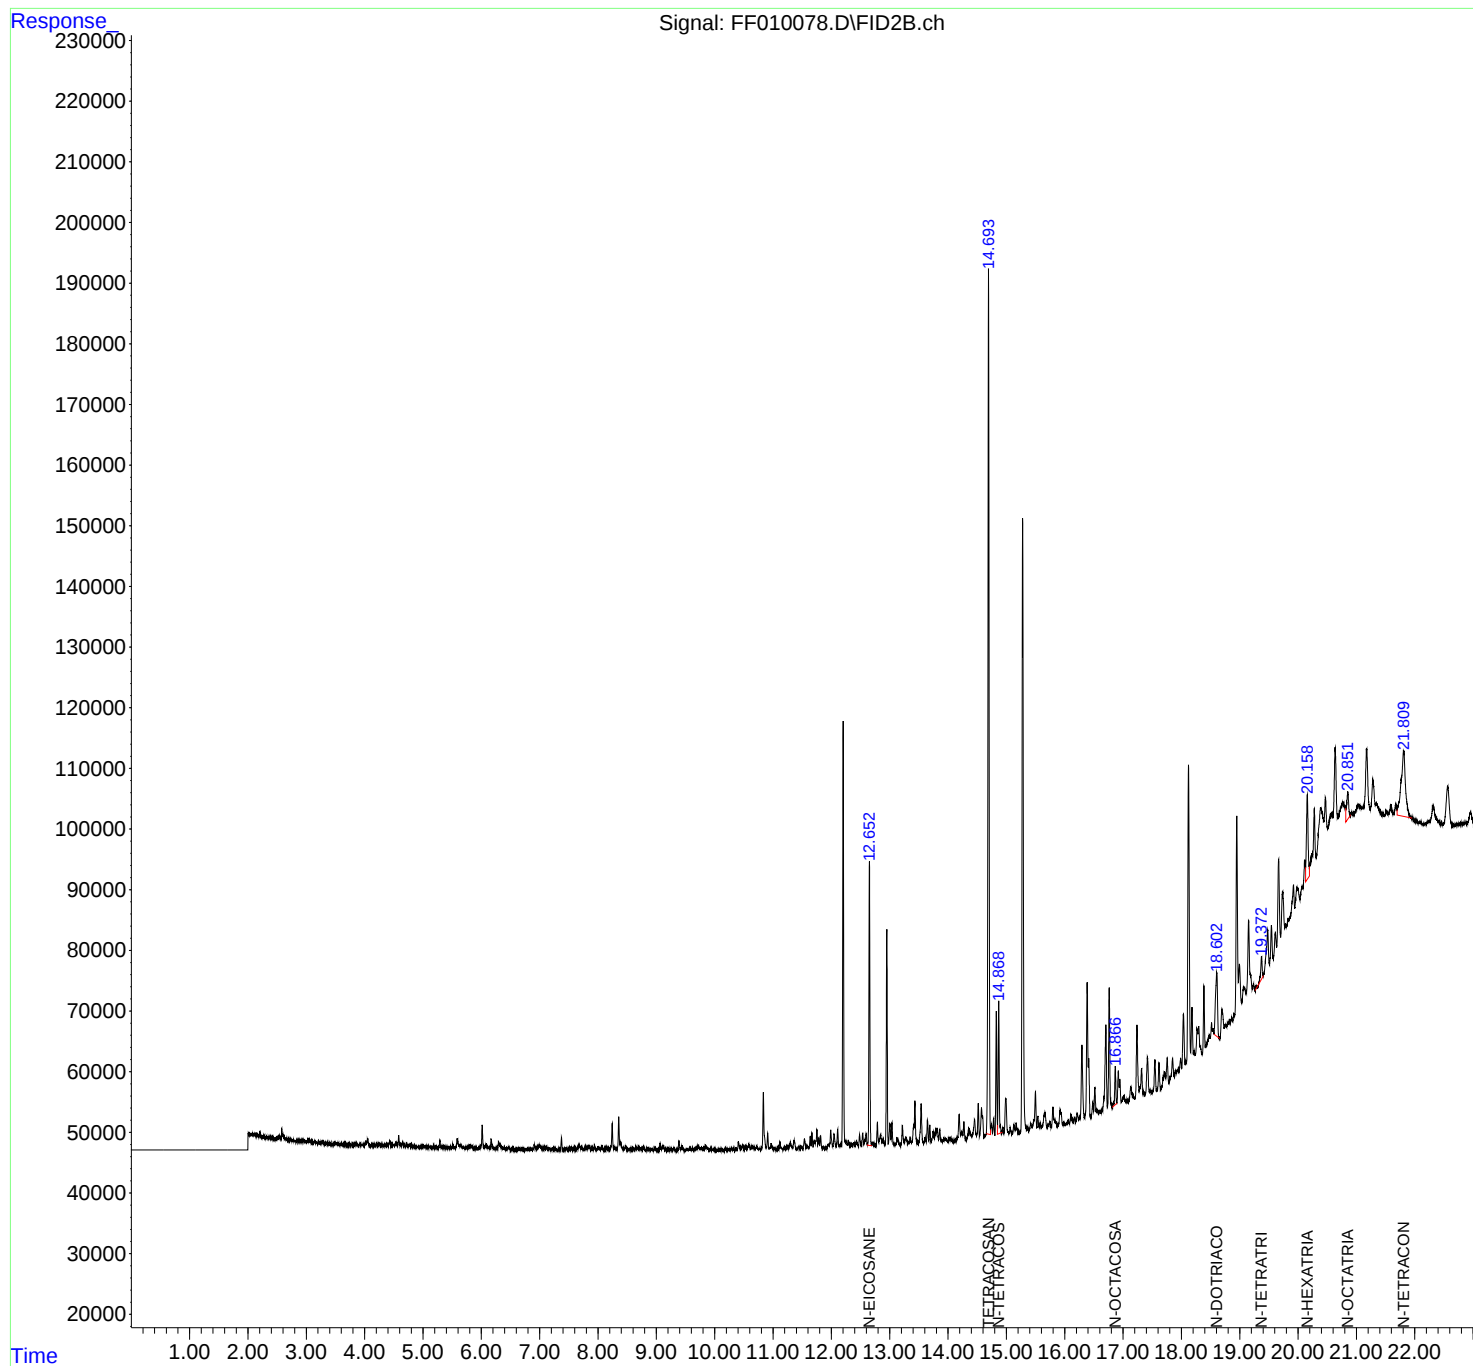


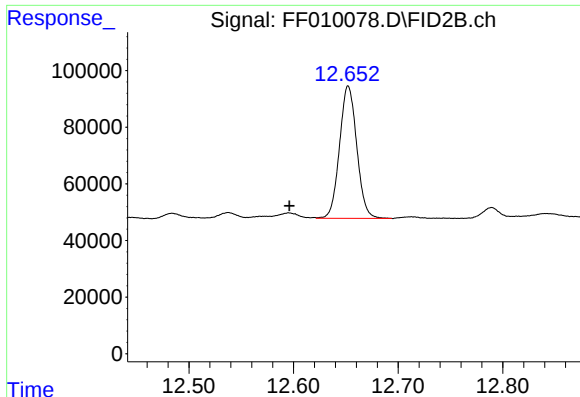

#7 N-EICOSANE


R.T.: 12.652 min
Delta R.T.: 0.056 min
Response: 535896
Conc: 3.09 ug/ml

Instrument :
FID_F
ClientSampleId :

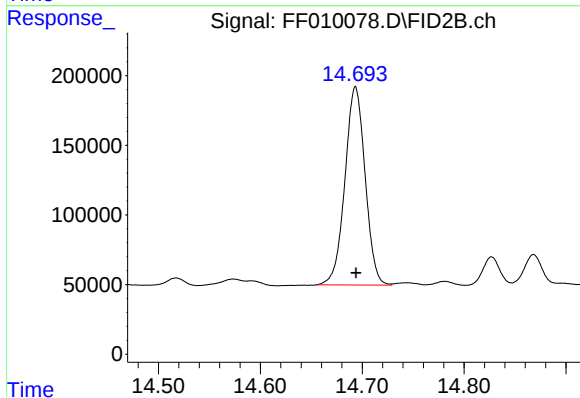


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.693 min
Delta R.T.: 0.000 min
Response: 1961164
Conc: 13.08 ug/ml

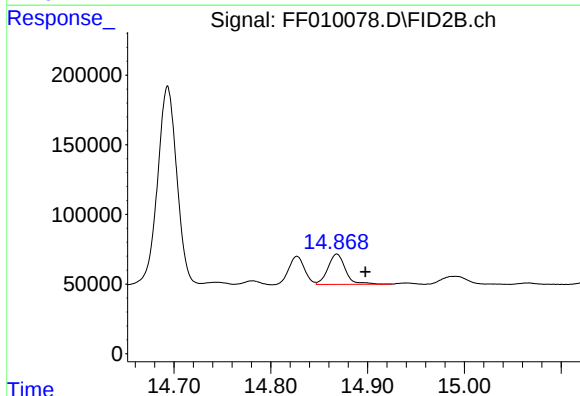


#10 N-TETRACOSANE

R.T.: 14.868 min
Delta R.T.: -0.029 min
Response: 272055
Conc: 1.61 ug/ml

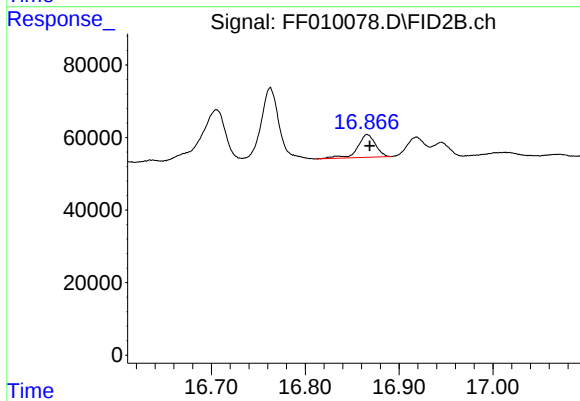

#12 N-OCTACOSANE


R.T.: 16.866 min
Delta R.T.: -0.002 min
Response: 82733
Conc: 0.52 ug/ml

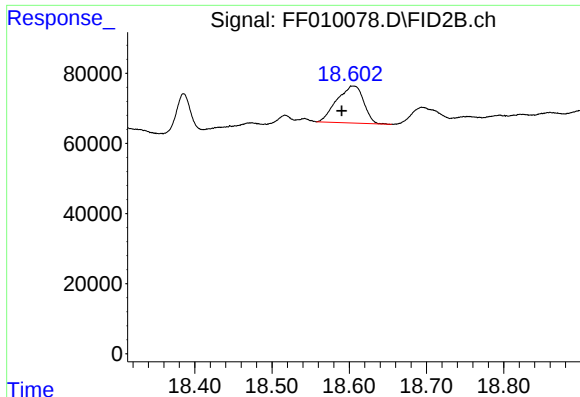

#14 N-DOTRIACONTANE


R.T.: 18.605 min
Delta R.T.: 0.015 min
Response: 253319
Conc: 1.73 ug/ml

Instrument :
FID_F
ClientSampleId :

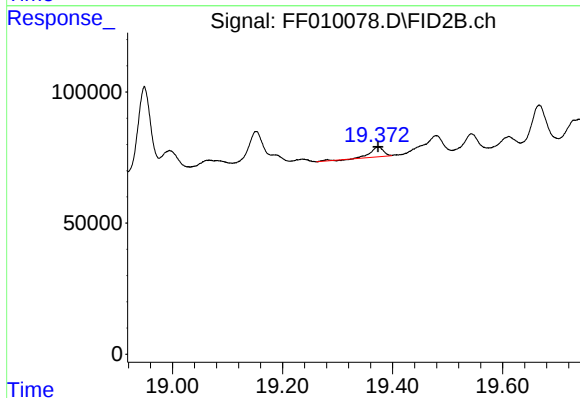


#15 N-TETRATRIACONTANE

R.T.: 19.374 min
Delta R.T.: 0.000 min
Response: 64097
Conc: 0.47 ug/ml

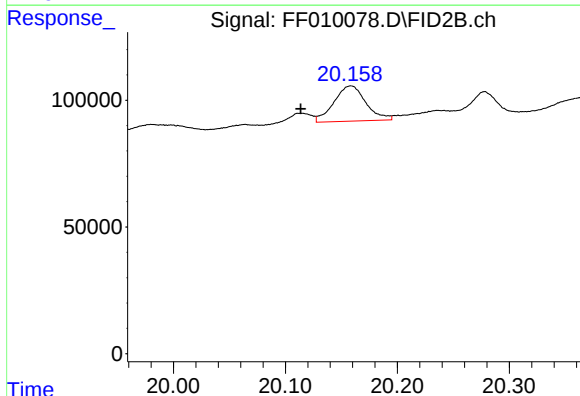


#16 N-HEXATRIACONTANE

R.T.: 20.158 min
Delta R.T.: 0.045 min
Response: 277433
Conc: 2.23 ug/ml

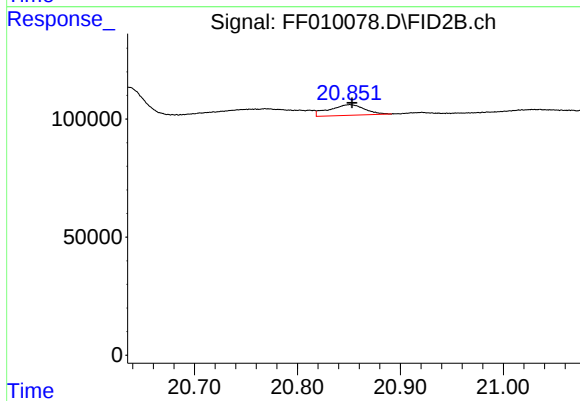

#17 N-OCTATRIACONTANE

R.T.: 20.851 min
Delta R.T.: -0.002 min
Response: 107402
Conc: 0.96 ug/ml

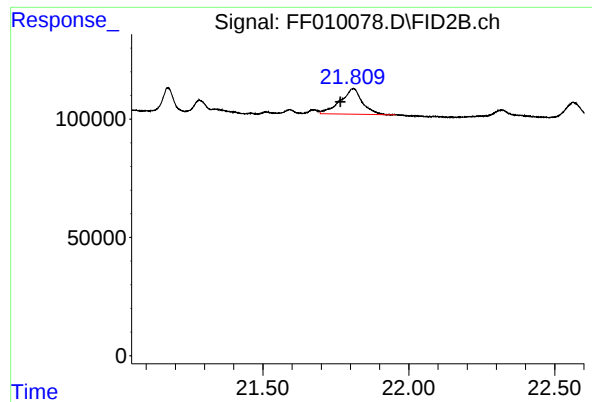

#18 N-TETRACONTANE

R.T.: 21.810 min
Delta R.T.: 0.044 min
Response: 565971
Conc: 5.52 ug/ml

Instrument :
FID_F
ClientSampleId :