

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
 Data File : FF010085.D
 Signal(s) : FID2B.ch
 Acq On : 18 Mar 2022 21:06
 Operator : AJ\MA
 Sample : N1995-02
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 18 23:32:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
 Quant Title :
 QLast Update : Thu Mar 10 12:46:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.693	3003183	20.025 ug/ml
Target Compounds			
3) N-DODECANE	6.413	219334	1.276 ug/ml
4) N-TETRADECANE	8.246	2471983	14.237 ug/ml
6) N-OCTADECANE	11.300	176367	0.986 ug/ml
7) N-EICOSANE	12.651f	508567	2.929 ug/ml
10) N-TETRACOSANE	14.867	224566	1.330 ug/ml
14) N-DOTRIACONTANE	18.584	269270	1.844 ug/ml
15) N-TETRATRIACONTANE	19.437f	111946	0.817 ug/ml
16) N-HEXATRIACONTANE	20.156	123338	0.992 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
Data File : FF010085.D
Signal(s) : FID2B.ch
Acq On : 18 Mar 2022 21:06
Operator : AJ\MA
Sample : N1995-02
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 18 23:32:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

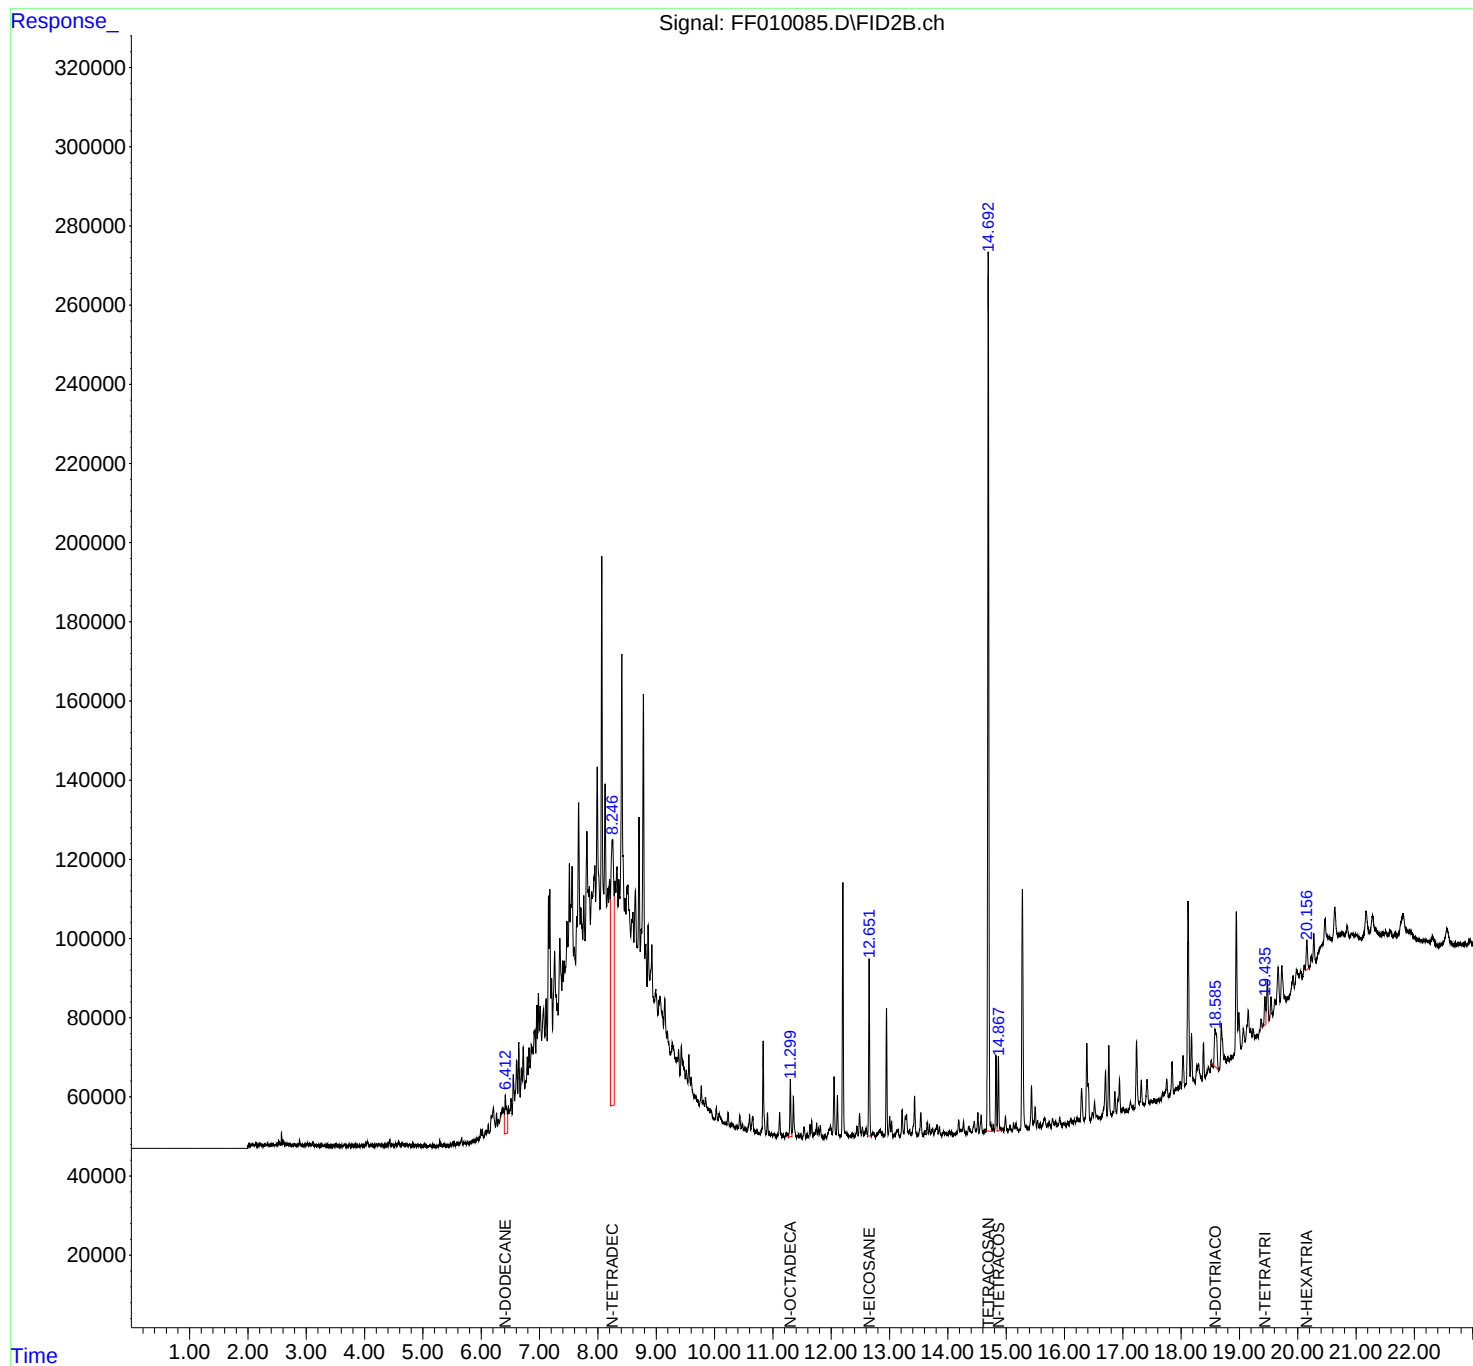


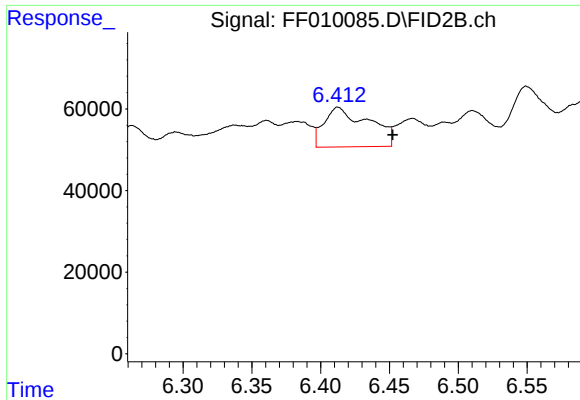

#3 N-DODECANE


R.T.: 6.413 min
Delta R.T.: -0.040 min
Response: 219334
Conc: 1.28 ug/ml

Instrument :
FID_F
ClientSampleId :

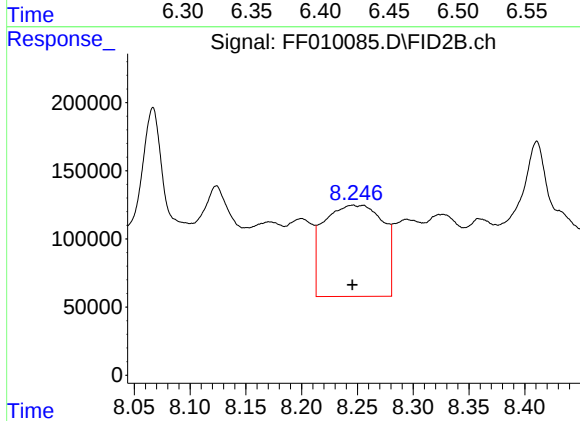


#4 N-TETRADECANE

R.T.: 8.246 min
Delta R.T.: 0.000 min
Response: 2471983
Conc: 14.24 ug/ml

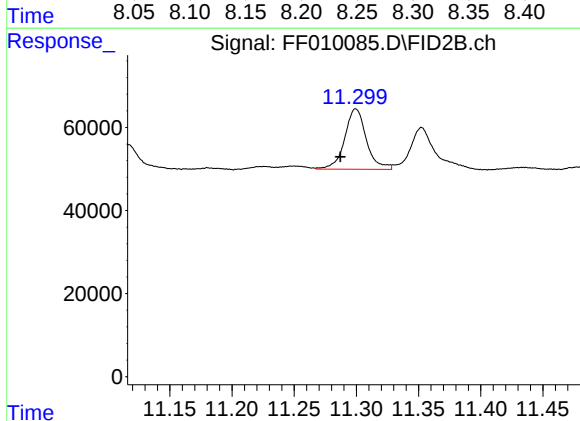


#6 N-OCTADECANE

R.T.: 11.300 min
Delta R.T.: 0.012 min
Response: 176367
Conc: 0.99 ug/ml

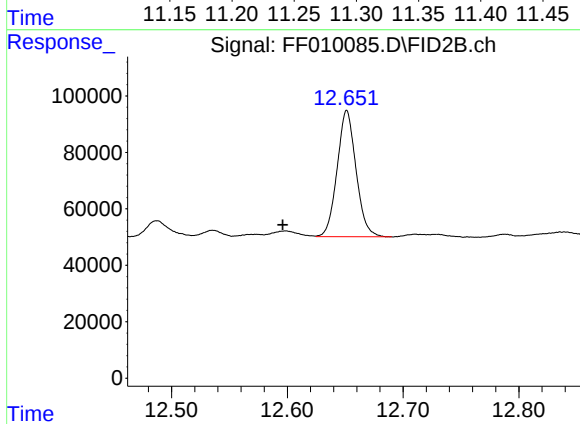

#7 N-EICOSANE


R.T.: 12.651 min
Delta R.T.: 0.055 min
Response: 508567
Conc: 2.93 ug/ml

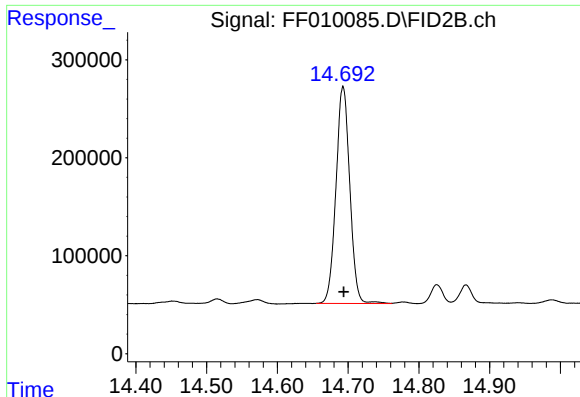

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.693 min
Delta R.T.: -0.001 min
Response: 3003183
Conc: 20.03 ug/ml

Instrument :
FID_F
ClientSampleId :

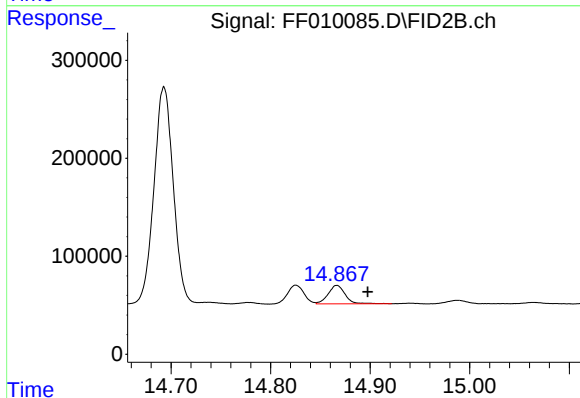


#10 N-TETRACOSANE

R.T.: 14.867 min
Delta R.T.: -0.031 min
Response: 224566
Conc: 1.33 ug/ml

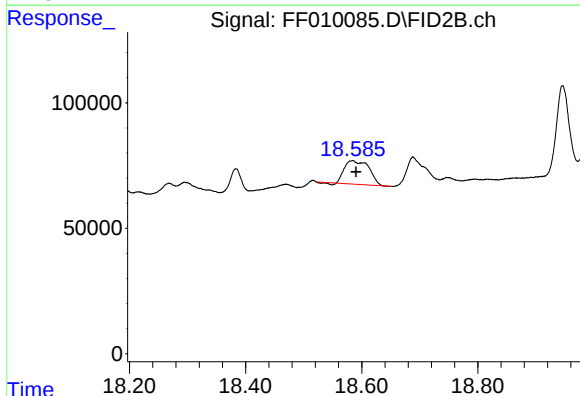


#14 N-DOTRIACONTANE

R.T.: 18.584 min
Delta R.T.: -0.007 min
Response: 269270
Conc: 1.84 ug/ml

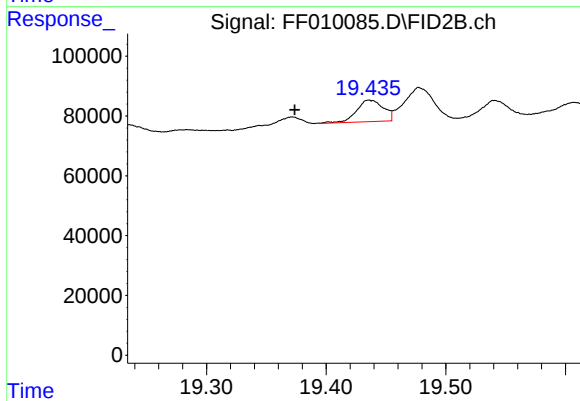

#15 N-TETRATRIACONTANE

R.T.: 19.437 min
Delta R.T.: 0.063 min
Response: 111946
Conc: 0.82 ug/ml

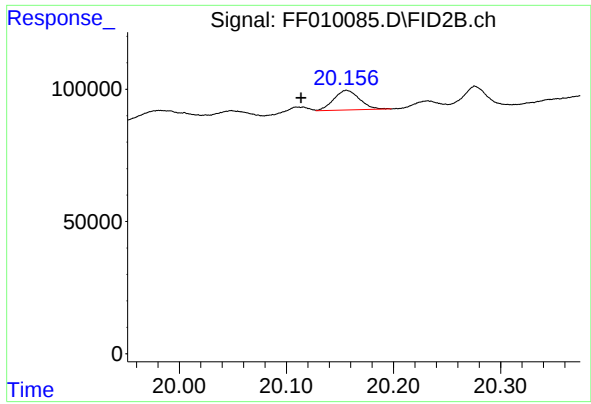

#16 N-HEXATRIACONTANE

R.T.: 20.156 min
Delta R.T.: 0.043 min
Response: 123338
Conc: 0.99 ug/ml

Instrument :
FID_F
ClientSampleId :