

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
 Data File : FF010086.D
 Signal(s) : FID2B.ch
 Acq On : 18 Mar 2022 21:36
 Operator : AJ\MA
 Sample : N1995-05
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 18 23:32:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
 Quant Title :
 QLast Update : Thu Mar 10 12:46:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.693	2039143	13.597 ug/ml
Target Compounds			
4) N-TETRADECANE	8.242	116821	0.673 ug/ml
7) N-EICOSANE	12.653f	1655005	9.531 ug/ml
8) N-DOCOSANE	13.816	310928	1.819 ug/ml
10) N-TETRACOSANE	14.869	1019894	6.039 ug/ml
12) N-OCTACOSANE	16.866	275856	1.724 ug/ml
13) N-TRIACONTANE	17.754	170785	1.112 ug/ml
14) N-DOTRIACONTANE	18.581	19626	0.134 ug/ml
15) N-TETRATRIACONTANE	19.438f	134921	0.985 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
Data File : FF010086.D
Signal(s) : FID2B.ch
Acq On : 18 Mar 2022 21:36
Operator : AJ\MA
Sample : N1995-05
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 18 23:32:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

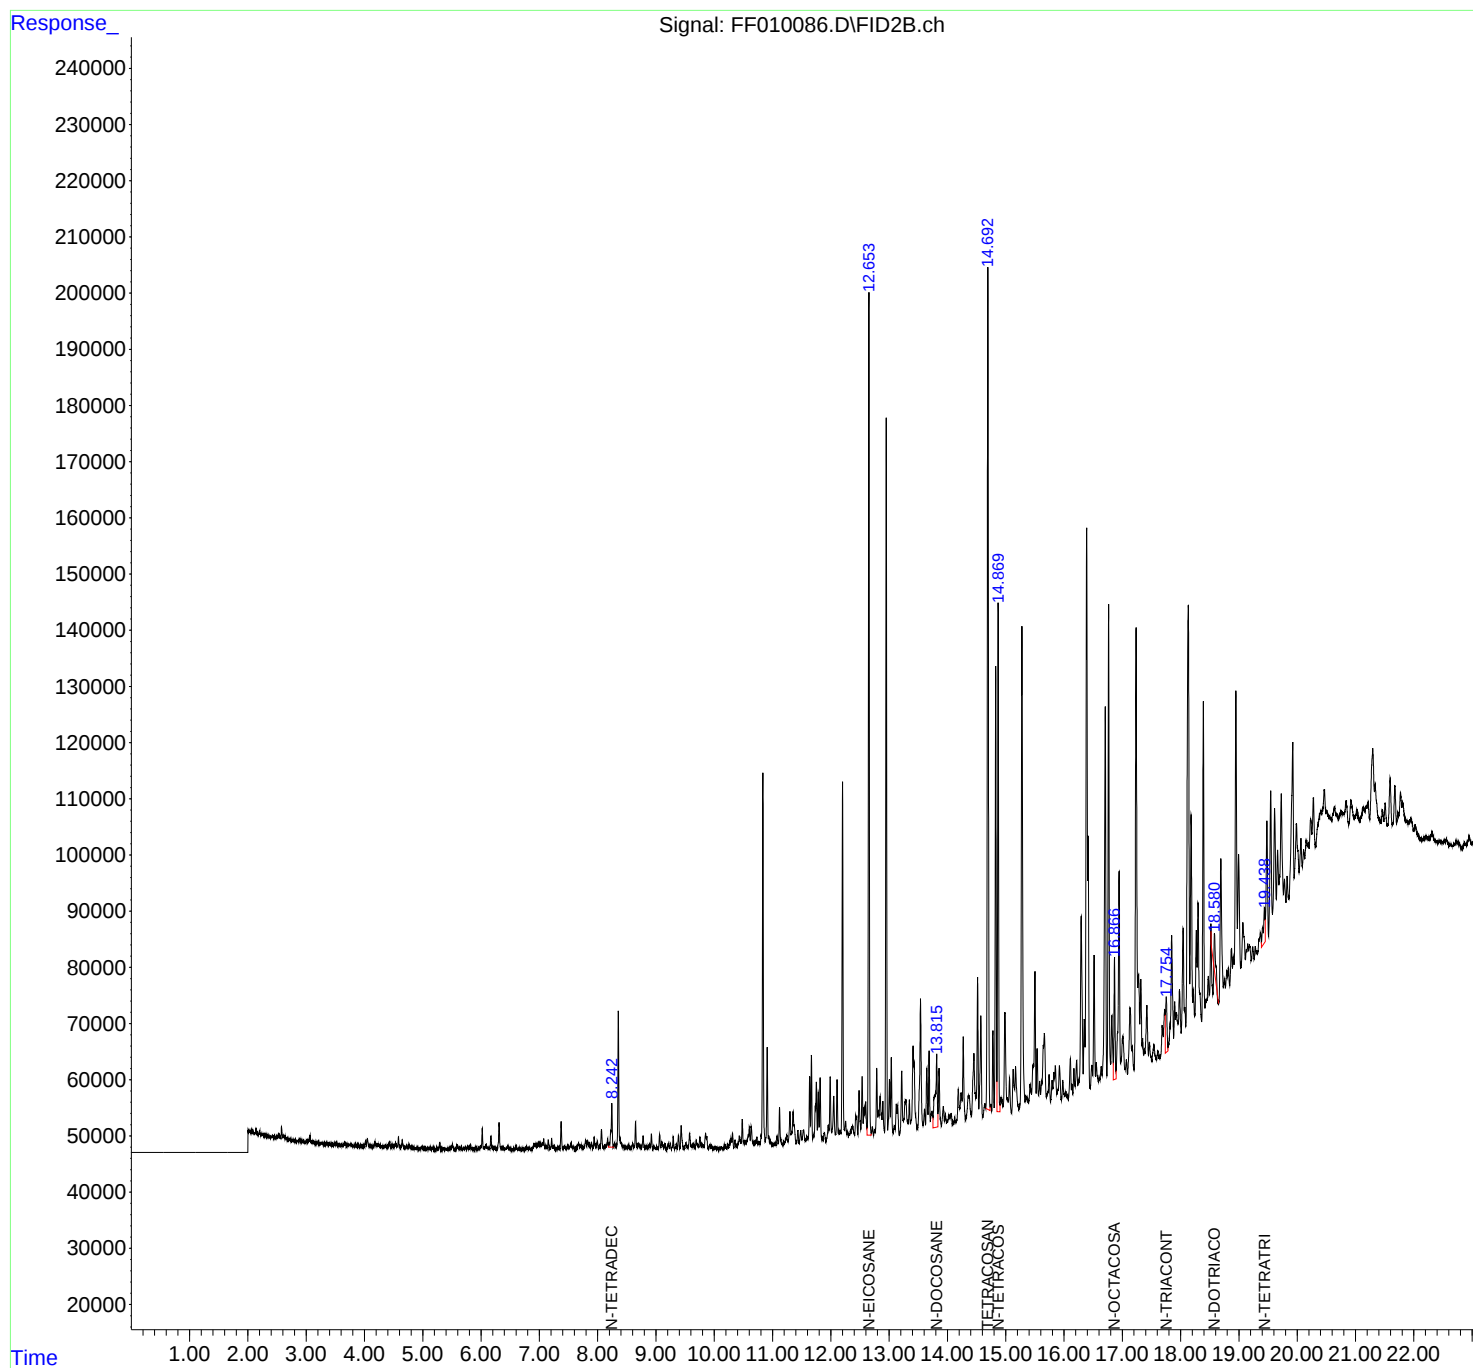


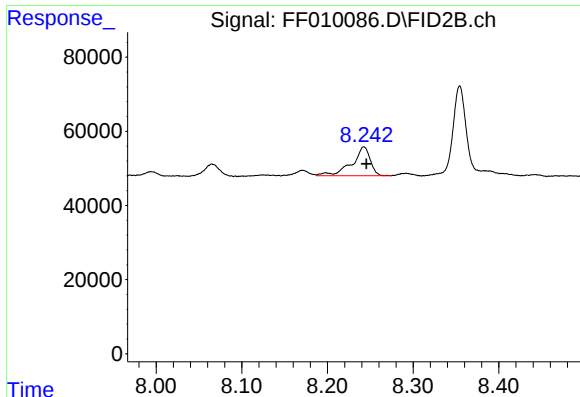

#4 N-TETRADECANE


R.T.: 8.242 min
Delta R.T.: -0.003 min
Response: 116821
Conc: 0.67 ug/ml

Instrument :
FID_F
ClientSampleId :

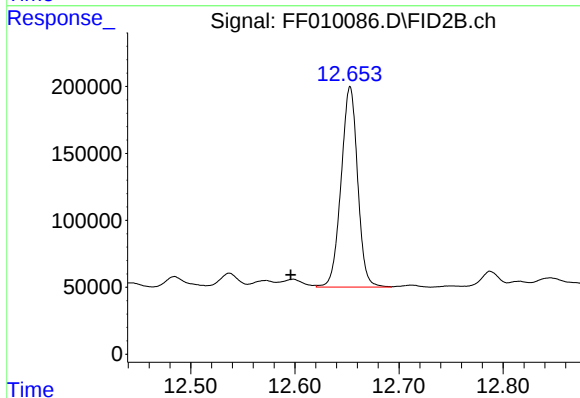


#7 N-EICOSANE

R.T.: 12.653 min
Delta R.T.: 0.057 min
Response: 1655005
Conc: 9.53 ug/ml

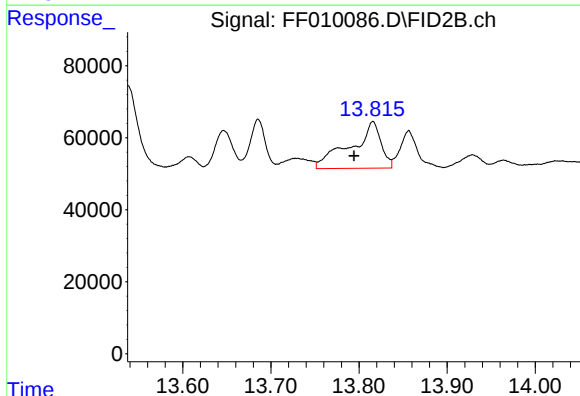


#8 N-DOCOSANE

R.T.: 13.816 min
Delta R.T.: 0.021 min
Response: 310928
Conc: 1.82 ug/ml

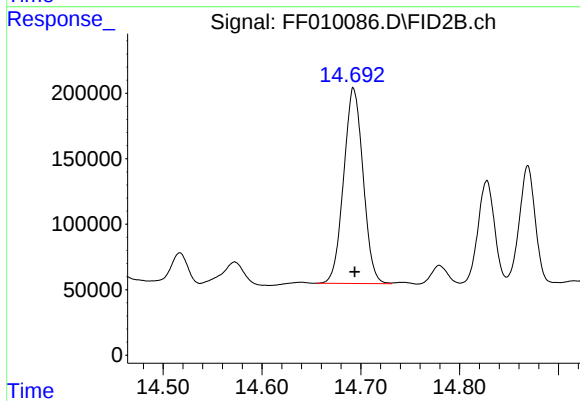

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.693 min
Delta R.T.: -0.001 min
Response: 2039143
Conc: 13.60 ug/ml

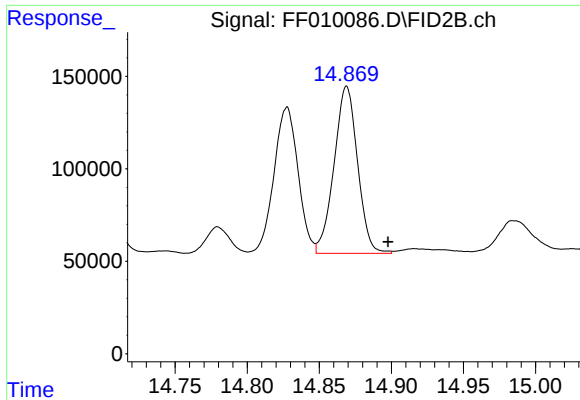

#10 N-TETRACOSANE


R.T.: 14.869 min
Delta R.T.: -0.029 min
Response: 1019894
Conc: 6.04 ug/ml

Instrument :
FID_F
ClientSampleId :

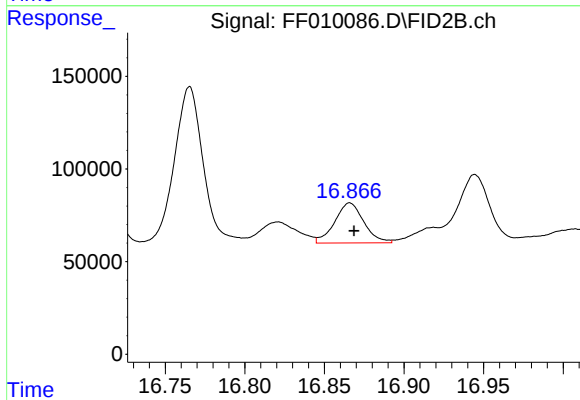


#12 N-OCTACOSANE

R.T.: 16.866 min
Delta R.T.: -0.003 min
Response: 275856
Conc: 1.72 ug/ml

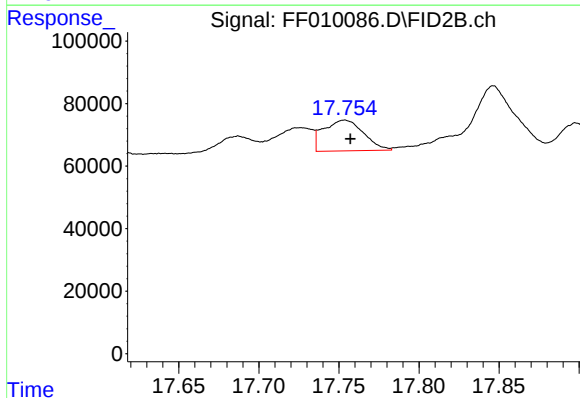


#13 N-TRIACONTANE

R.T.: 17.754 min
Delta R.T.: -0.004 min
Response: 170785
Conc: 1.11 ug/ml

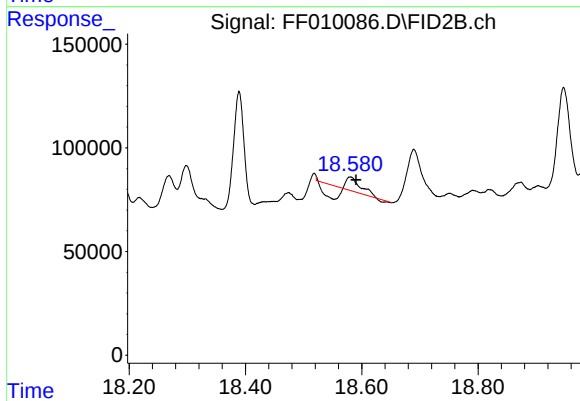

#14 N-DOTRIACONTANE

R.T.: 18.581 min
Delta R.T.: -0.010 min
Response: 19626
Conc: 0.13 ug/ml

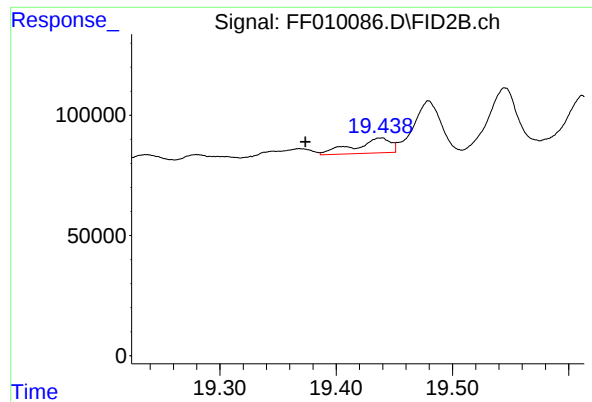

#15 N-TETRATRIACONTANE

R.T.: 19.438 min
Delta R.T.: 0.064 min
Response: 134921
Conc: 0.99 ug/ml

Instrument :

FID_F

ClientSampleId :